

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090722\
 Data File : FB028173.D
 Signal(s) : FID2B.CH
 Acq On : 8 Sep 2022 6:37
 Operator : AJ/MA
 Sample : N4500-02MS 50X
 Misc : 5.06G/5.00 ML MEOH
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-24-COMPMS

Integration File: Calibration.e
 Quant Time: Sep 08 09:18:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	236416	20.399 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	370884	20.501 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	452737	23.087 ng/ml
3) t n-Heptane	7.752	130919	6.796 ng/ml
4) t Benzene	7.890	190839	8.208 ng/ml
6) t Toluene	10.623	540977	24.671 ng/ml
7) t Ethylbenzene	13.060	172883	8.390 ng/ml
8) t m-Xylene	13.193	337522	16.495 ng/ml
9) t O-Xylene	13.920	327757	16.546 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	314965	16.151 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090722\
Data File : FB028173.D
Signal(s) : FID2B.CH
Acq On : 8 Sep 2022 6:37
Operator : AJ/MA
Sample : N4500-02MS 50X
Misc : 5.06G/5.00 ML MEOH
ALS Vial : 35 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-24-COMPMS

Integration File: Calibration.e
Quant Time: Sep 08 09:18:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

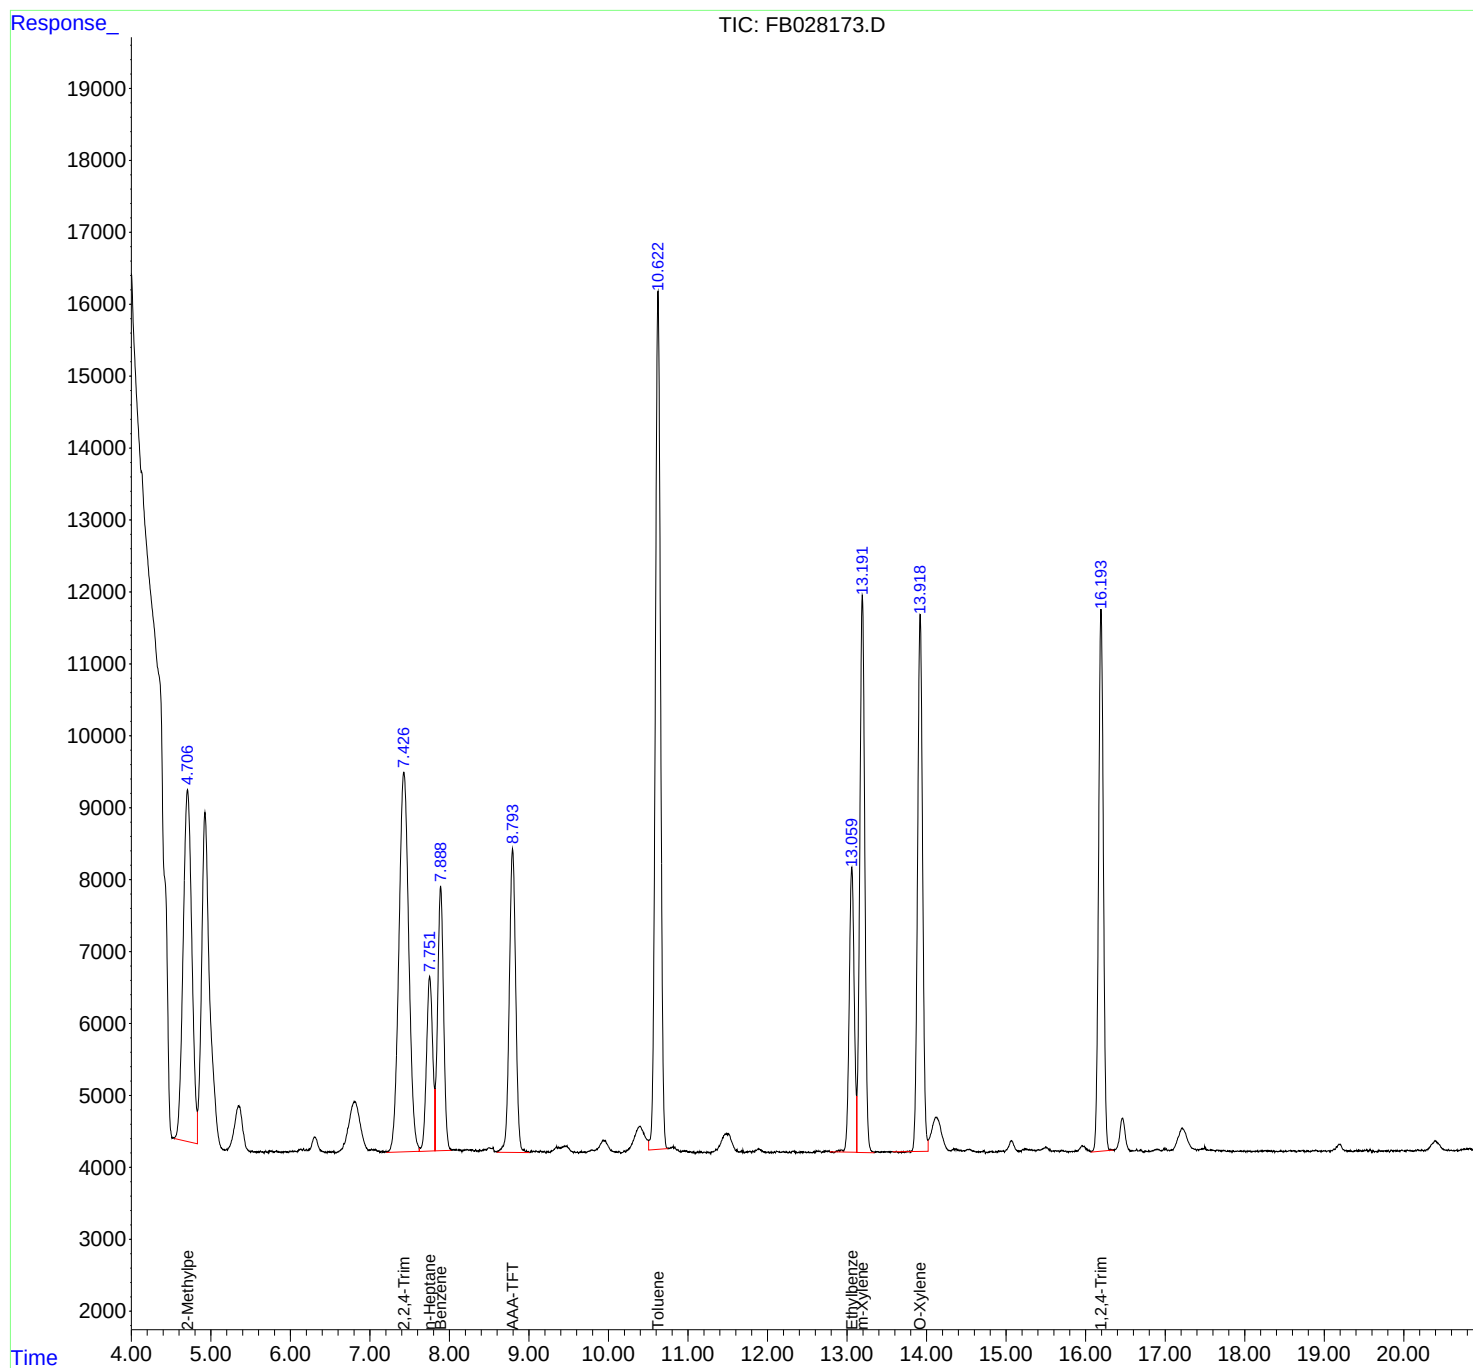


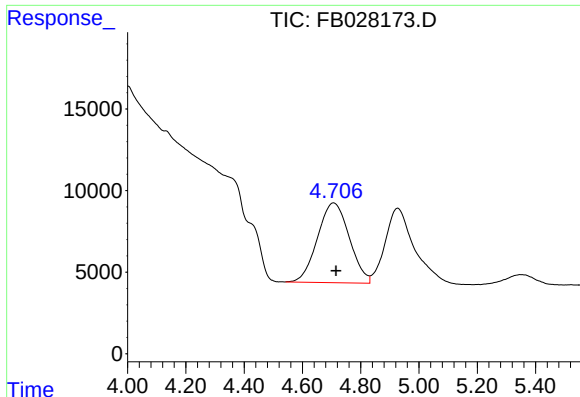

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.008 min
Response: 370884
Conc: 20.50 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-24-COMPMS

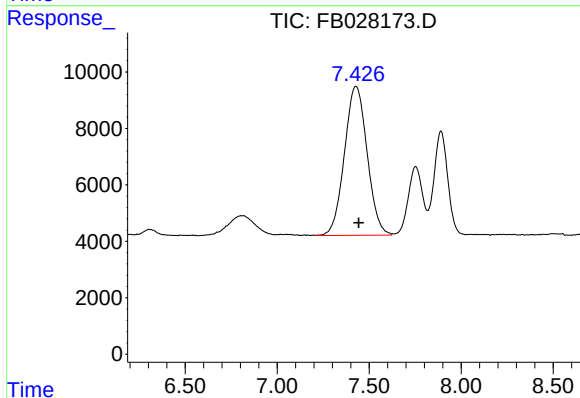


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: -0.015 min
Response: 452737
Conc: 23.09 ng/ml

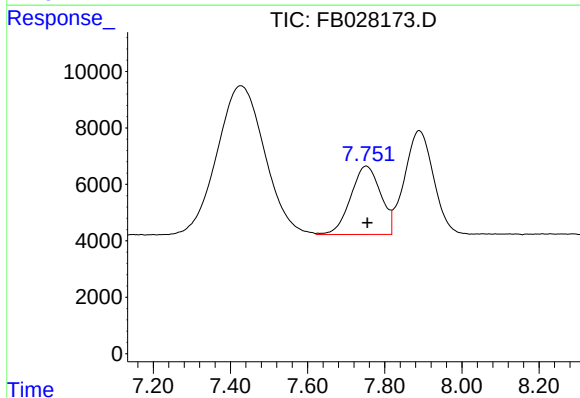


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.003 min
Response: 130919
Conc: 6.80 ng/ml

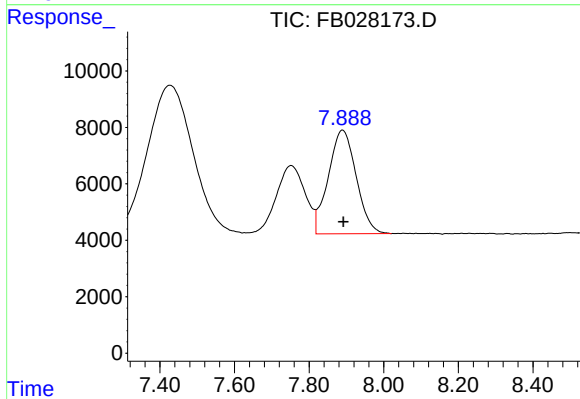

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 190839
Conc: 8.21 ng/ml

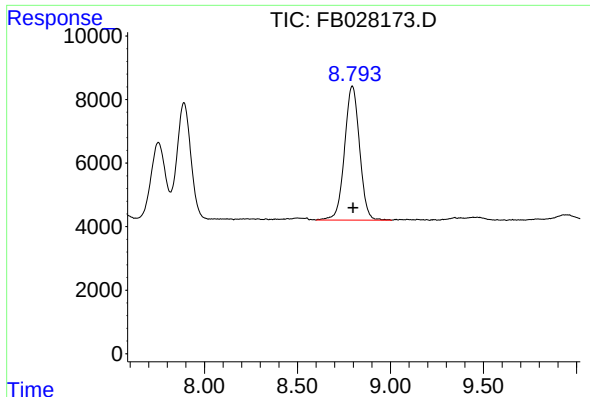

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 236416
Conc: 20.40 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-24-COMPMS

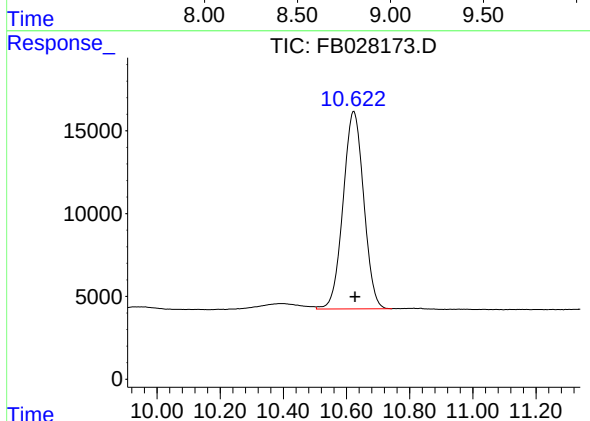


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.004 min
Response: 540977
Conc: 24.67 ng/ml

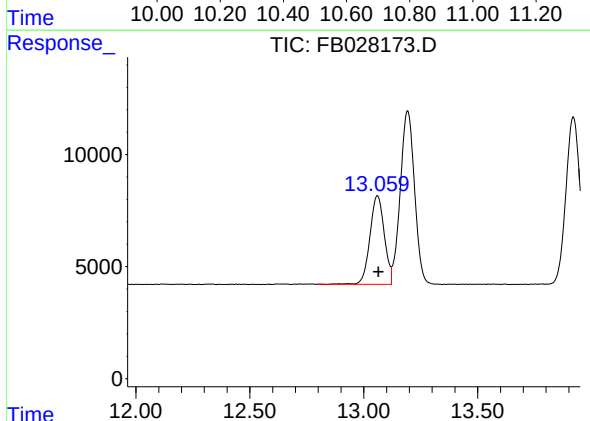


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: -0.004 min
Response: 172883
Conc: 8.39 ng/ml

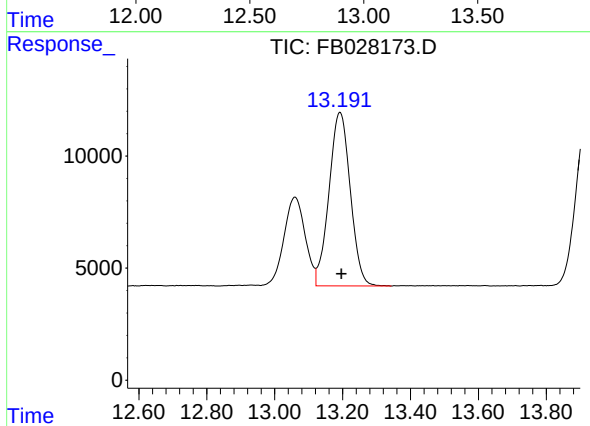

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: -0.004 min
Response: 337522
Conc: 16.49 ng/ml

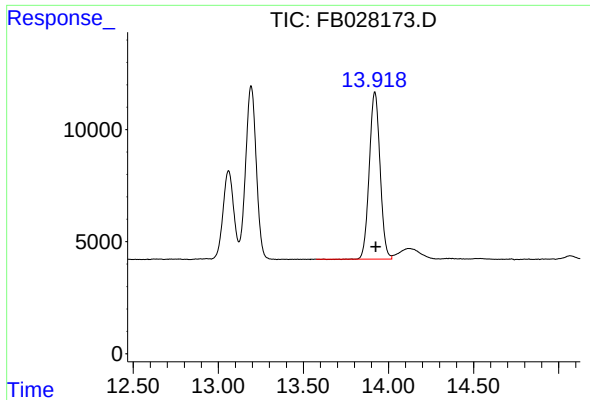

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: -0.004 min
Response: 327757
Conc: 16.55 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-24-COMPMS

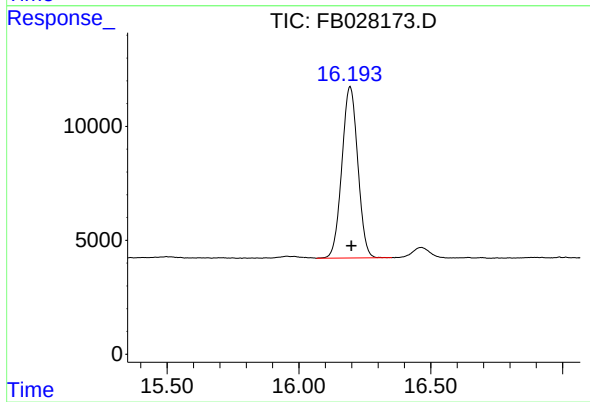

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: -0.005 min
Response: 314965
Conc: 16.15 ng/ml