

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090722\
 Data File : FB028174.D
 Signal(s) : FID2B.CH
 Acq On : 8 Sep 2022 7:14
 Operator : AJ/MA
 Sample : N4500-02MSD 50X
 Misc : 5.03G/5.00 ML MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-24-COMPMSD

Integration File: Calibration.e
 Quant Time: Sep 08 09:18:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	202261	17.452 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	379837	20.996 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	492364	25.108 ng/ml
3) t n-Heptane	7.751	128532	6.672 ng/ml
4) t Benzene	7.889	193081	8.304 ng/ml
6) t Toluene	10.623	542160	24.724 ng/ml
7) t Ethylbenzene	13.059	175130	8.499 ng/ml
8) t m-Xylene	13.192	347759	16.995 ng/ml
9) t O-Xylene	13.919	352575	17.799 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	363080	18.619 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090722\
Data File : FB028174.D
Signal(s) : FID2B.CH
Acq On : 8 Sep 2022 7:14
Operator : AJ/MA
Sample : N4500-02MSD 50X
Misc : 5.03G/5.00 ML MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-24-COMPMSD

Integration File: Calibration.e
Quant Time: Sep 08 09:18:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

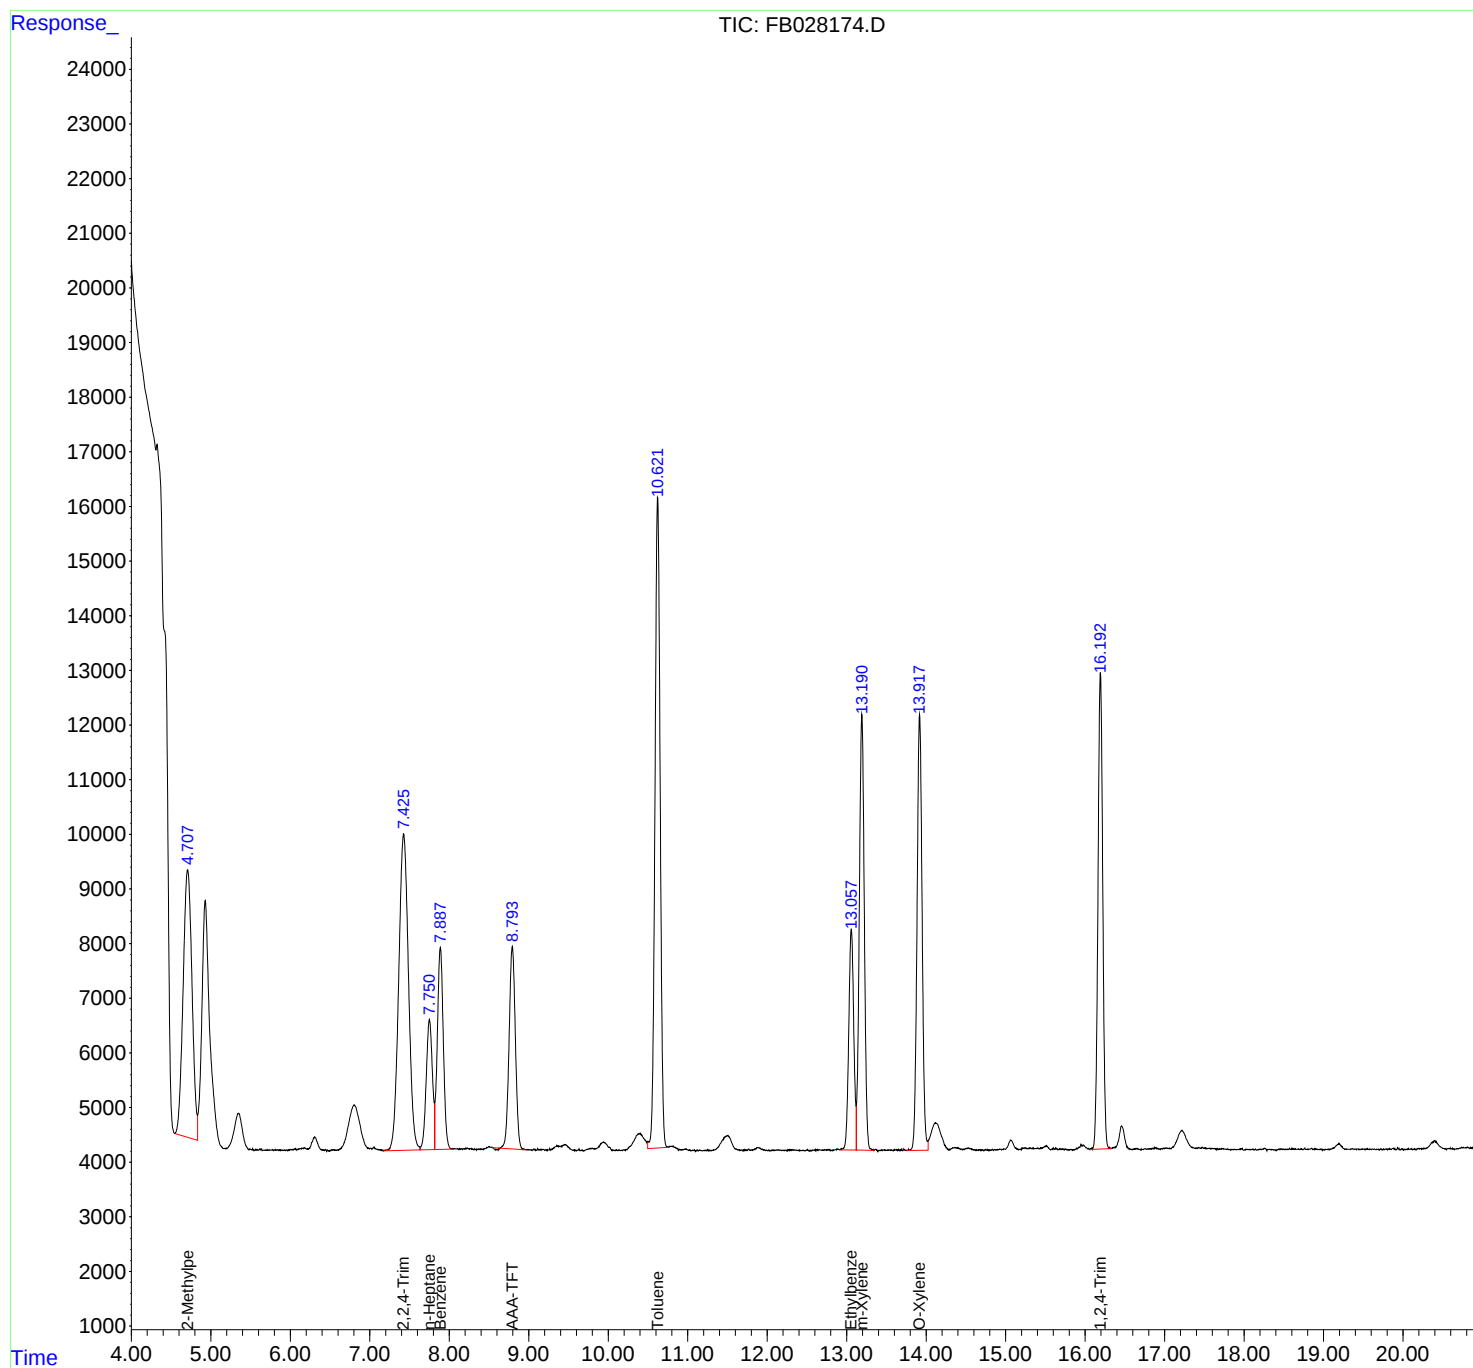


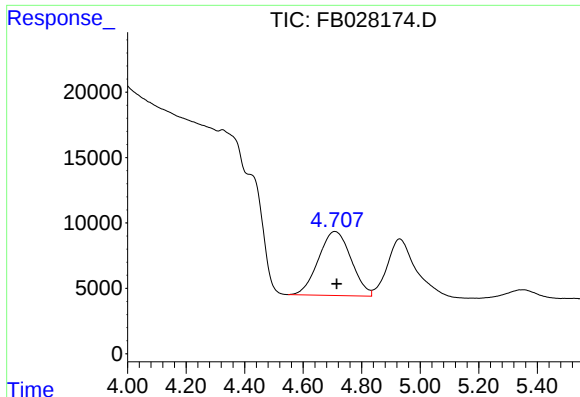

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: -0.006 min
Response: 379837
Conc: 21.00 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-24-COMPMSD

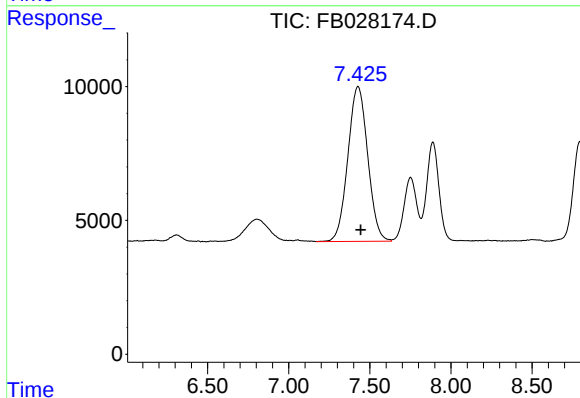


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: -0.016 min
Response: 492364
Conc: 25.11 ng/ml

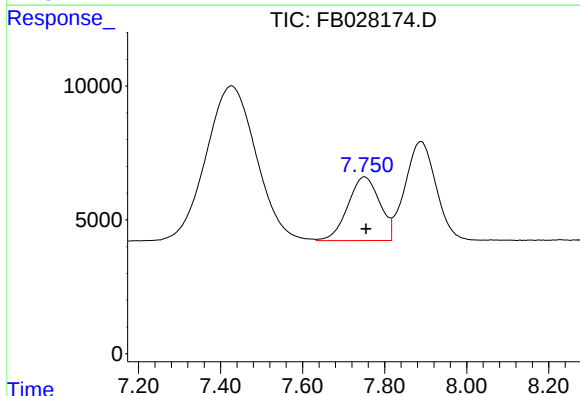


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.004 min
Response: 128532
Conc: 6.67 ng/ml

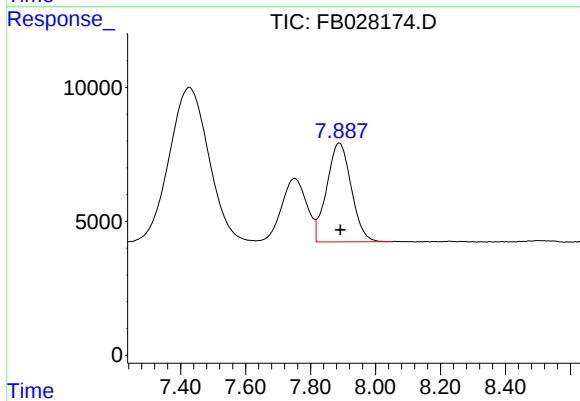

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.003 min
Response: 193081
Conc: 8.30 ng/ml

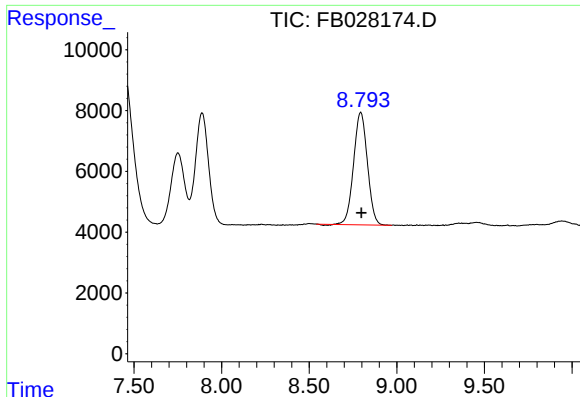

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.004 min
Response: 202261
Conc: 17.45 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-24-COMPMSD

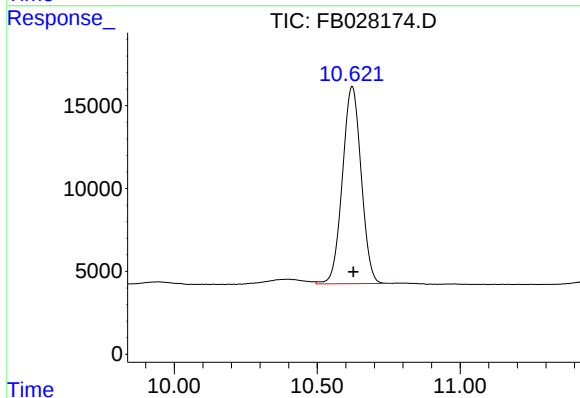


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.004 min
Response: 542160
Conc: 24.72 ng/ml

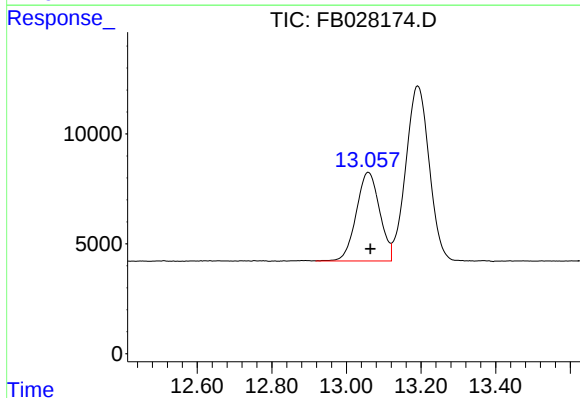


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: -0.005 min
Response: 175130
Conc: 8.50 ng/ml

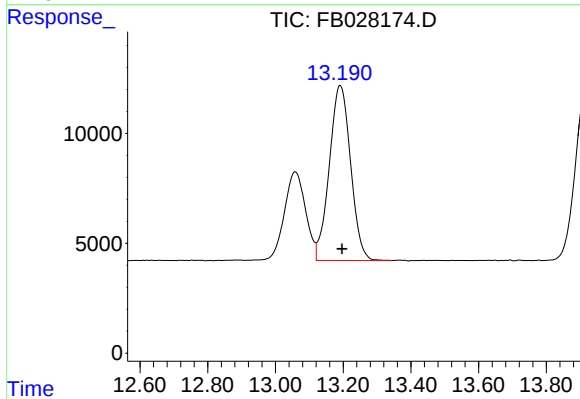

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: -0.005 min
Response: 347759
Conc: 16.99 ng/ml

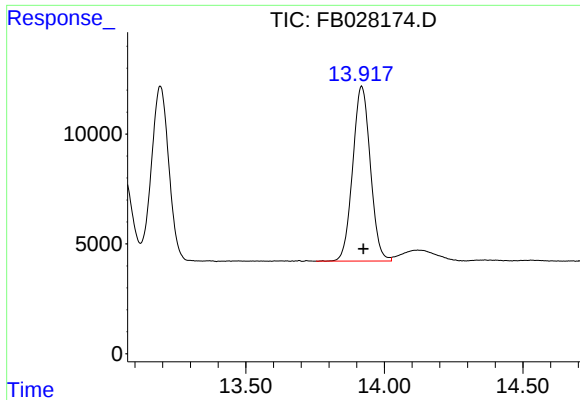

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.006 min
Response: 352575
Conc: 17.80 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-24-COMPMSD

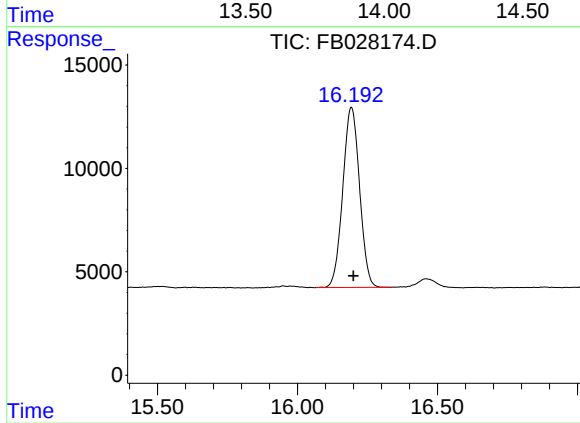

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: -0.006 min
Response: 363080
Conc: 18.62 ng/ml