

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090820\
Data File : FB024842.D
Signal(s) : FID2B.CH
Acq On : 8 Sep 2020 14:46
Operator : DD/AJ
Sample : L3808-09
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 09 00:40:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
Quant Title :
QLast Update : Mon Aug 10 12:11:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.799	501588	24.291 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.687	288	0.012 ng/ml
4) t	Benzene	7.893	1125	0.032 ng/ml
6) t	Toluene	10.629	2053	0.060 ng/ml
7) t	Ethylbenzene	13.062	2824	0.088 ng/ml
8) t	m-Xylene	13.202	1217	0.039 ng/ml
9) t	O-Xylene	13.907	721	0.024 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090820\
Data File : FB024842.D
Signal(s) : FID2B.CH
Acq On : 8 Sep 2020 14:46
Operator : DD/AJ
Sample : L3808-09
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 09 00:40:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
Quant Title :
QLast Update : Mon Aug 10 12:11:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

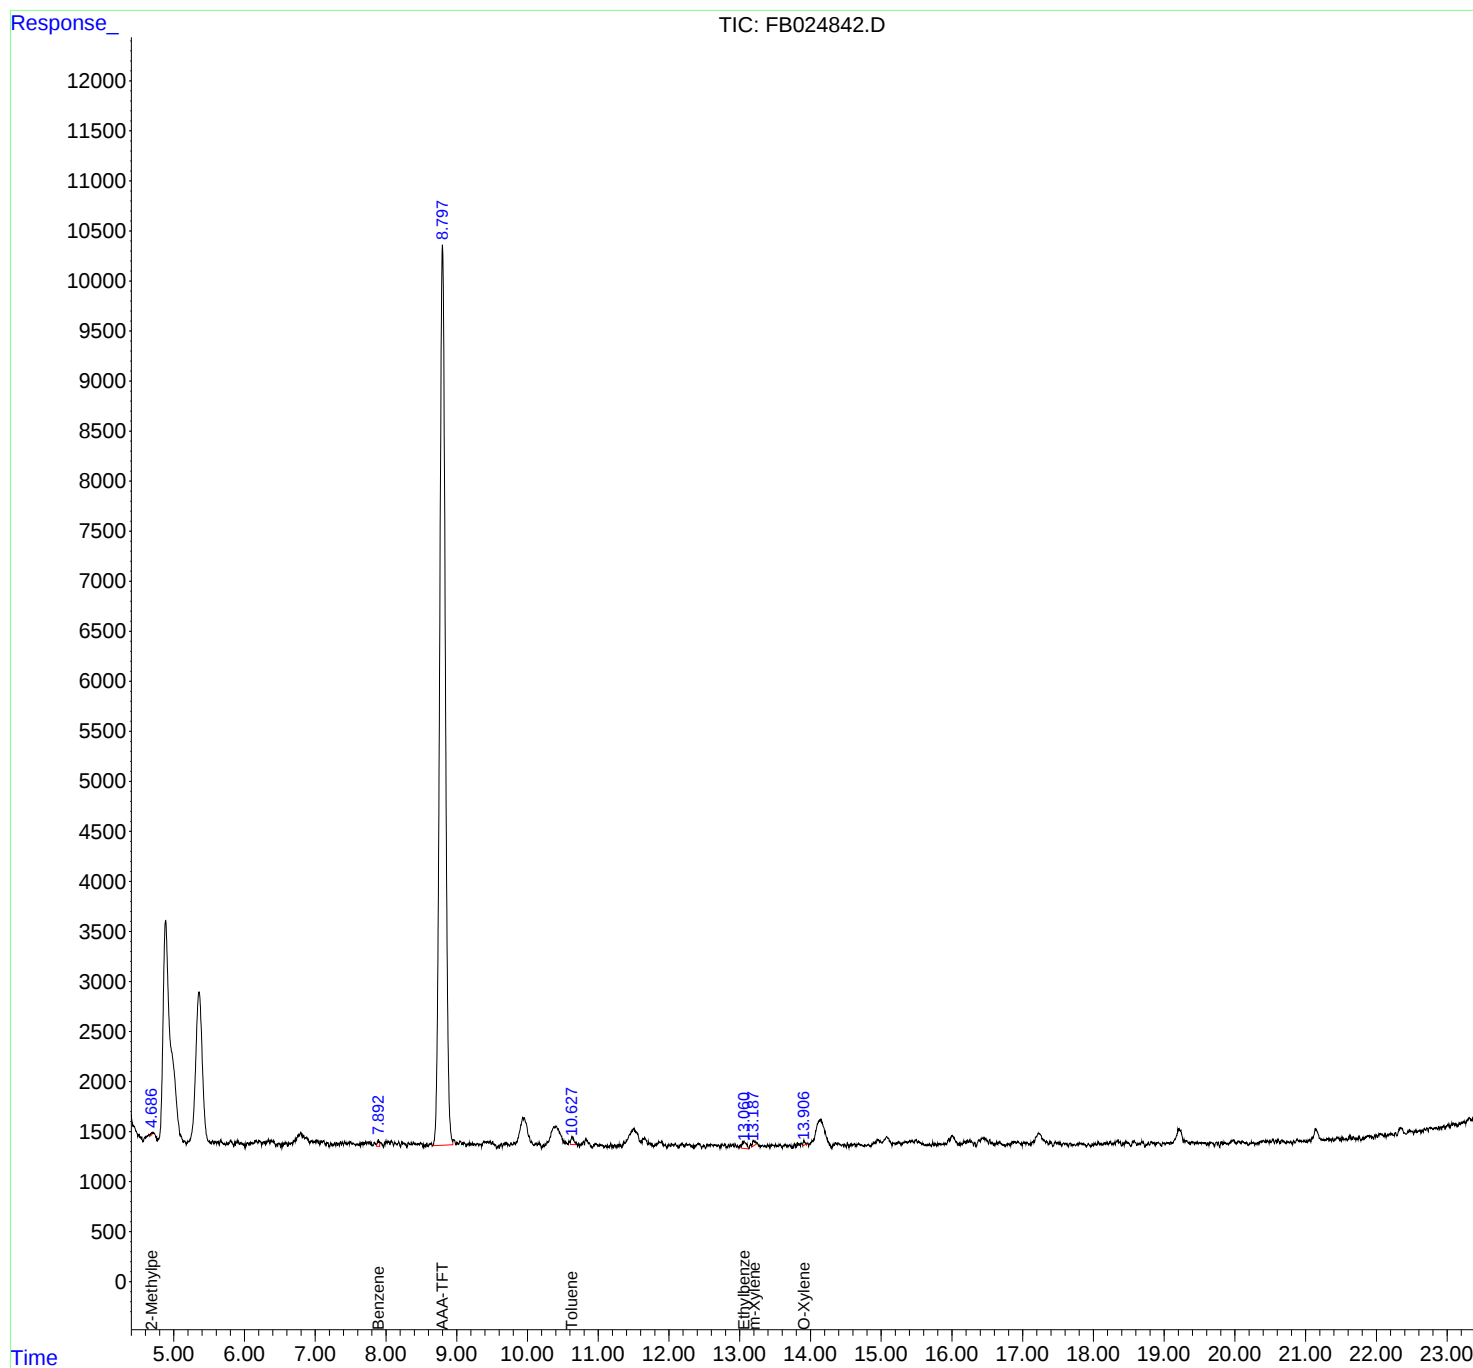

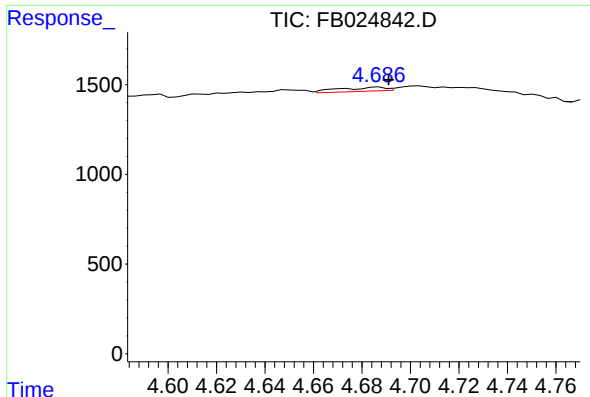


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.004 min
Response: 288
Conc: 0.01 ng/ml

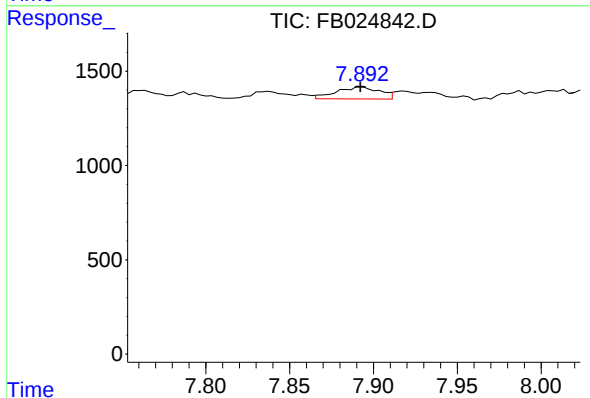


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.001 min
Response: 1125
Conc: 0.03 ng/ml

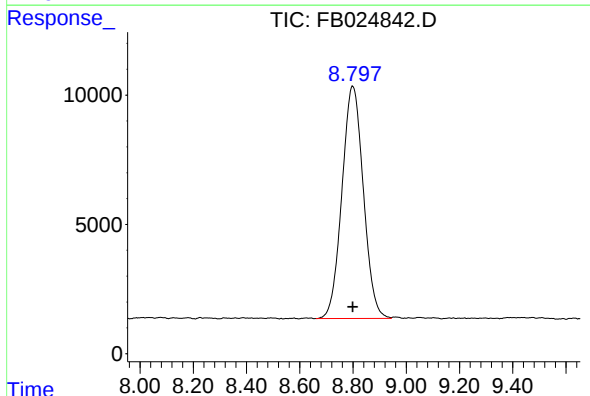


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 501588
Conc: 24.29 ng/ml

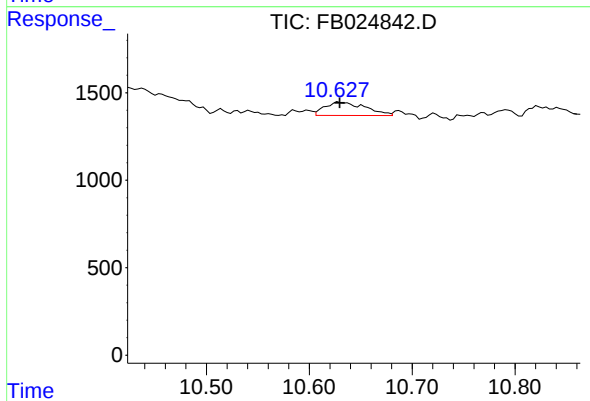


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 2053
Conc: 0.06 ng/ml

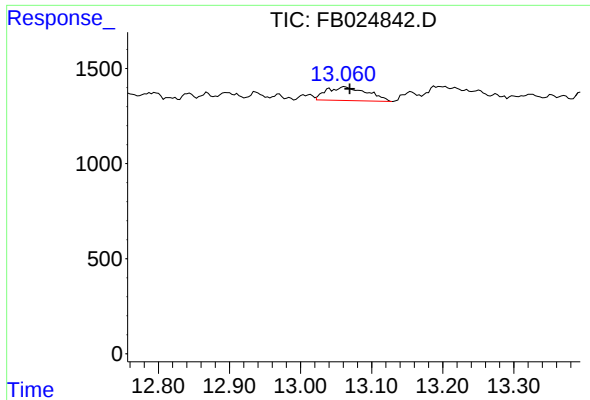


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.007 min
Response: 2824
Conc: 0.09 ng/ml

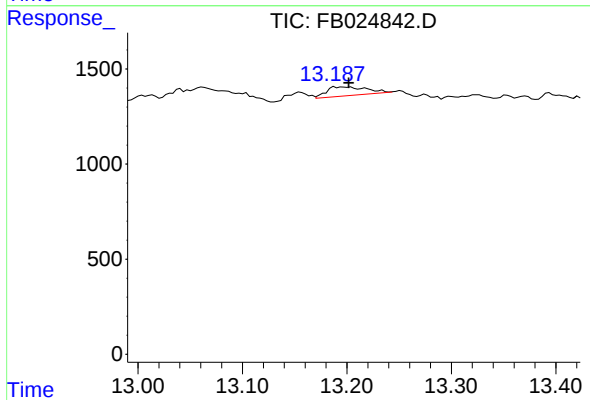

#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 1217
Conc: 0.04 ng/ml

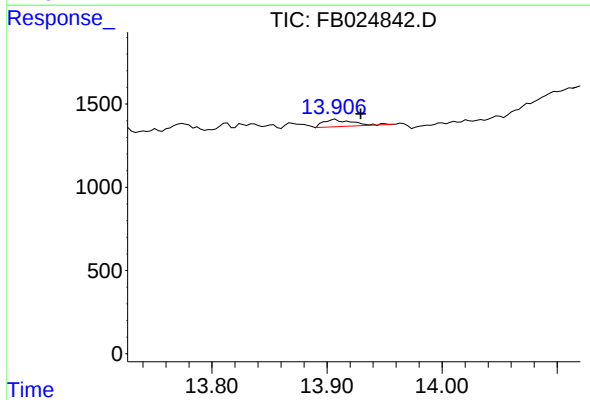

#9 o-Xylene

R.T.: 13.907 min
Delta R.T.: -0.022 min
Response: 721
Conc: 0.02 ng/ml