

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090822\
 Data File : FB028191.D
 Signal(s) : FID2B.CH
 Acq On : 8 Sep 2022 19:05
 Operator : AJ/MA
 Sample : BSF0908S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0908S1

Integration File: Calibration.e
 Quant Time: Sep 09 07:11:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	224749	18.778 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.722	544369	26.886 ng/ml
2) t 2,2,4-Trimethylpentane	7.440	577667	27.461 ng/ml
3) t n-Heptane	7.761	185618	8.635 ng/ml
4) t Benzene	7.898	208528	8.476 ng/ml
6) t Toluene	10.630	608736	26.147 ng/ml
7) t Ethylbenzene	13.067	193226	8.689 ng/ml
8) t m-Xylene	13.199	384189	17.605 ng/ml
9) t O-Xylene	13.926	369140	17.618 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	367648	18.284 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090822\
Data File : FB028191.D
Signal(s) : FID2B.CH
Acq On : 8 Sep 2022 19:05
Operator : AJ/MA
Sample : BSF0908S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0908S1

Integration File: Calibration.e
Quant Time: Sep 09 07:11:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

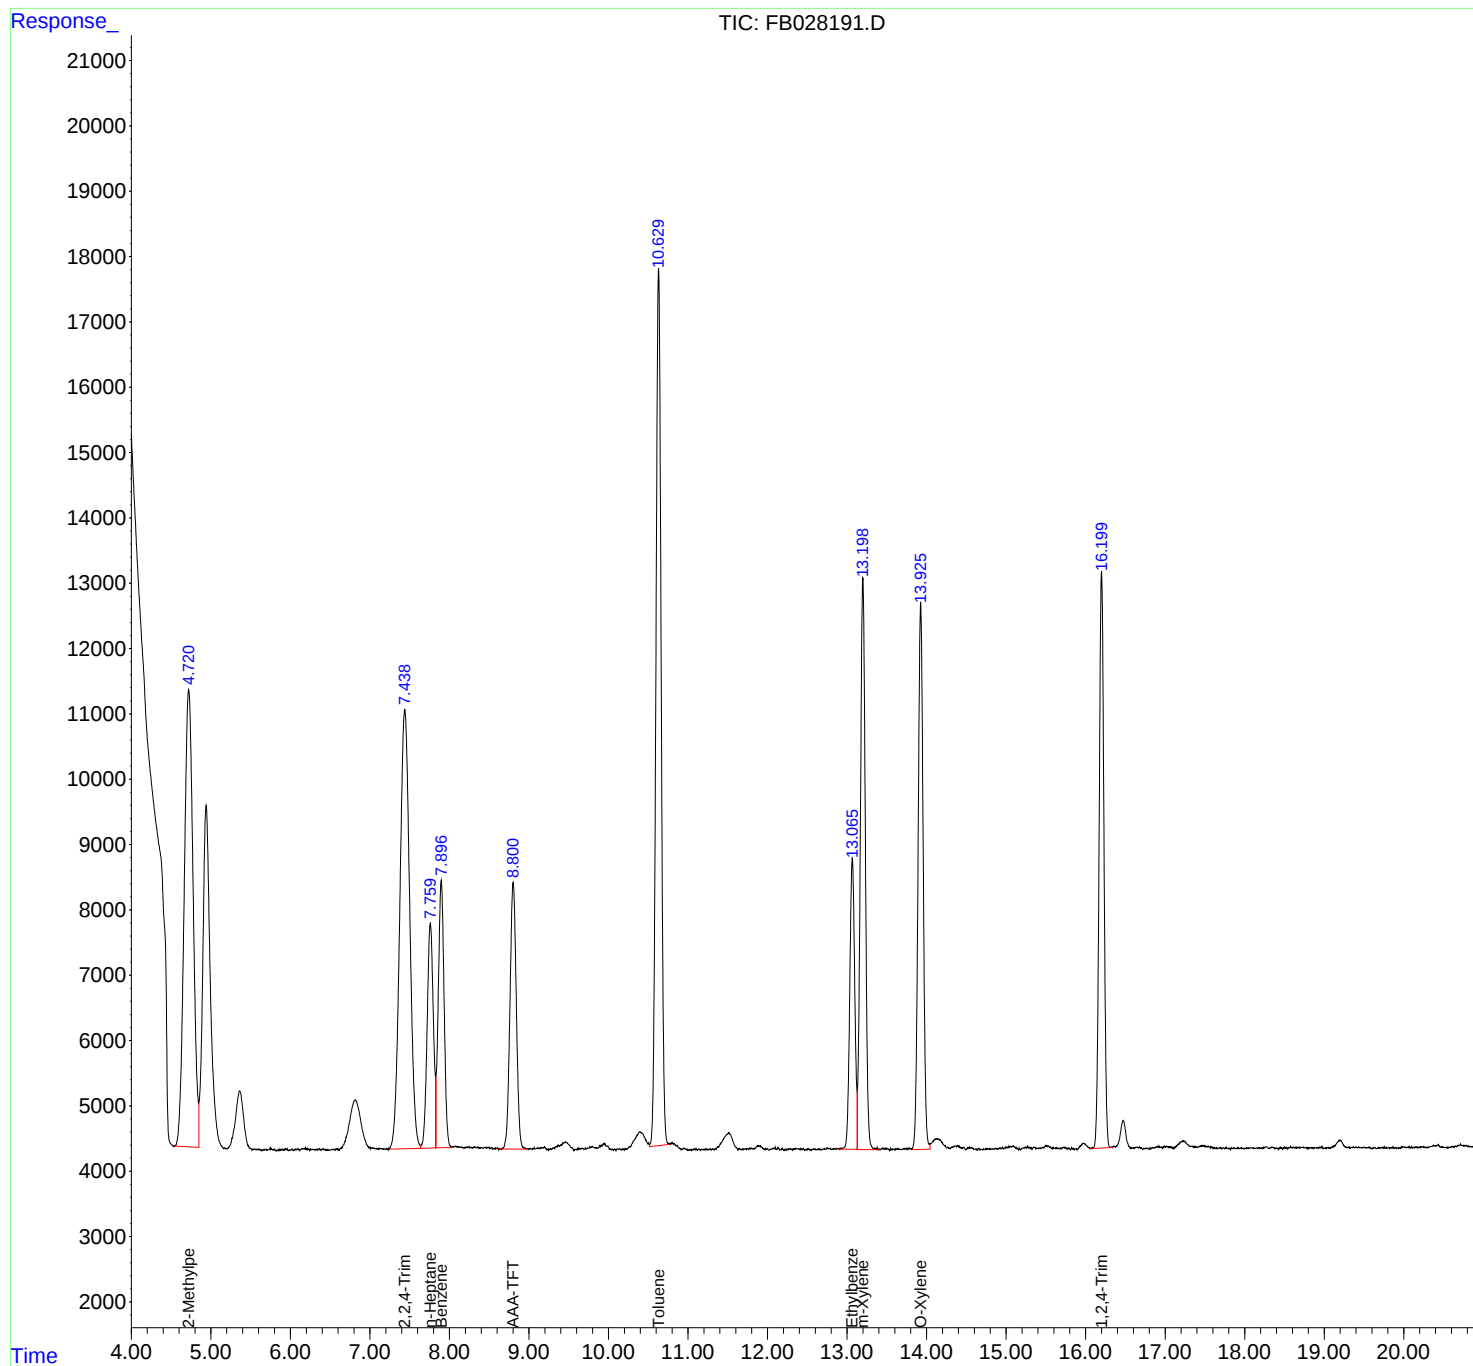


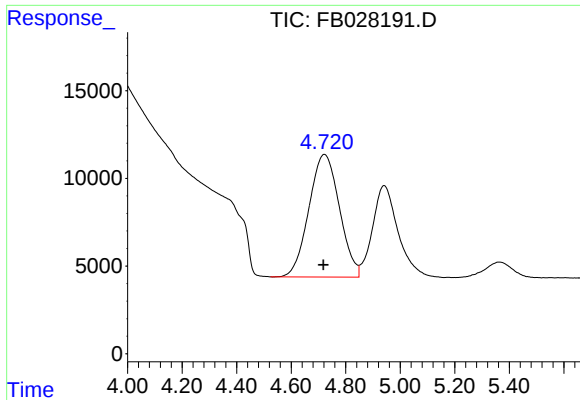

#1 2-Methylpentane


R.T.: 4.722 min
Delta R.T.: 0.004 min
Response: 544369
Conc: 26.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0908S1

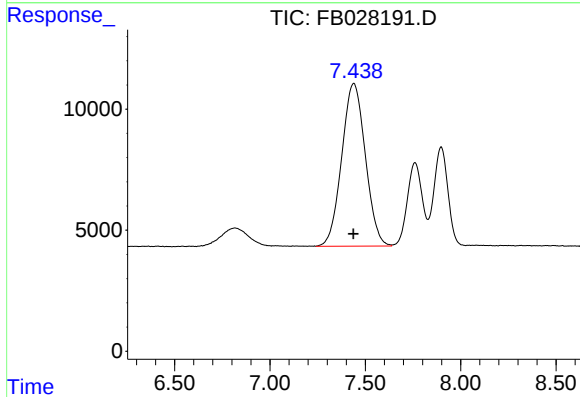


#2 2,2,4-Trimethylpentane

R.T.: 7.440 min
Delta R.T.: 0.003 min
Response: 577667
Conc: 27.46 ng/ml

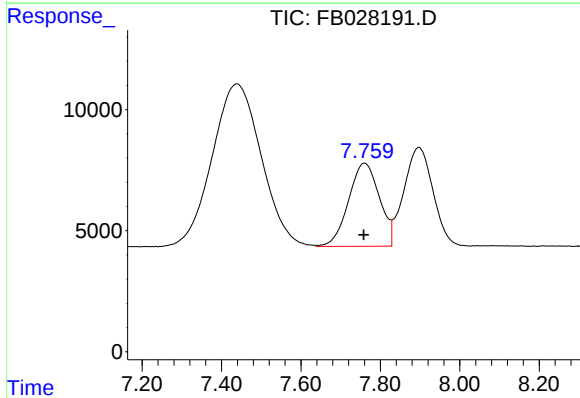


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.002 min
Response: 185618
Conc: 8.63 ng/ml

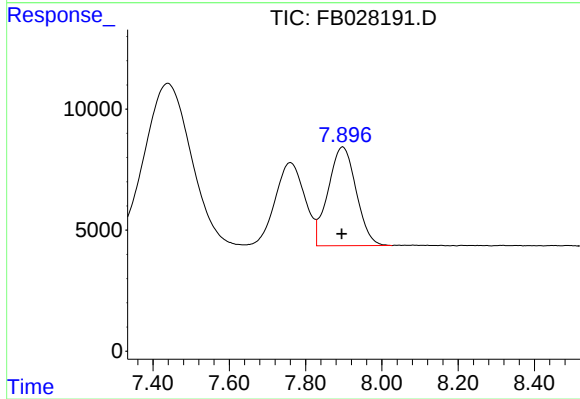

#4 Benzene


R.T.: 7.898 min
Delta R.T.: 0.003 min
Response: 208528
Conc: 8.48 ng/ml

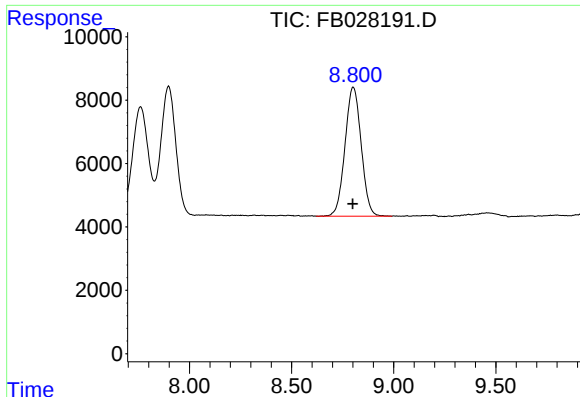

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.002 min
Response: 224749
Conc: 18.78 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0908S1

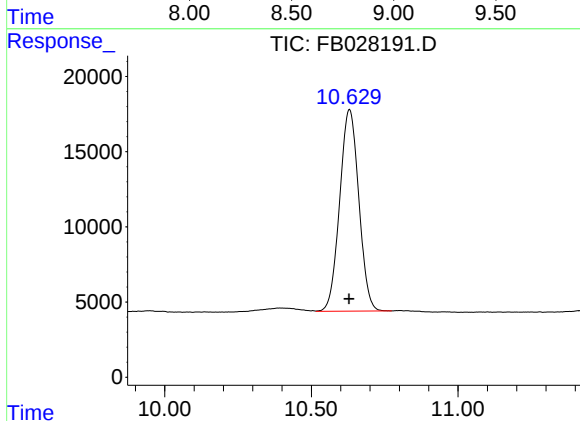


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.002 min
Response: 608736
Conc: 26.15 ng/ml

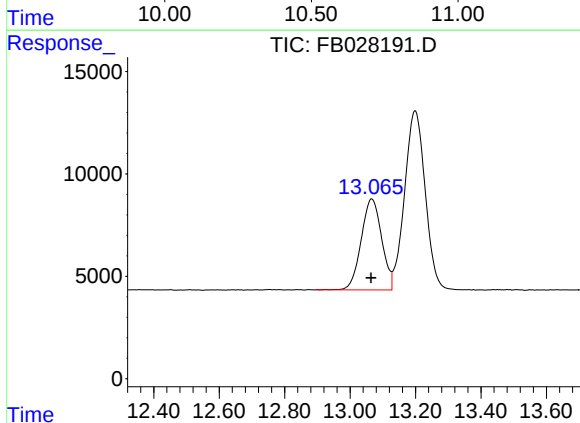


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.002 min
Response: 193226
Conc: 8.69 ng/ml

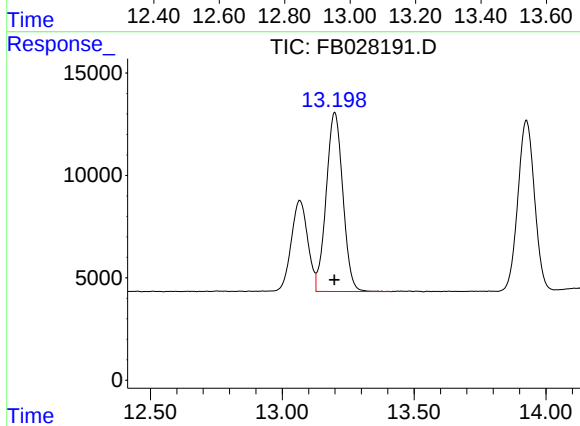

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: 0.002 min
Response: 384189
Conc: 17.61 ng/ml

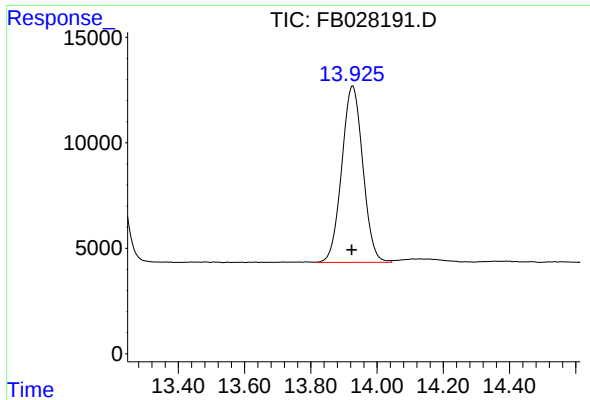

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.003 min
Response: 369140
Conc: 17.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0908S1

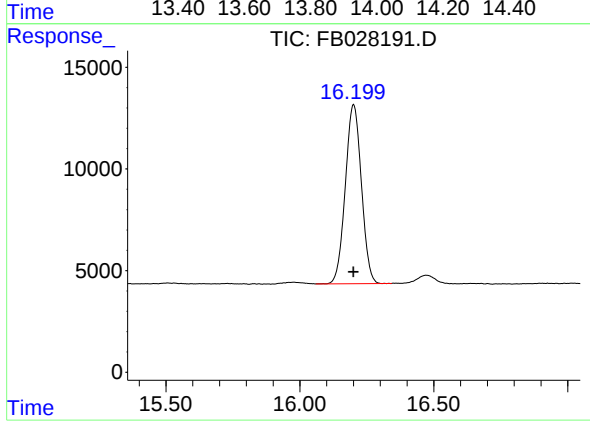

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.002 min
Response: 367648
Conc: 18.28 ng/ml