

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090822\
 Data File : FB028184.D
 Signal(s) : FID2B.CH
 Acq On : 8 Sep 2022 14:01
 Operator : AJ/MA
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 GRO STD

Integration File: Calibration.e
 Quant Time: Sep 08 14:14:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 14:13:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	244864	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	610912	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.437	633088	30.000 ng/ml
3) t n-Heptane	7.758	213207	10.000 ng/ml
4) t Benzene	7.895	245410	10.000 ng/ml
6) t Toluene	10.628	693453	30.000 ng/ml
7) t Ethylbenzene	13.065	221359	10.000 ng/ml
8) t m-Xylene	13.197	434958	20.000 ng/ml
9) t O-Xylene	13.924	419623	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	404777	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090822\
Data File : FB028184.D
Signal(s) : FID2B.CH
Acq On : 8 Sep 2022 14:01
Operator : AJ/MA
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 GRO STD

Integration File: Calibration.e
Quant Time: Sep 08 14:14:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 14:13:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

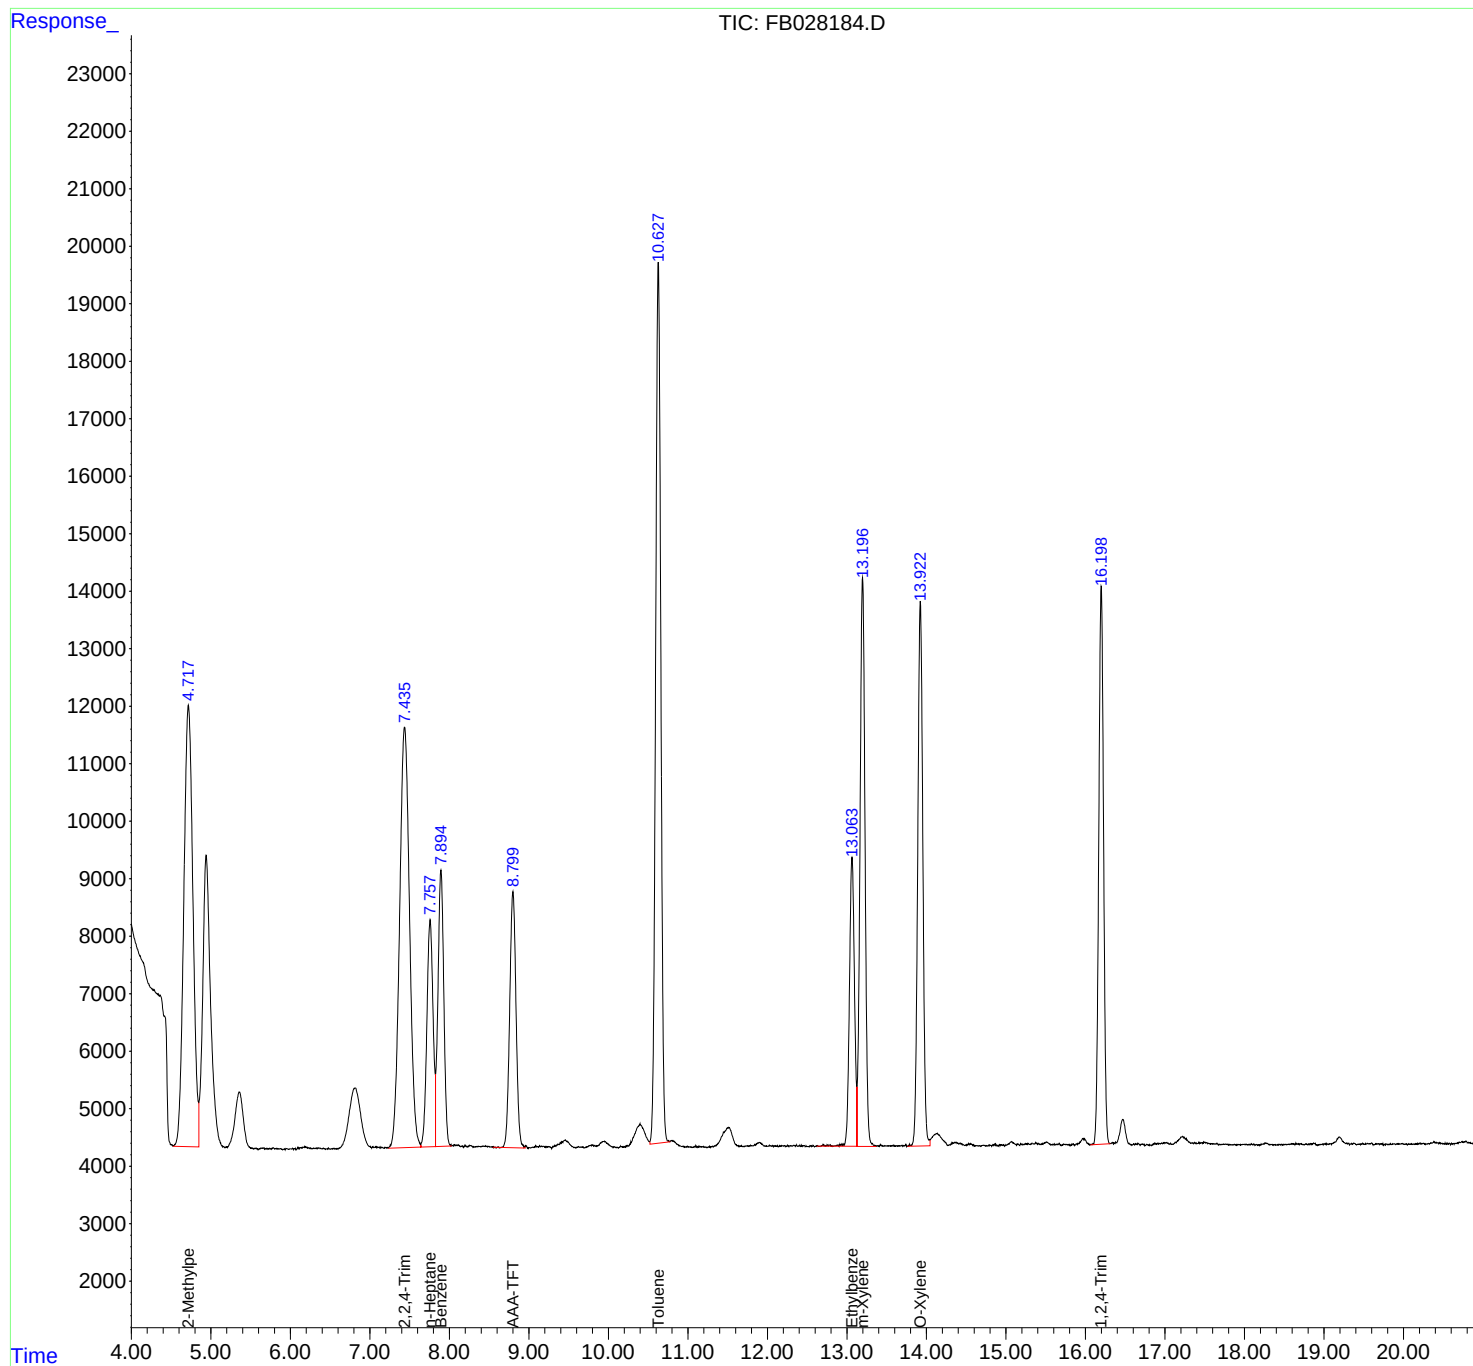


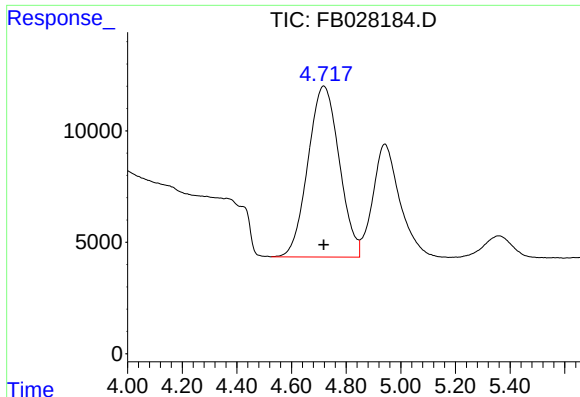

#1 2-Methylpentane


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 610912
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

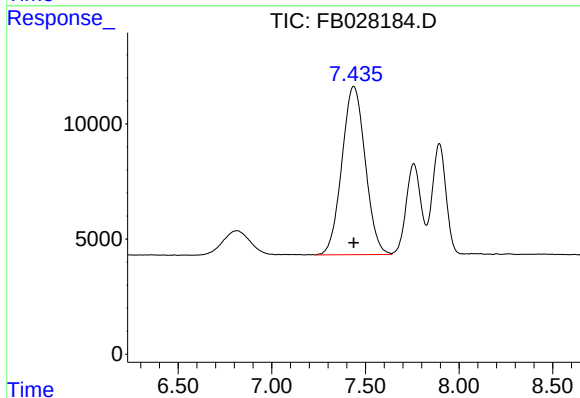


#2 2,2,4-Trimethylpentane

R.T.: 7.437 min
Delta R.T.: 0.000 min
Response: 633088
Conc: 30.00 ng/ml

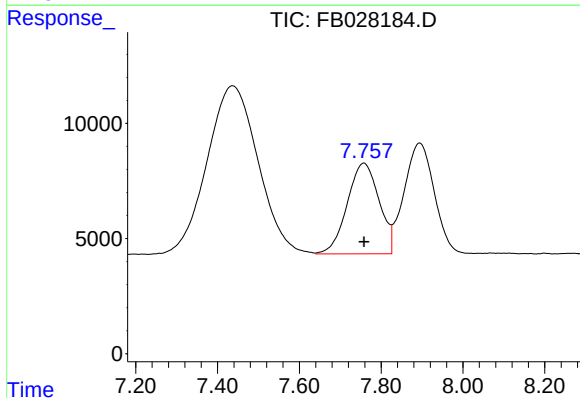


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 213207
Conc: 10.00 ng/ml

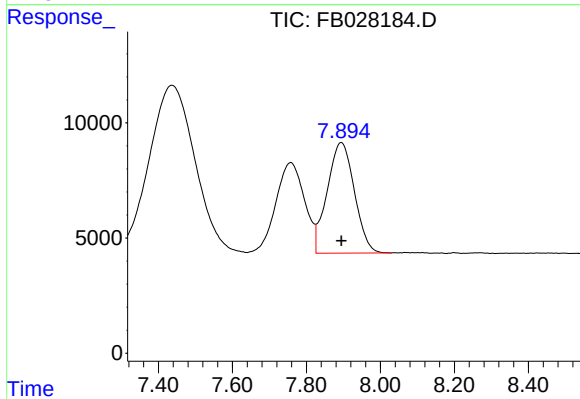

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 245410
Conc: 10.00 ng/ml

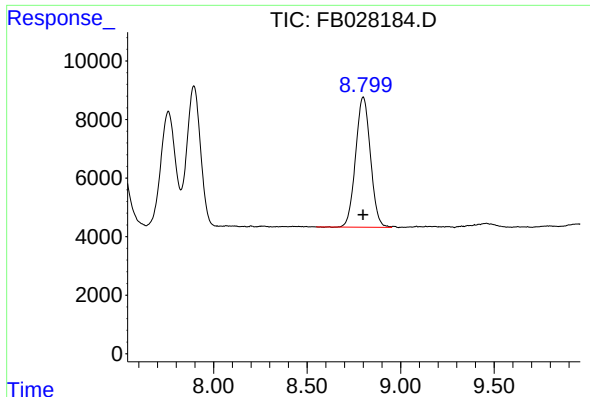

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 244864
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

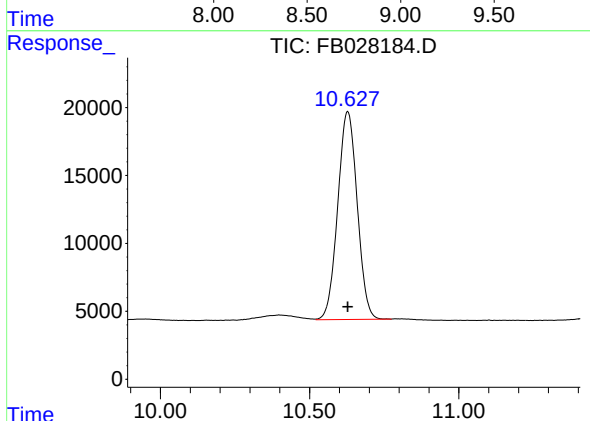


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 693453
Conc: 30.00 ng/ml

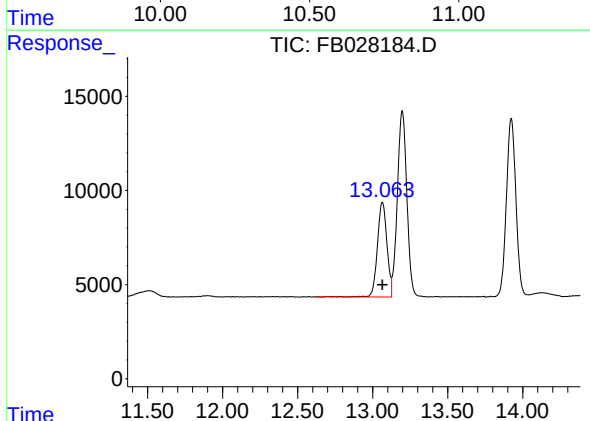


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: 0.000 min
Response: 221359
Conc: 10.00 ng/ml

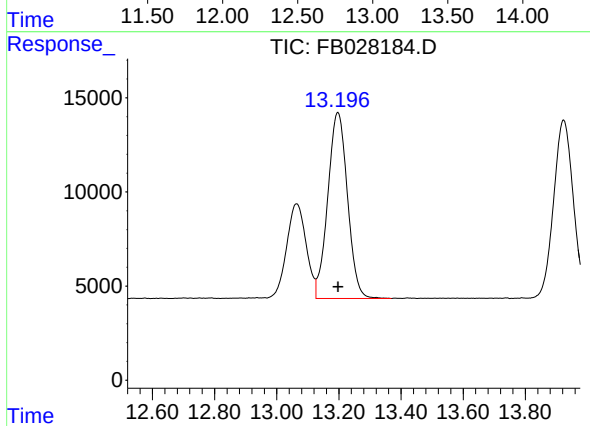

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.000 min
Response: 434958
Conc: 20.00 ng/ml

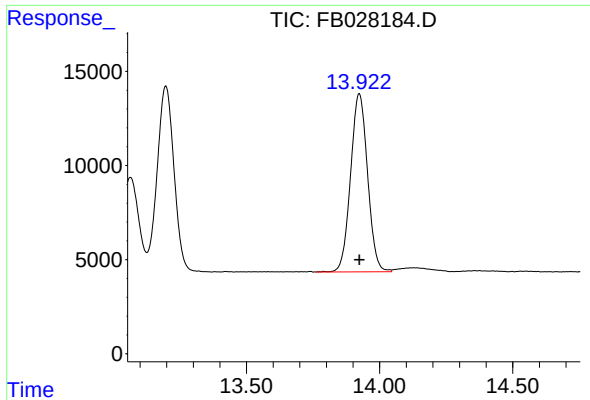

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.000 min
Response: 419623
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

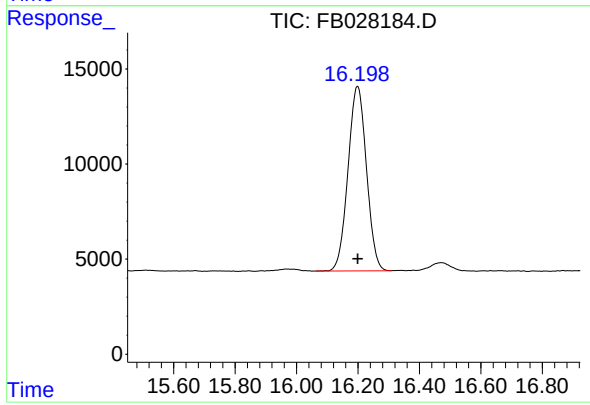

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.000 min
Response: 404777
Conc: 20.00 ng/ml