

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090822\
Data File : FB028199.D
Signal(s) : FID2B.CH
Acq On : 9 Sep 2022 00:38
Operator : AJ/MA
Sample : N4509-07
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
S1-SO_PW002-20220902

Integration File: Calibration.e
Quant Time: Sep 09 07:12:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090822\
Data File : FB028199.D
Signal(s) : FID2B.CH
Acq On : 9 Sep 2022 00:38
Operator : AJ/MA
Sample : N4509-07
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
S1-SO_PW002-20220902

Integration File: Calibration.e
Quant Time: Sep 09 07:12:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

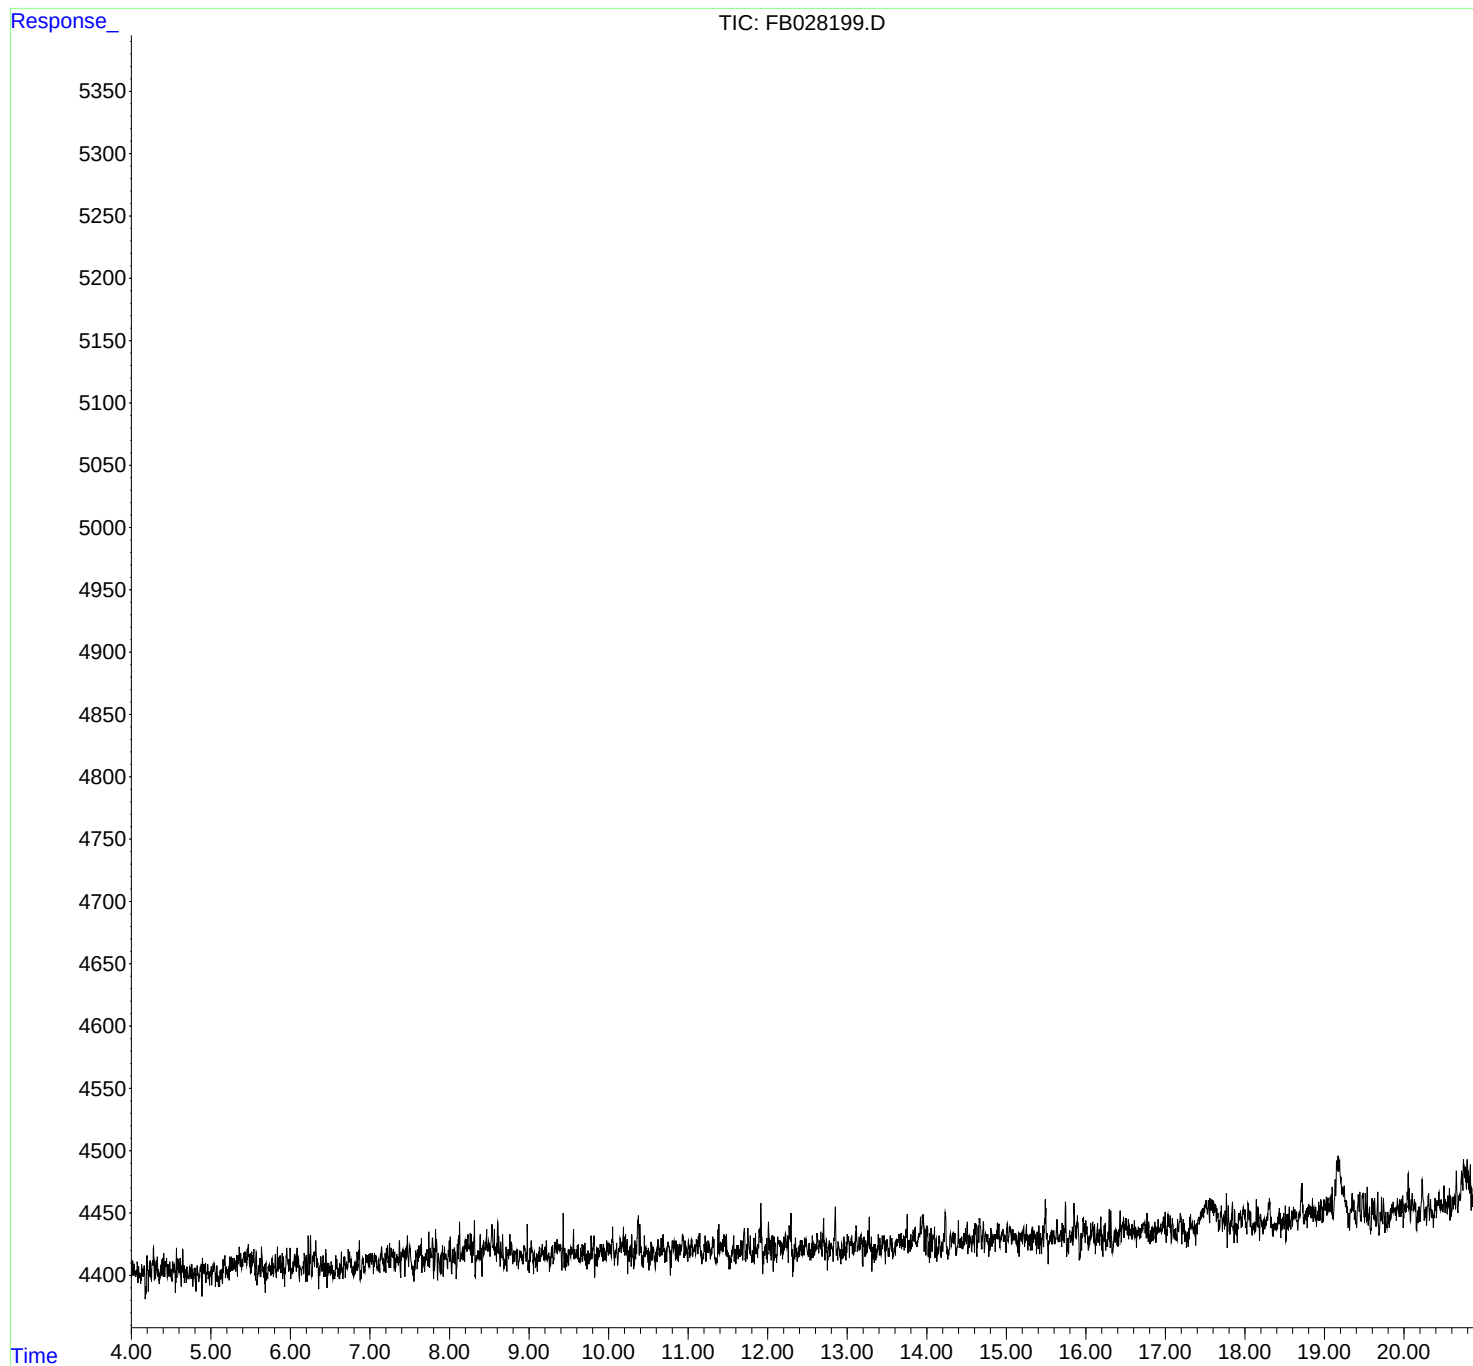

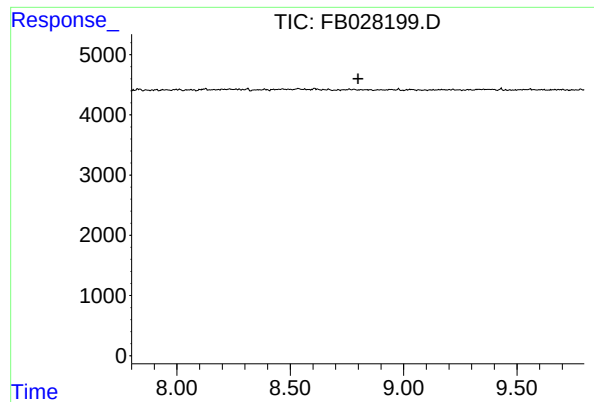

#5 AAA-TFT

R.T.: 0.000 min
Exp R.T.: 8.800 min
Response: 0
Conc: N.D.

Instrument :

FID_B

ClientSampleId :

S1-SO_PW002-20220902