

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090822\
 Data File : FB028209.D
 Signal(s) : FID2B.CH
 Acq On : 9 Sep 2022 7:22
 Operator : AJ/MA
 Sample : BSF0908S2
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0908S2

Integration File: Calibration.e
 Quant Time: Sep 09 07:44:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	213660	17.851 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	599022	29.586 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	626969	29.804 ng/ml
3) t n-Heptane	7.753	201673	9.382 ng/ml
4) t Benzene	7.889	240405	9.772 ng/ml
6) t Toluene	10.622	695973	29.894 ng/ml
7) t Ethylbenzene	13.058	212922	9.574 ng/ml
8) t m-Xylene	13.191	424614	19.458 ng/ml
9) t O-Xylene	13.918	414136	19.766 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	407381	20.261 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090822\
Data File : FB028209.D
Signal(s) : FID2B.CH
Acq On : 9 Sep 2022 7:22
Operator : AJ/MA
Sample : BSF0908S2
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0908S2

Integration File: Calibration.e
Quant Time: Sep 09 07:44:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

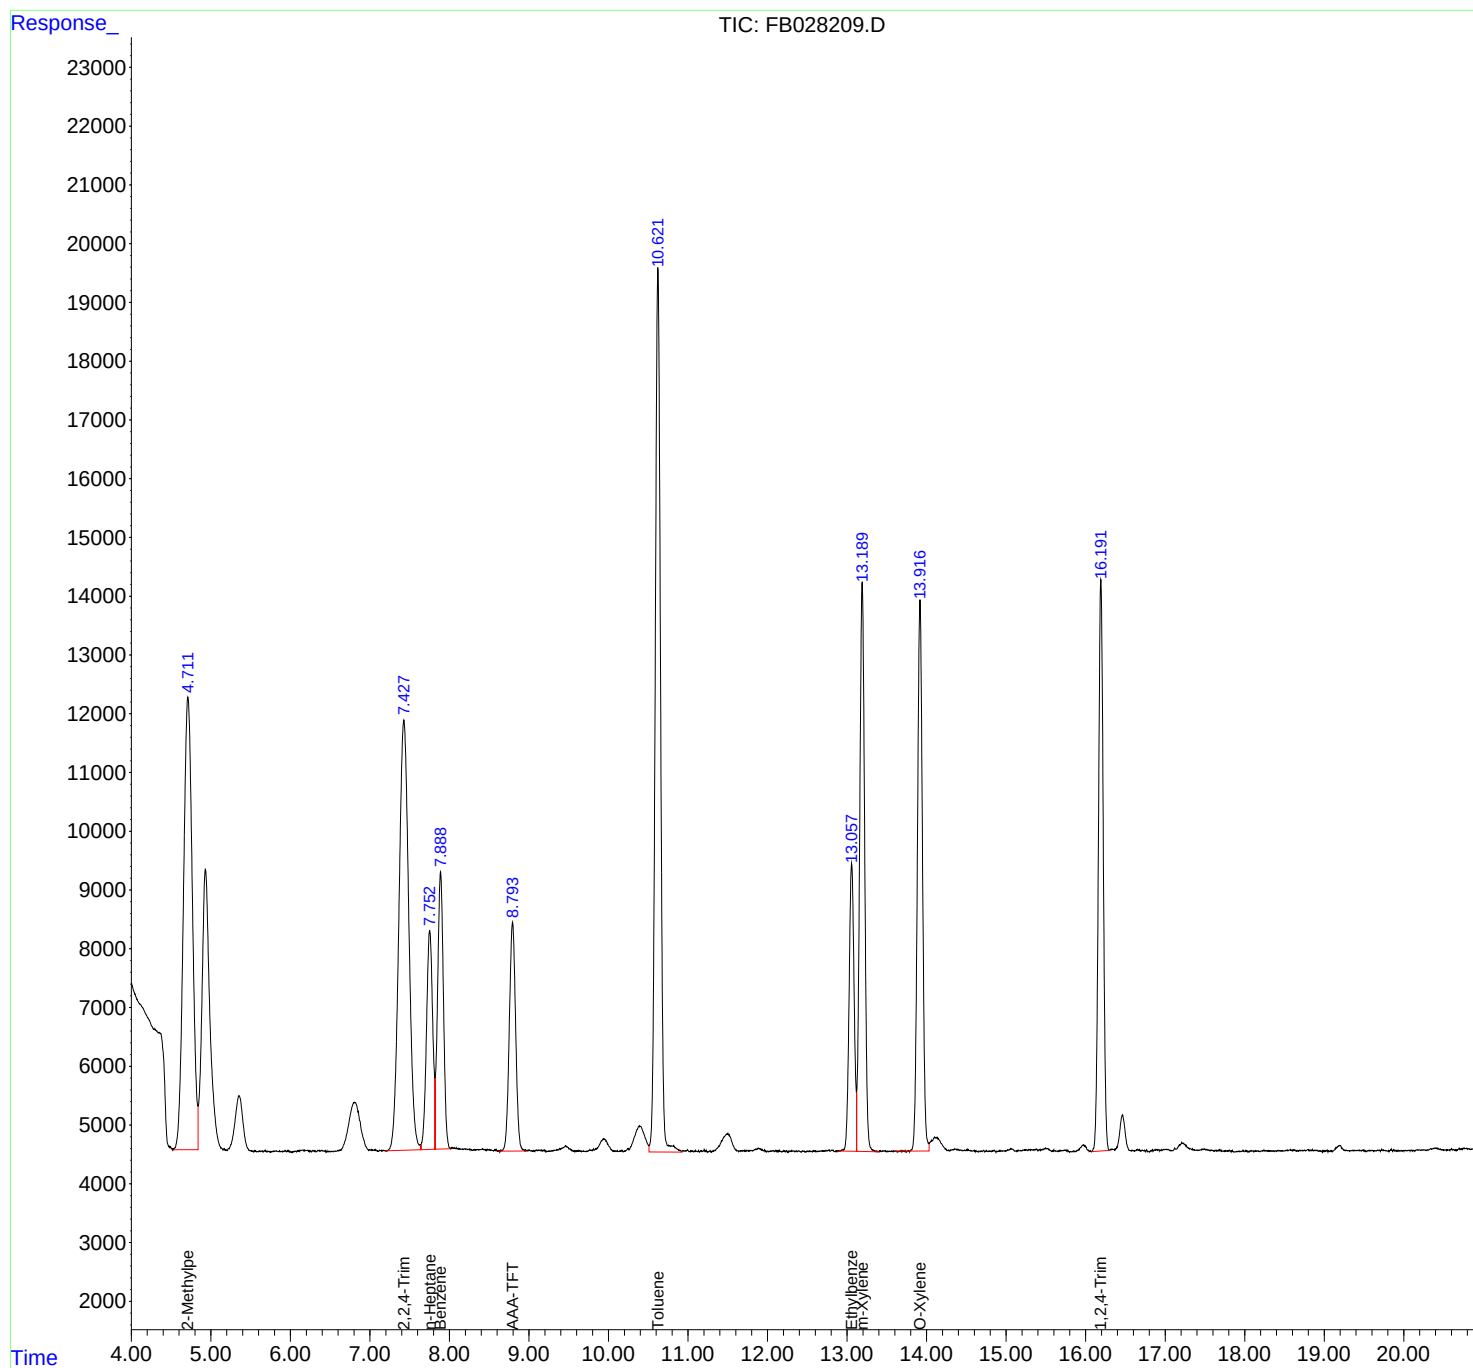


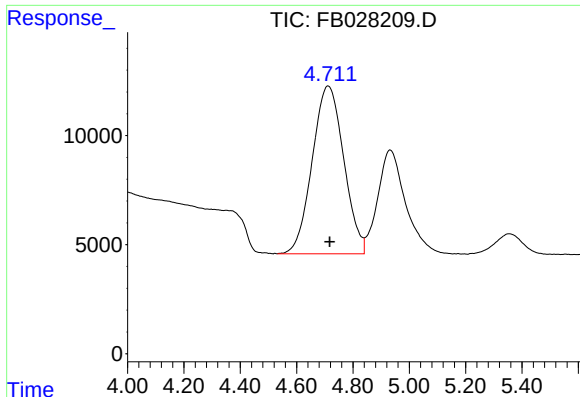

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: -0.006 min
Response: 599022
Conc: 29.59 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0908S2

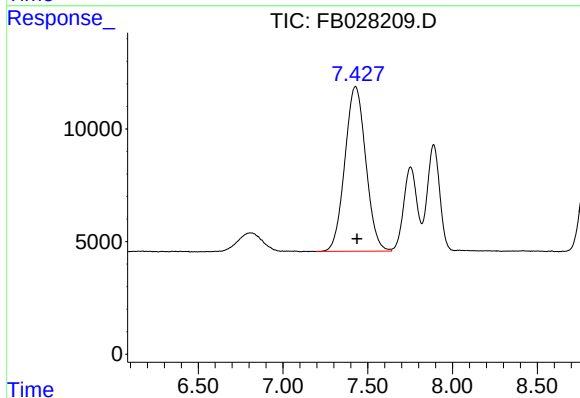


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: -0.009 min
Response: 626969
Conc: 29.80 ng/ml

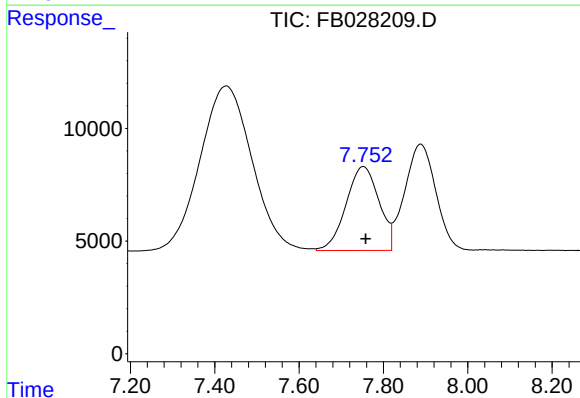


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.006 min
Response: 201673
Conc: 9.38 ng/ml

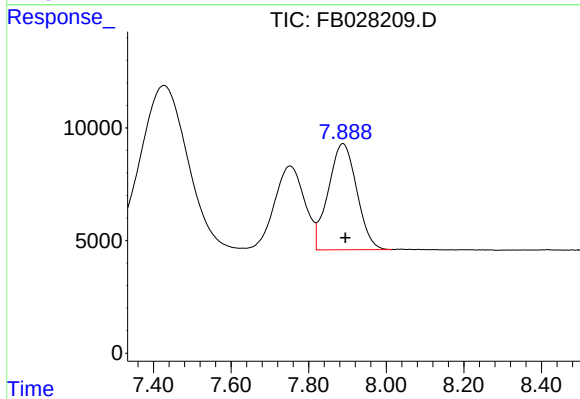

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.006 min
Response: 240405
Conc: 9.77 ng/ml

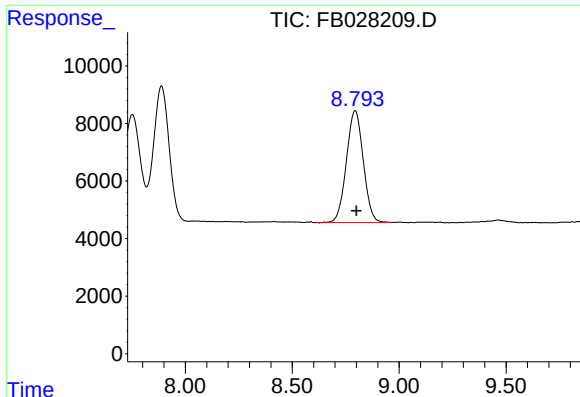

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.005 min
Response: 213660
Conc: 17.85 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0908S2

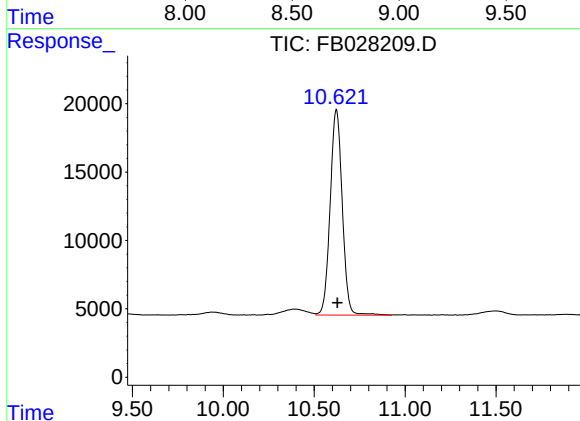


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.006 min
Response: 695973
Conc: 29.89 ng/ml

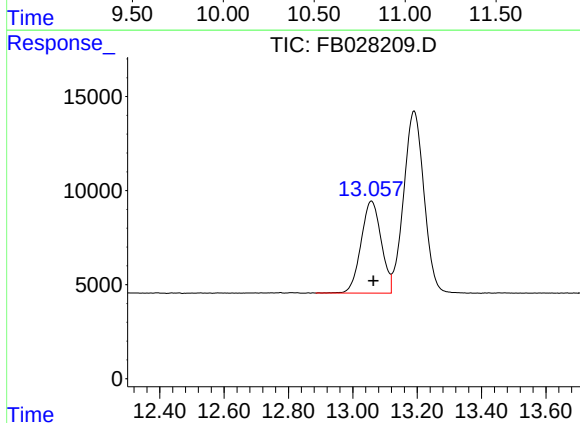


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: -0.006 min
Response: 212922
Conc: 9.57 ng/ml

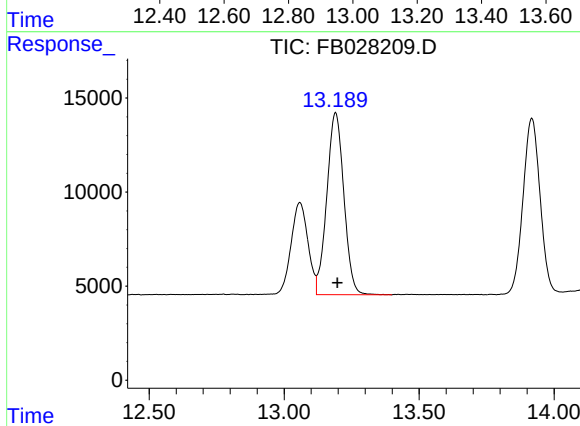

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: -0.006 min
Response: 424614
Conc: 19.46 ng/ml

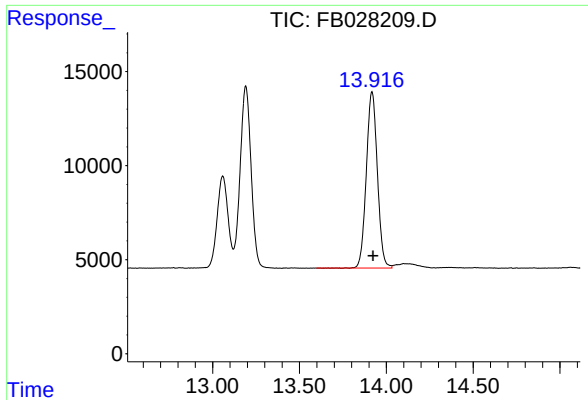

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: -0.006 min
Response: 414136
Conc: 19.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0908S2

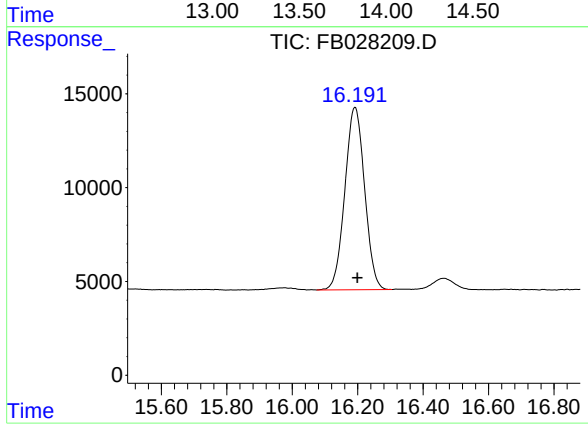

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.007 min
Response: 407381
Conc: 20.26 ng/ml