

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090919\
 Data File : FB022411.D
 Signal(s) : FID2B.CH
 Acq On : 9 Sep 2019 20:14
 Operator : DD/AJ
 Sample : K4757-05MS
 Misc : 5.01g/5.00ML DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 10 05:02:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.970	516279	17.749 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.835	1053230	21.436 ng/ml
2) t	2,2,4-Trimethylpentane	7.587	1175172	22.758 ng/ml
3) t	n-Heptane	7.928	387131	7.692 ng/ml
4) t	Benzene	8.063	470166	7.922 ng/ml
6) t	Toluene	10.811	1358646	28.559 ng/ml
7) t	Ethylbenzene	13.257	418598	13.963 ng/ml
8) t	m-Xylene	13.390	824415	31.032 ng/ml
9) t	O-Xylene	14.119	765964	31.573 ng/ml
10) t	1,2,4-Trimethylbenzene	16.400	509003	19.524 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090919\
Data File : FB022411.D
Signal(s) : FID2B.CH
Acq On : 9 Sep 2019 20:14
Operator : DD/AJ
Sample : K4757-05MS
Misc : 5.01g/5.00ML DI WATER
ALS Vial : 22 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 10 05:02:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

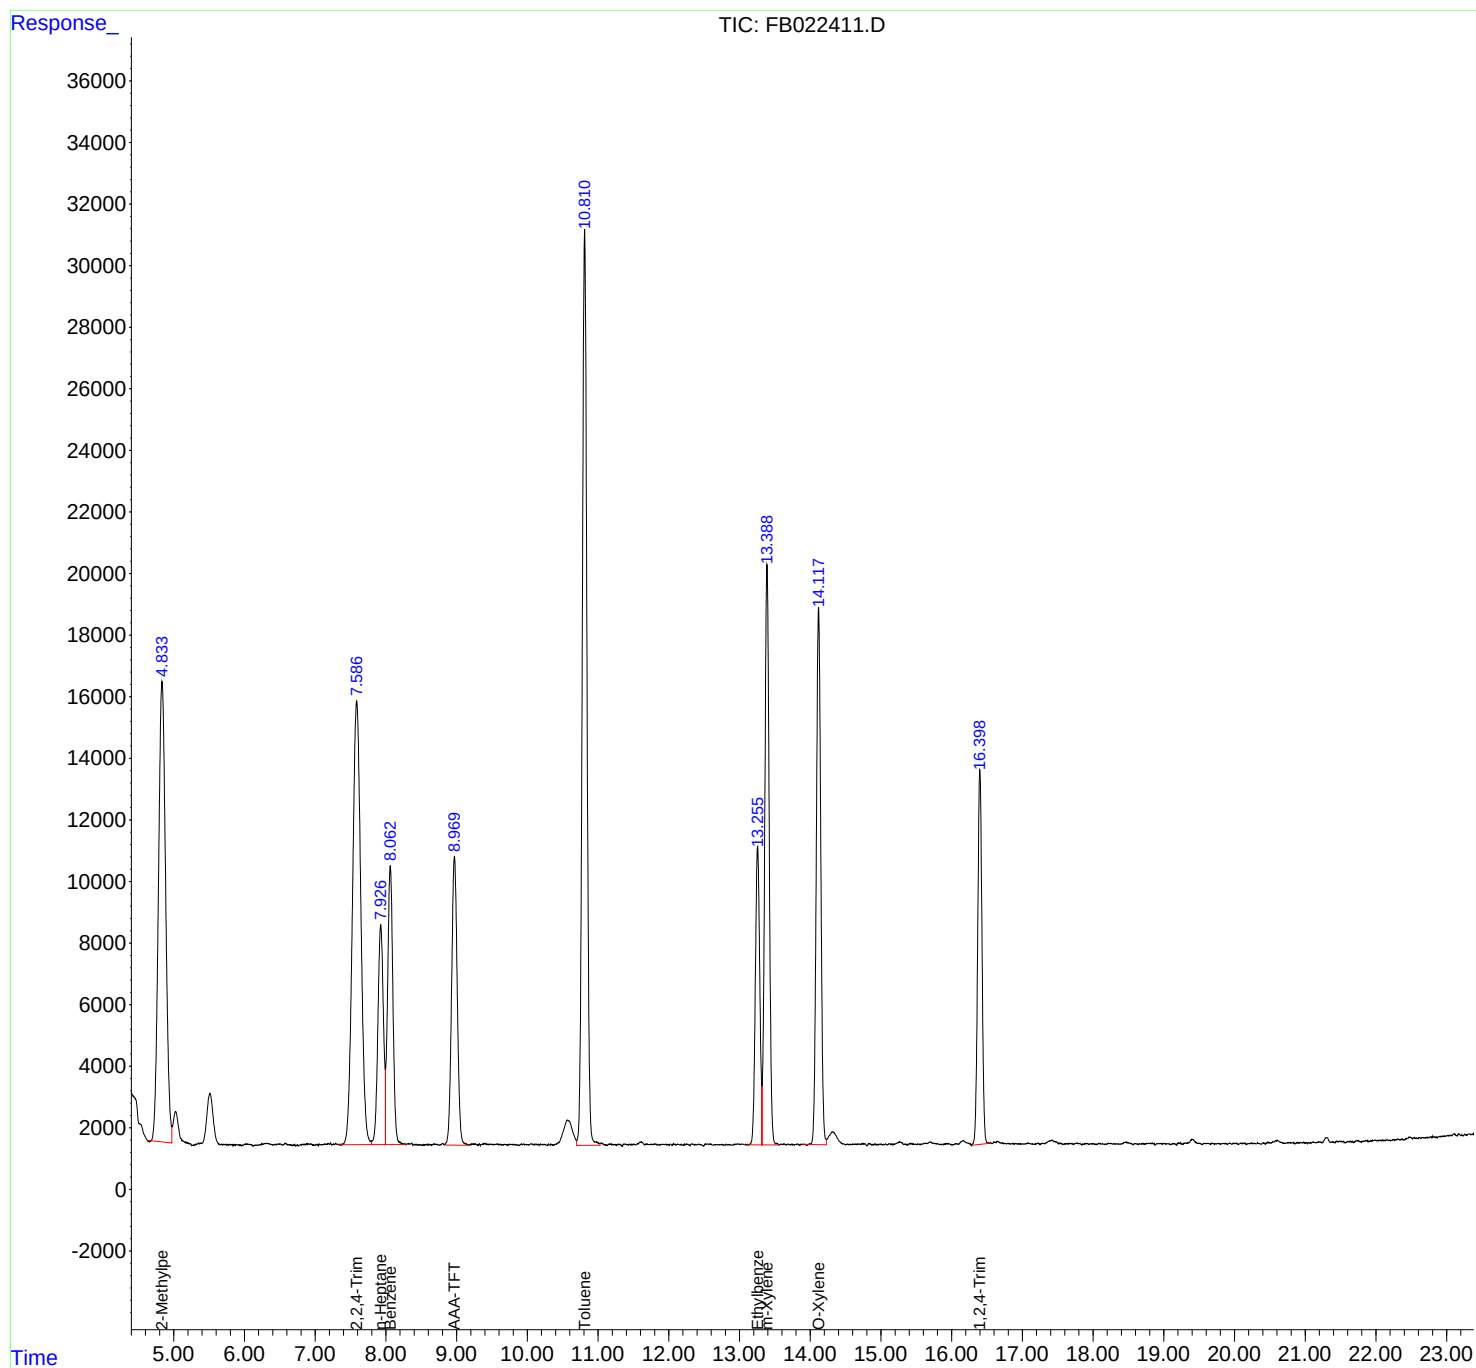

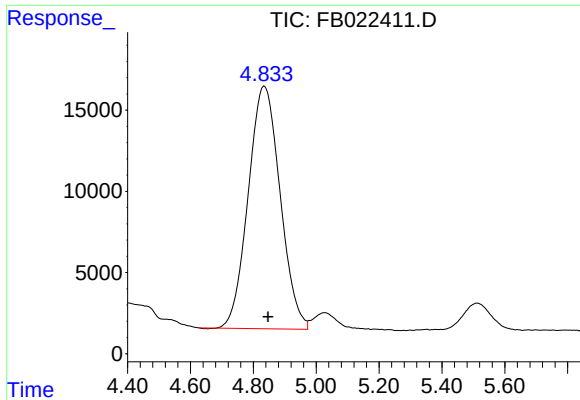


#1 2-Methylpentane

R.T.: 4.835 min
Delta R.T.: -0.012 min
Response: 1053230
Conc: 21.44 ng/ml

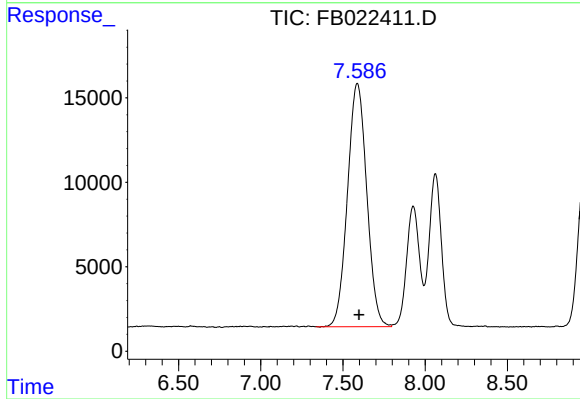


#2 2,2,4-Trimethylpentane

R.T.: 7.587 min
Delta R.T.: -0.010 min
Response: 1175172
Conc: 22.76 ng/ml

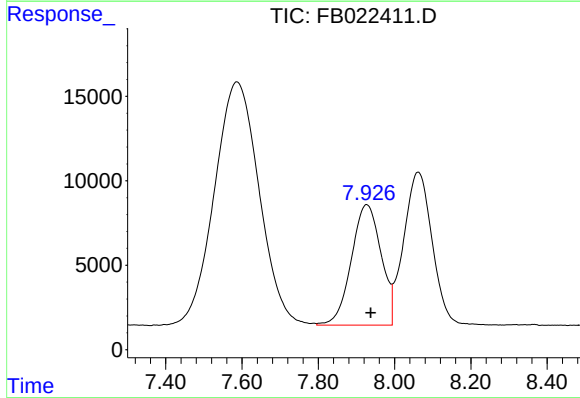


#3 n-Heptane

R.T.: 7.928 min
Delta R.T.: -0.010 min
Response: 387131
Conc: 7.69 ng/ml

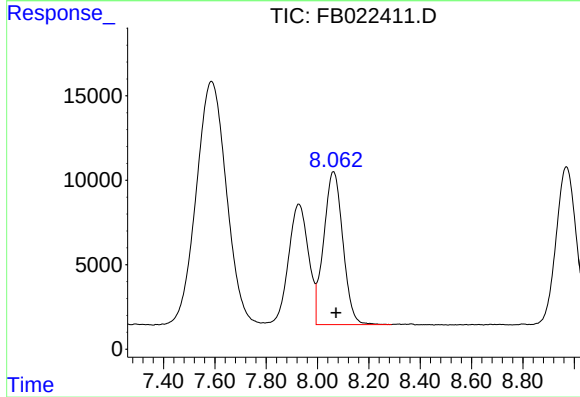


#4 Benzene

R.T.: 8.063 min
Delta R.T.: -0.010 min
Response: 470166
Conc: 7.92 ng/ml

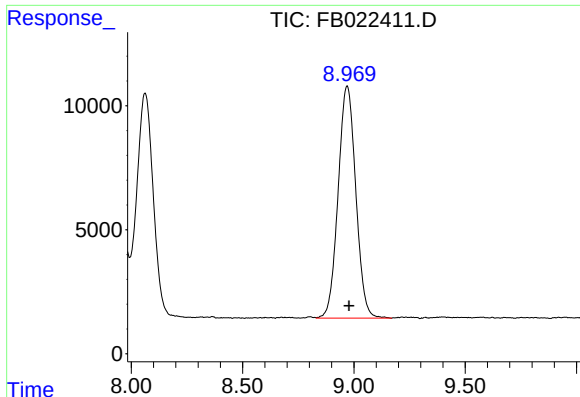


#5 AAA-TFT

R.T.: 8.970 min
Delta R.T.: -0.009 min
Response: 516279
Conc: 17.75 ng/ml

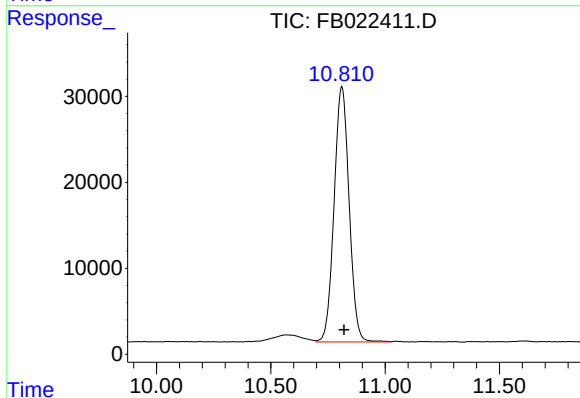


#6 Toluene

R.T.: 10.811 min
Delta R.T.: -0.009 min
Response: 1358646
Conc: 28.56 ng/ml

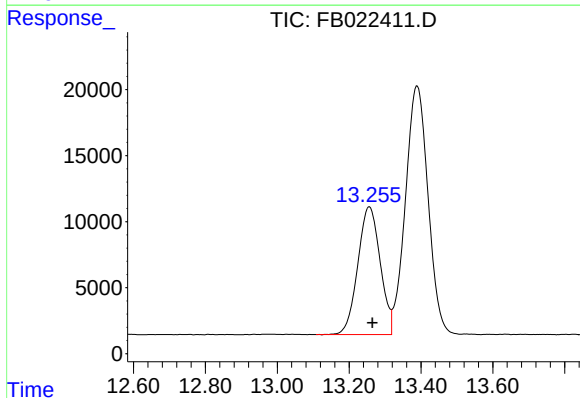


#7 Ethylbenzene

R.T.: 13.257 min
Delta R.T.: -0.008 min
Response: 418598
Conc: 13.96 ng/ml

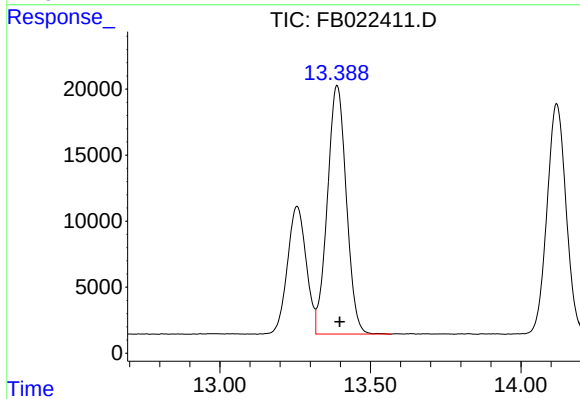


#8 m-Xylene

R.T.: 13.390 min
Delta R.T.: -0.008 min
Response: 824415
Conc: 31.03 ng/ml

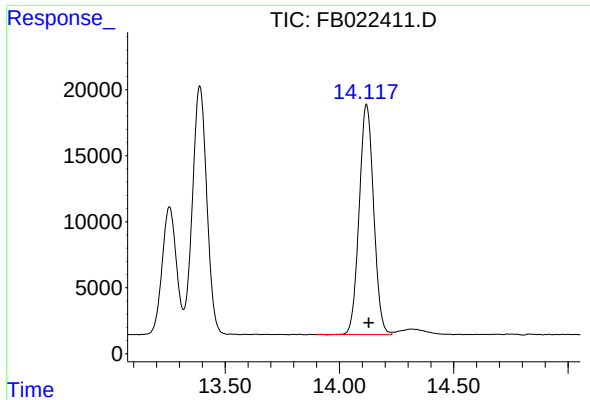

#9 O-Xylene

R.T.: 14.119 min
Delta R.T.: -0.009 min
Response: 765964
Conc: 31.57 ng/ml

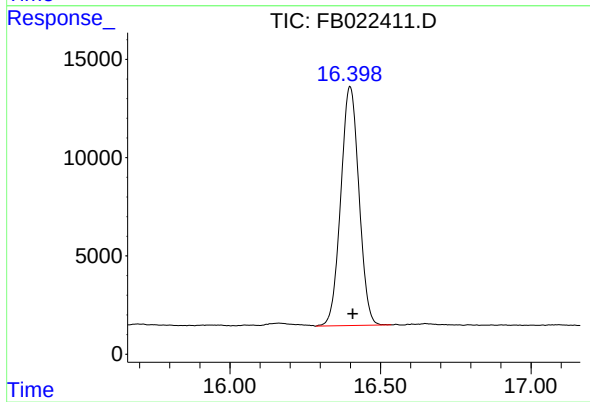

#10 1,2,4-Trimethylbenzene

R.T.: 16.400 min
Delta R.T.: -0.008 min
Response: 509003
Conc: 19.52 ng/ml