

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090919\
 Data File : FB022412.D
 Signal(s) : FID2B.CH
 Acq On : 9 Sep 2019 20:44
 Operator : DD/AJ
 Sample : K4757-05MSD
 Misc : 5.01g/5.00ML DI WATER
 ALS Vial : 23 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 10 05:03:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.970	516668	17.763 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.834	1120297	22.801 ng/ml
2) t 2,2,4-Trimethylpentane	7.587	1271413	24.622 ng/ml
3) t n-Heptane	7.927	417194	8.289 ng/ml
4) t Benzene	8.062	500807	8.438 ng/ml
6) t Toluene	10.810	1416823	29.782 ng/ml
7) t Ethylbenzene	13.257	440582	14.696 ng/ml
8) t m-Xylene	13.390	866639	32.622 ng/ml
9) t O-Xylene	14.120	805499	33.203 ng/ml
10) t 1,2,4-Trimethylbenzene	16.400	535107	20.525 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090919\
Data File : FB022412.D
Signal(s) : FID2B.CH
Acq On : 9 Sep 2019 20:44
Operator : DD/AJ
Sample : K4757-05MSD
Misc : 5.01g/5.00ML DI WATER
ALS Vial : 23 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 10 05:03:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

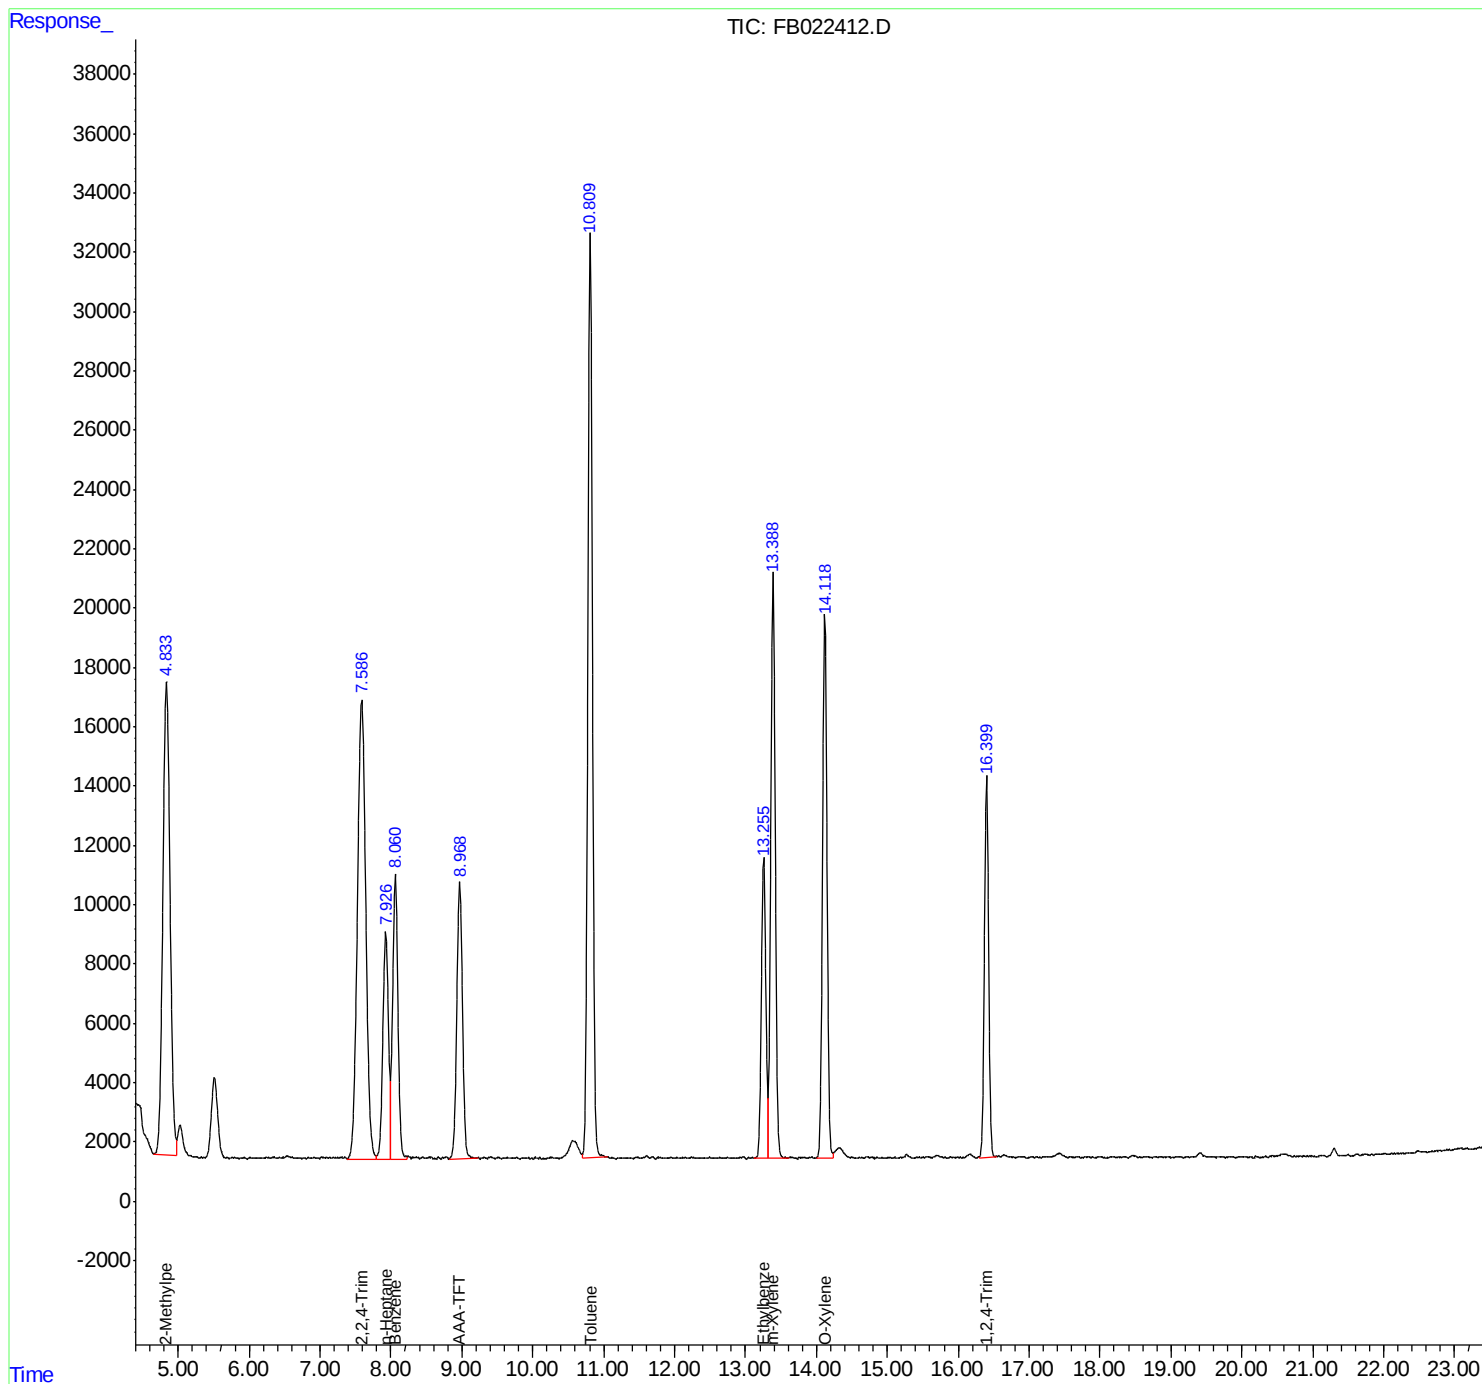

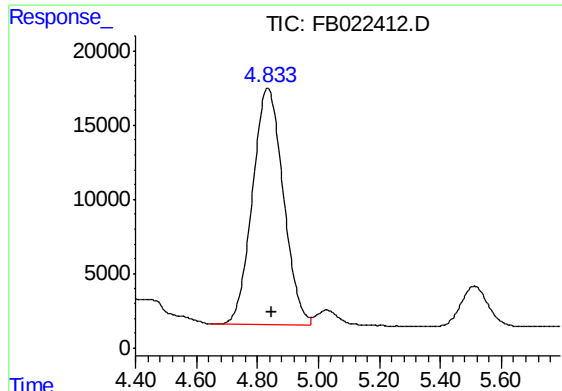


#1 2-Methylpentane

R.T.: 4.834 min
Delta R.T.: -0.013 min
Response: 1120297
Conc: 22.80 ng/ml

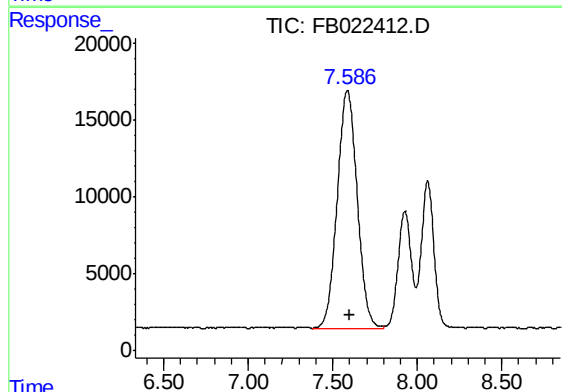


#2 2,2,4-Trimethylpentane

R.T.: 7.587 min
Delta R.T.: -0.011 min
Response: 1271413
Conc: 24.62 ng/ml

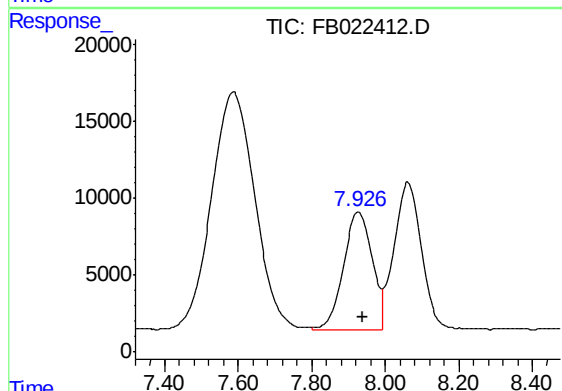


#3 n-Heptane

R.T.: 7.927 min
Delta R.T.: -0.011 min
Response: 417194
Conc: 8.29 ng/ml

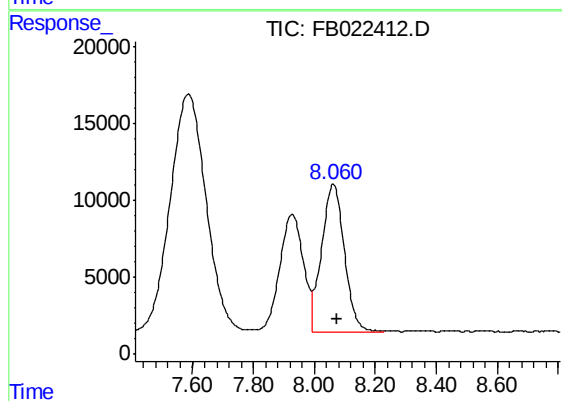


#4 Benzene

R.T.: 8.062 min
Delta R.T.: -0.011 min
Response: 500807
Conc: 8.44 ng/ml

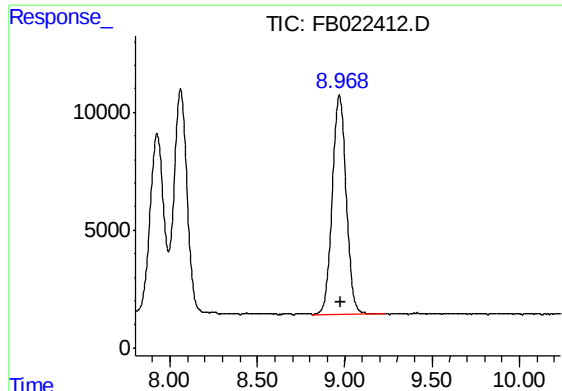


#5 AAA-TFT

R.T.: 8.970 min
Delta R.T.: -0.010 min
Response: 516668
Conc: 17.76 ng/ml

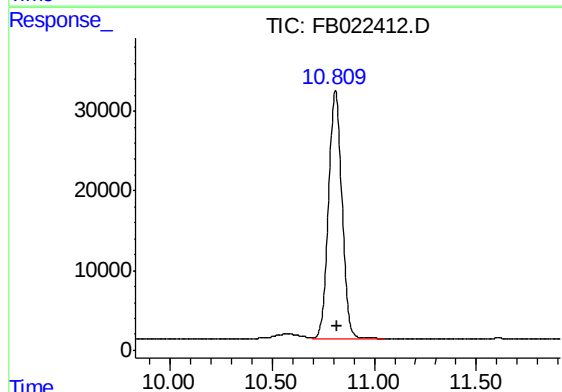


#6 Toluene

R.T.: 10.810 min
Delta R.T.: -0.009 min
Response: 1416823
Conc: 29.78 ng/ml

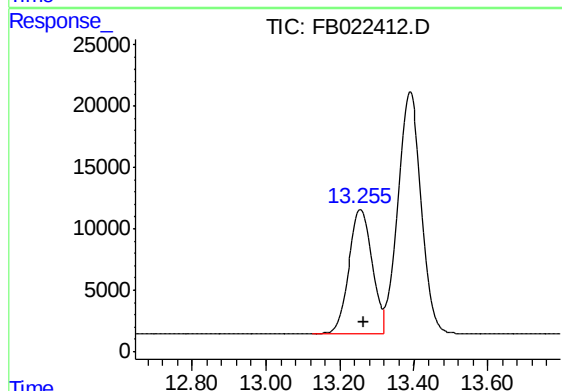


#7 Ethylbenzene

R.T.: 13.257 min
Delta R.T.: -0.008 min
Response: 440582
Conc: 14.70 ng/ml

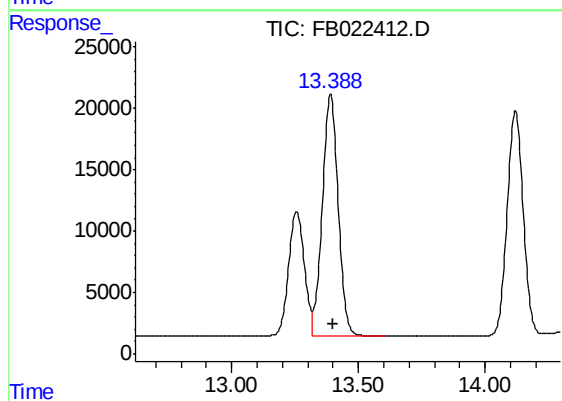


#8 m-Xylene

R.T.: 13.390 min
Delta R.T.: -0.008 min
Response: 866639
Conc: 32.62 ng/ml

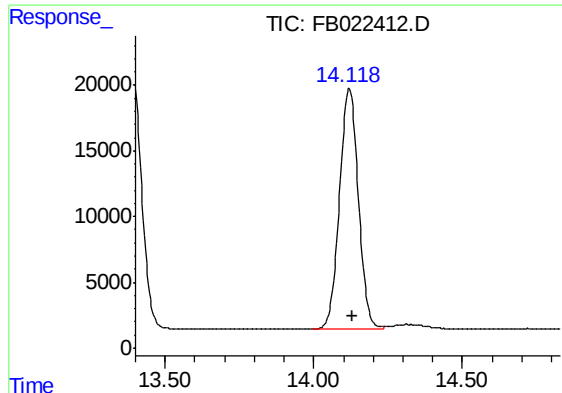

#9 O-Xylene

R.T.: 14.120 min
Delta R.T.: -0.008 min
Response: 805499
Conc: 33.20 ng/ml

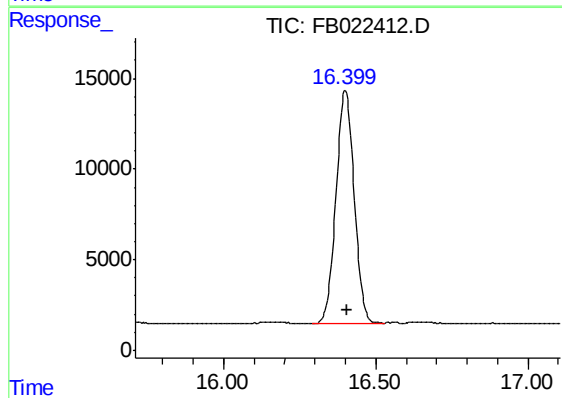

#10 1,2,4-Trimethylbenzene

R.T.: 16.400 min
Delta R.T.: -0.007 min
Response: 535107
Conc: 20.52 ng/ml