

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090922\
 Data File : FB028217.D
 Signal(s) : FID2B.CH
 Acq On : 9 Sep 2022 13:47
 Operator : AJ/MA
 Sample : BSF0909S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0909S1

Integration File: Calibration.e
 Quant Time: Sep 12 01:41:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	226918	18.959 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	632828	31.255 ng/ml
2) t 2,2,4-Trimethylpentane	7.437	667892	31.750 ng/ml
3) t n-Heptane	7.756	217390	10.113 ng/ml
4) t Benzene	7.892	261387	10.625 ng/ml
6) t Toluene	10.625	726621	31.210 ng/ml
7) t Ethylbenzene	13.062	227458	10.228 ng/ml
8) t m-Xylene	13.195	450302	20.635 ng/ml
9) t O-Xylene	13.922	437607	20.886 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	412687	20.524 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090922\
Data File : FB028217.D
Signal(s) : FID2B.CH
Acq On : 9 Sep 2022 13:47
Operator : AJ/MA
Sample : BSF0909S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0909S1

Integration File: Calibration.e
Quant Time: Sep 12 01:41:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

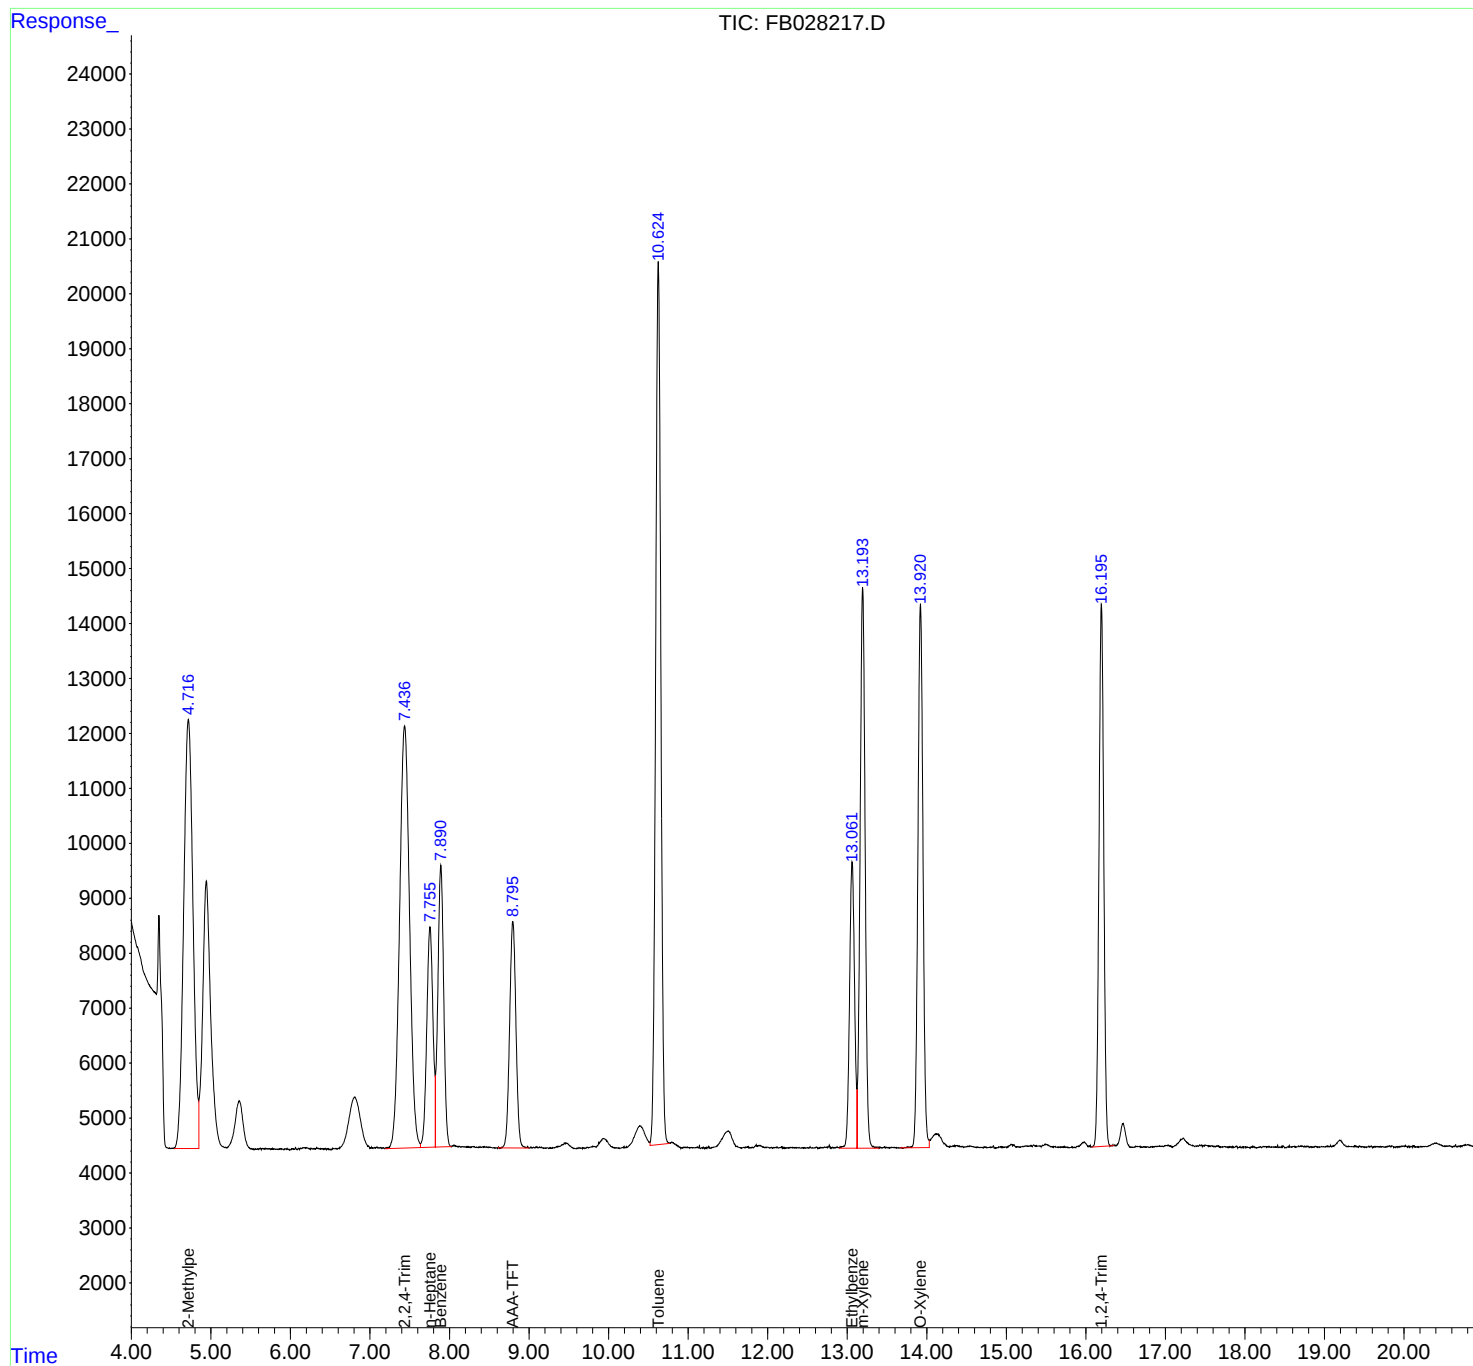


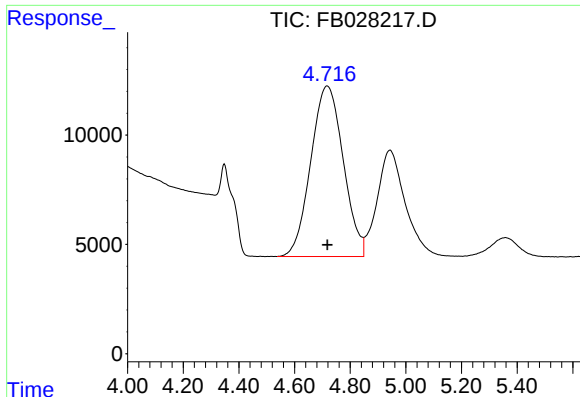

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: 0.000 min
Response: 632828
Conc: 31.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0909S1

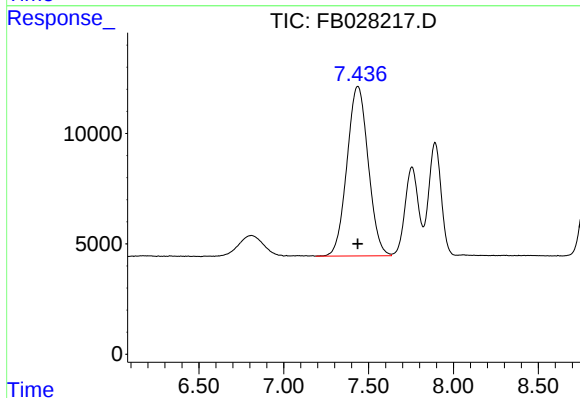


#2 2,2,4-Trimethylpentane

R.T.: 7.437 min
Delta R.T.: 0.000 min
Response: 667892
Conc: 31.75 ng/ml

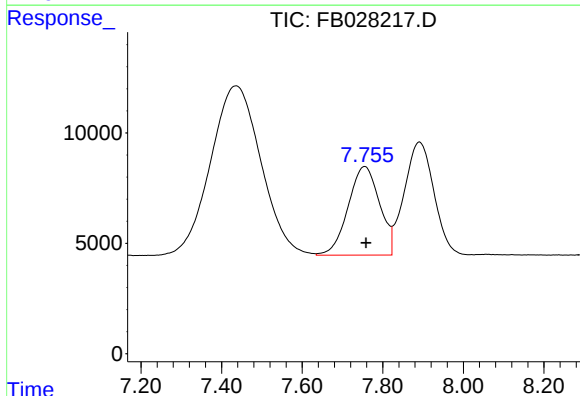


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 217390
Conc: 10.11 ng/ml

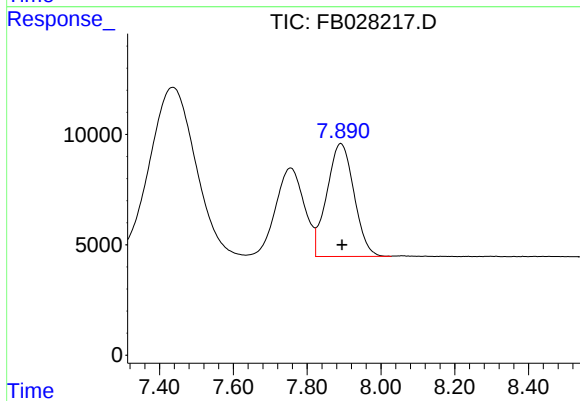

#4 Benzene


R.T.: 7.892 min
Delta R.T.: -0.003 min
Response: 261387
Conc: 10.62 ng/ml

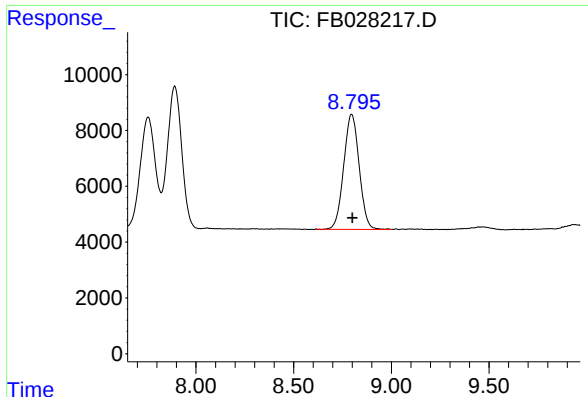

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.003 min
Response: 226918
Conc: 18.96 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0909S1

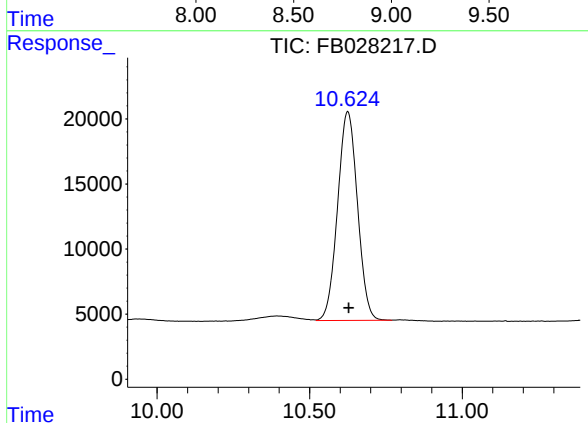


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.003 min
Response: 726621
Conc: 31.21 ng/ml

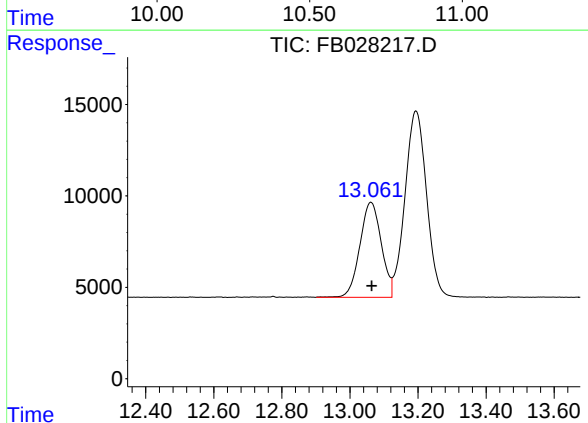


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.002 min
Response: 227458
Conc: 10.23 ng/ml

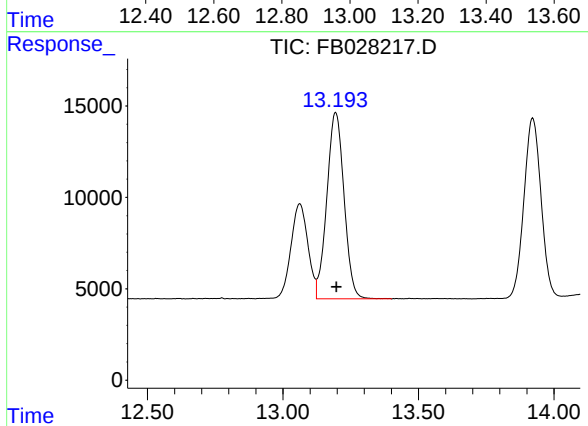

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: -0.003 min
Response: 450302
Conc: 20.63 ng/ml

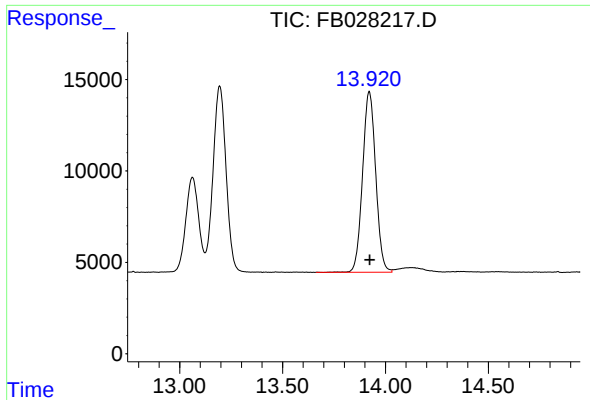

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.002 min
Response: 437607
Conc: 20.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0909S1

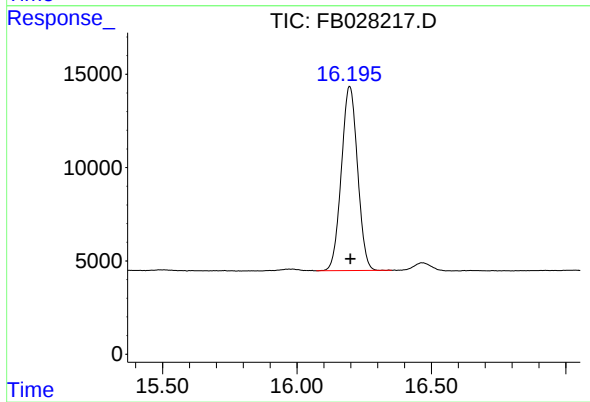

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: -0.003 min
Response: 412687
Conc: 20.52 ng/ml