

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090922\
 Data File : FB028221.D
 Signal(s) : FID2B.CH
 Acq On : 9 Sep 2022 16:19
 Operator : AJ/MA
 Sample : N4530-10MS
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-21-COMPMS

Integration File: Calibration.e
 Quant Time: Sep 12 01:41:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	213003	17.796 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	582588	28.774 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	607775	28.892 ng/ml
3) t n-Heptane	7.754	212235	9.873 ng/ml
4) t Benzene	7.891	266108	10.817 ng/ml
6) t Toluene	10.625	728441	31.288 ng/ml
7) t Ethylbenzene	13.063	226982	10.207 ng/ml
8) t m-Xylene	13.195	446113	20.443 ng/ml
9) t O-Xylene	13.923	429831	20.515 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	389048	19.349 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090922\
Data File : FB028221.D
Signal(s) : FID2B.CH
Acq On : 9 Sep 2022 16:19
Operator : AJ/MA
Sample : N4530-10MS
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-21-COMPMS

Integration File: Calibration.e
Quant Time: Sep 12 01:41:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

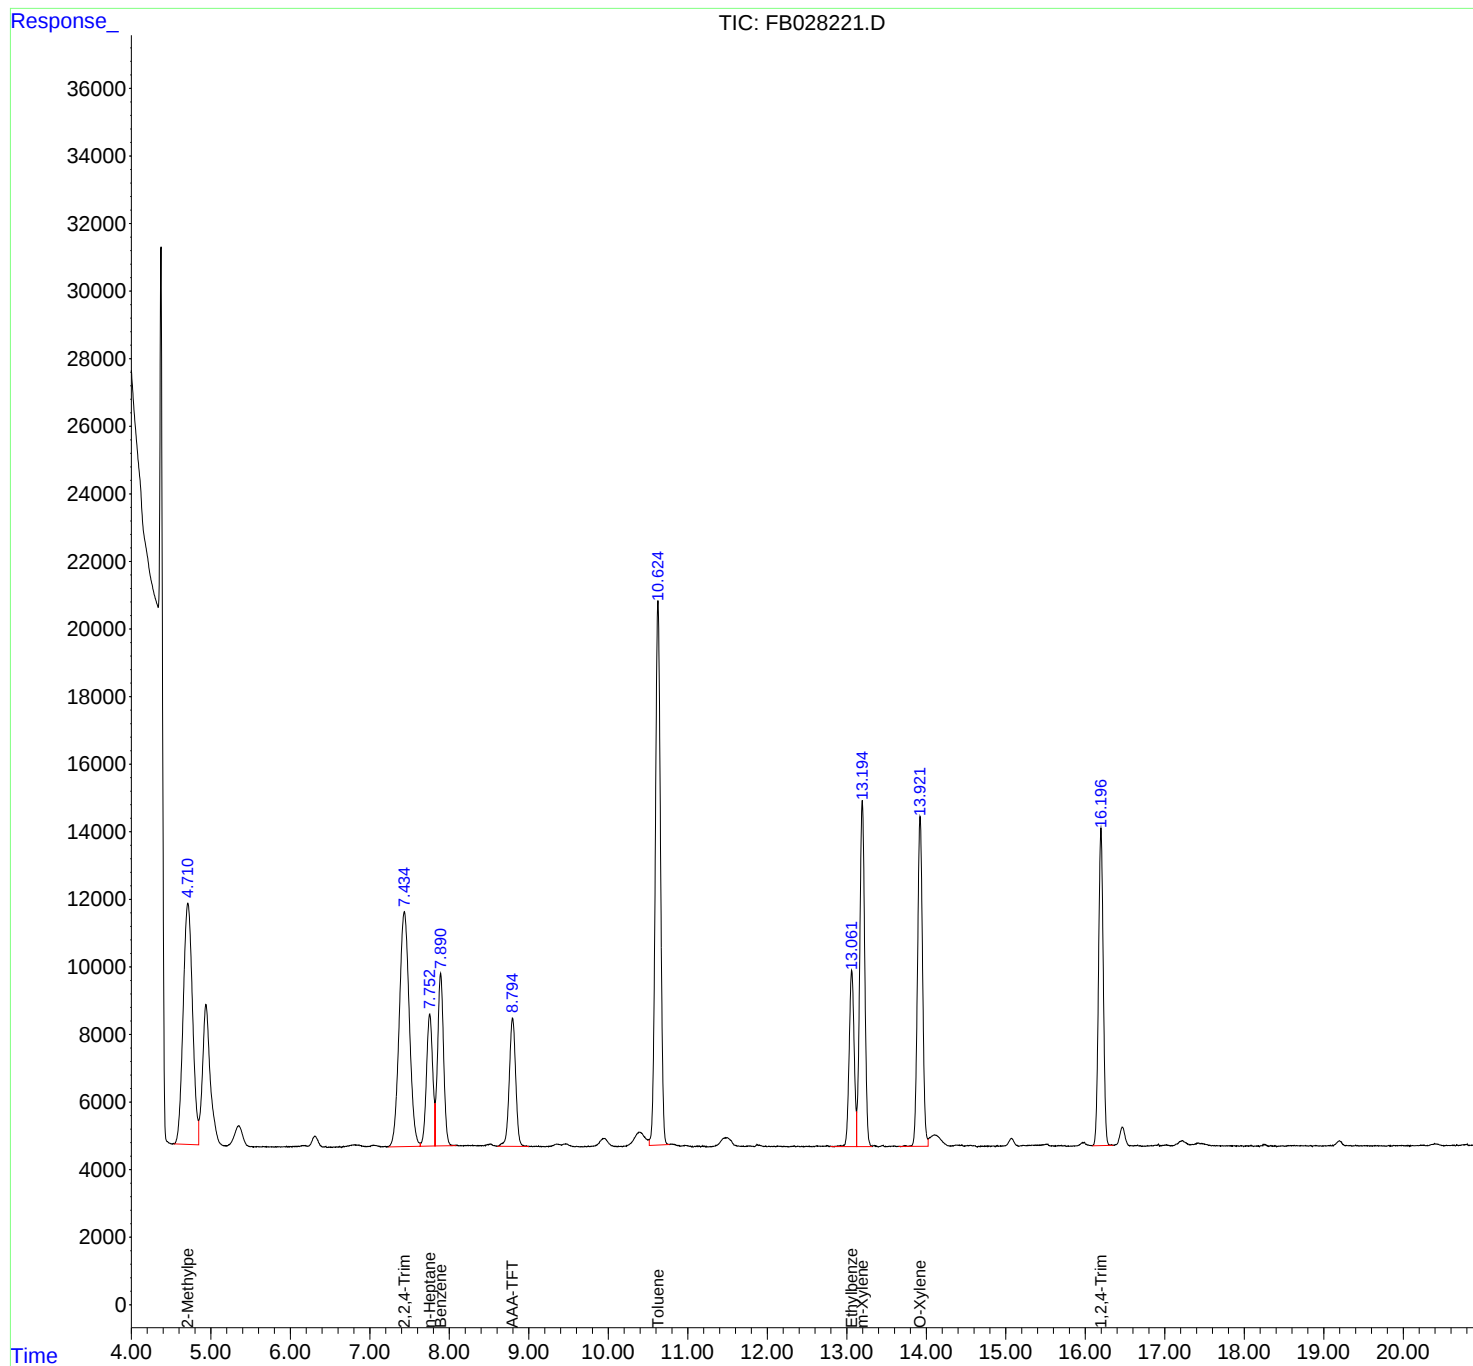


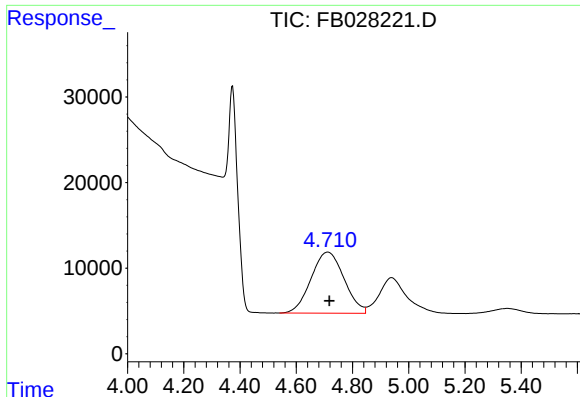

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: -0.006 min
Response: 582588
Conc: 28.77 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-21-COMPMS

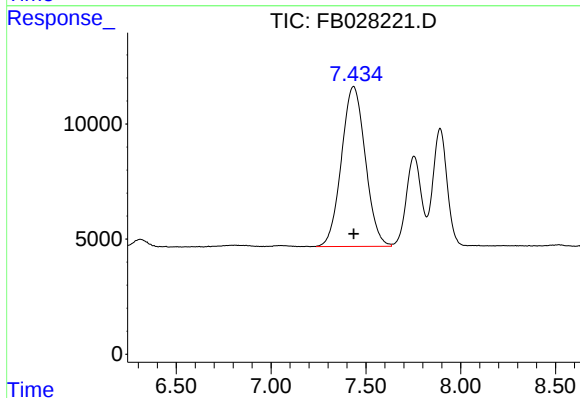


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: -0.002 min
Response: 607775
Conc: 28.89 ng/ml

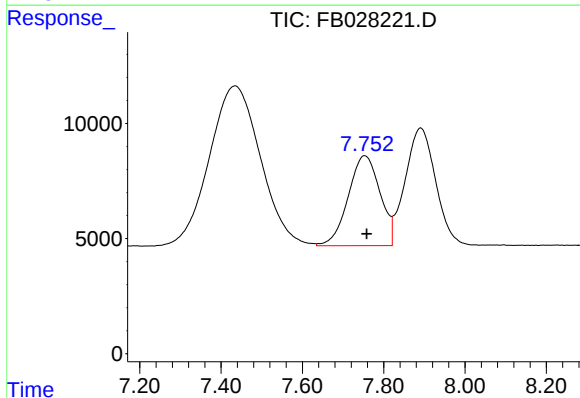


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.005 min
Response: 212235
Conc: 9.87 ng/ml

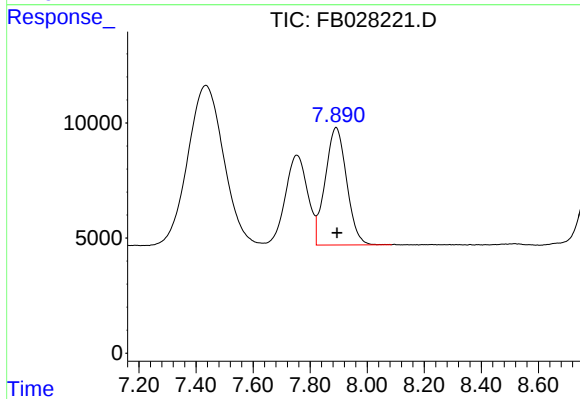

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.003 min
Response: 266108
Conc: 10.82 ng/ml

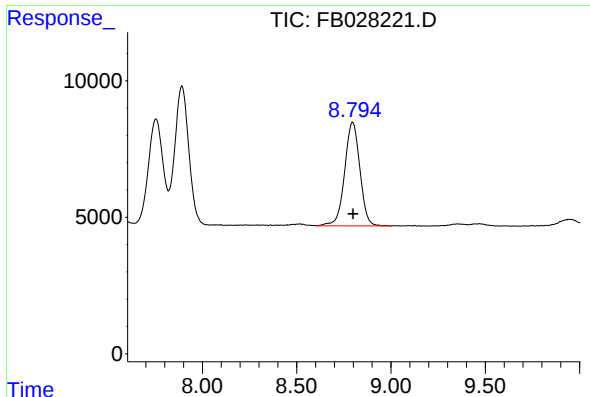

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 213003
Conc: 17.80 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-21-COMPMS

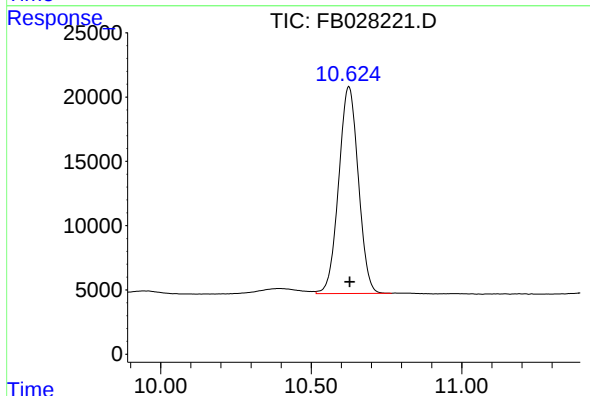


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.003 min
Response: 728441
Conc: 31.29 ng/ml

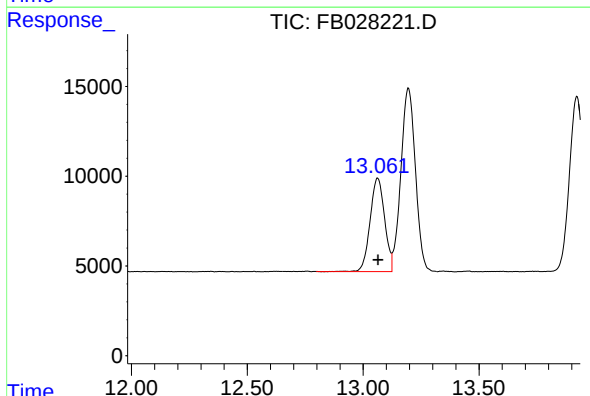


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.002 min
Response: 226982
Conc: 10.21 ng/ml

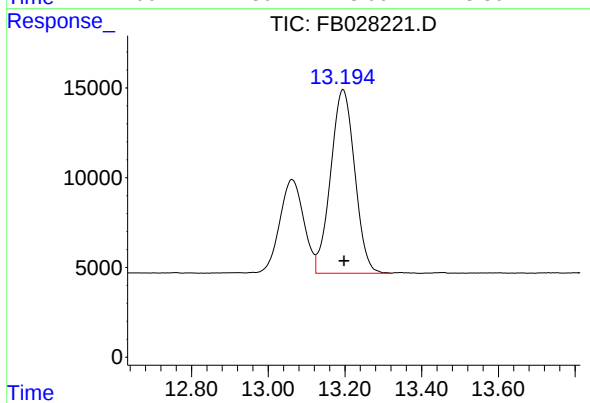

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: -0.002 min
Response: 446113
Conc: 20.44 ng/ml

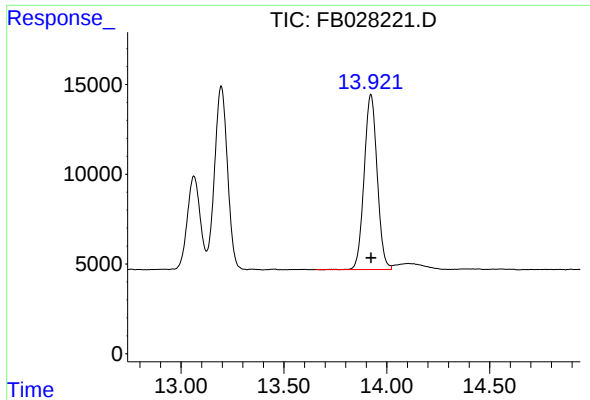

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: -0.001 min
Response: 429831
Conc: 20.52 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-21-COMPMS

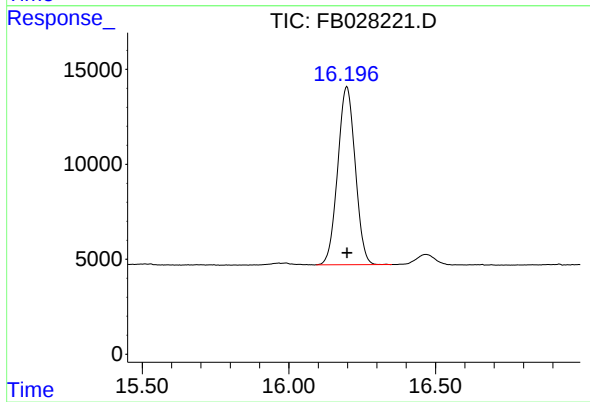

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: -0.001 min
Response: 389048
Conc: 19.35 ng/ml