

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090922\
 Data File : FB028222.D
 Signal(s) : FID2B.CH
 Acq On : 9 Sep 2022 16:56
 Operator : AJ/MA
 Sample : N4530-10MSD
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-21-COMPMSD

Integration File: Calibration.e
 Quant Time: Sep 12 01:41:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	200207	16.727 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	543130	26.825 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	577131	27.435 ng/ml
3) t n-Heptane	7.753	198276	9.224 ng/ml
4) t Benzene	7.891	253329	10.297 ng/ml
6) t Toluene	10.625	688508	29.573 ng/ml
7) t Ethylbenzene	13.062	215243	9.679 ng/ml
8) t m-Xylene	13.195	422216	19.348 ng/ml
9) t O-Xylene	13.922	407880	19.467 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	372118	18.507 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090922\
Data File : FB028222.D
Signal(s) : FID2B.CH
Acq On : 9 Sep 2022 16:56
Operator : AJ/MA
Sample : N4530-10MSD
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-21-COMPMSD

Integration File: Calibration.e
Quant Time: Sep 12 01:41:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

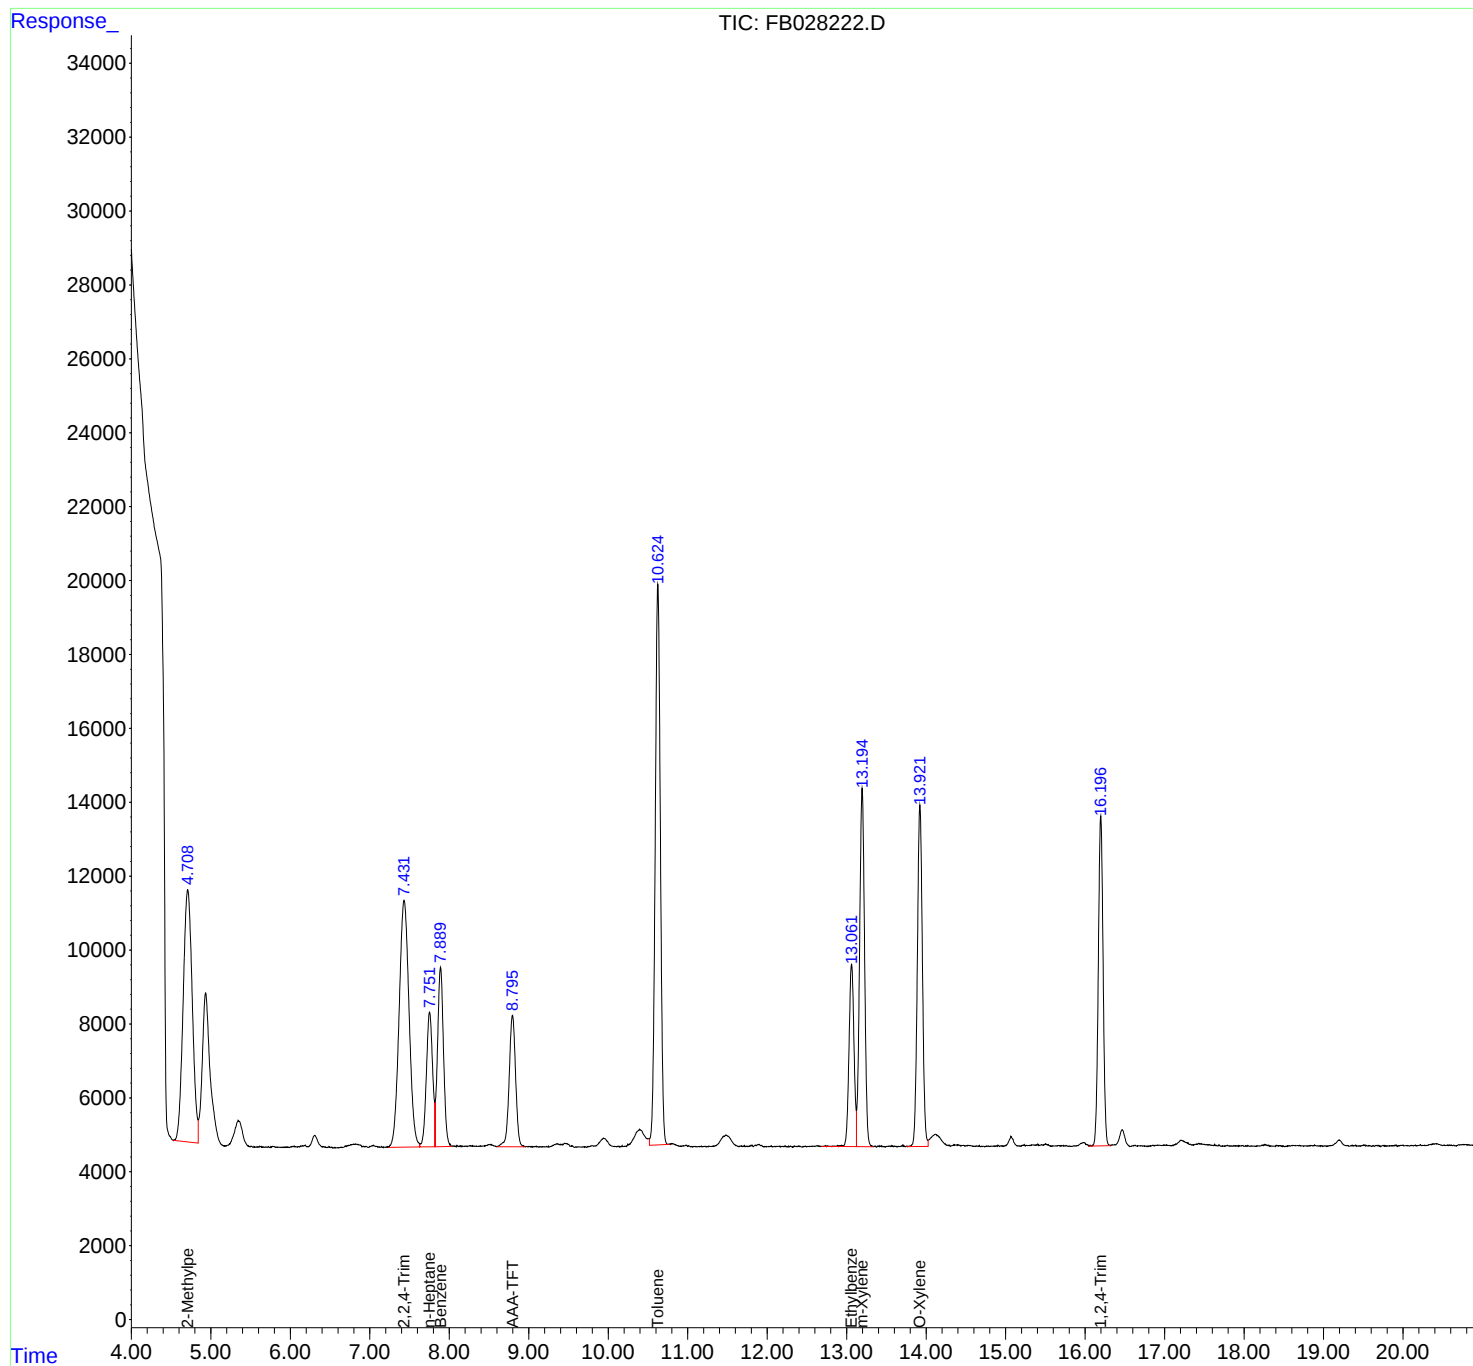


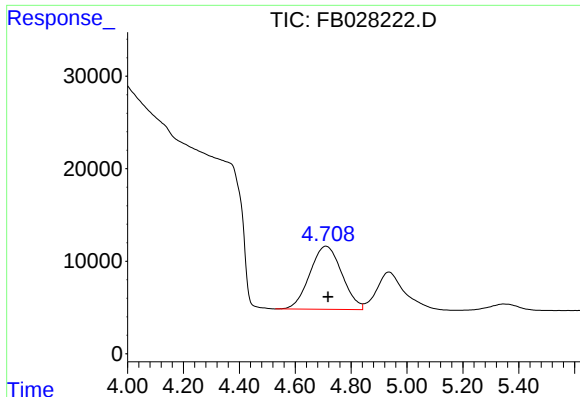

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: -0.008 min
Response: 543130
Conc: 26.83 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-21-COMPMSD

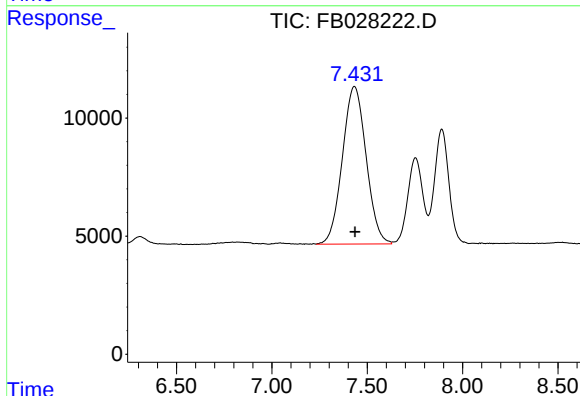


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
Delta R.T.: -0.005 min
Response: 577131
Conc: 27.44 ng/ml

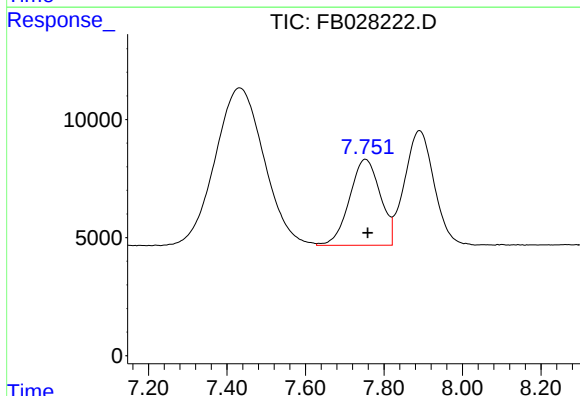


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.005 min
Response: 198276
Conc: 9.22 ng/ml

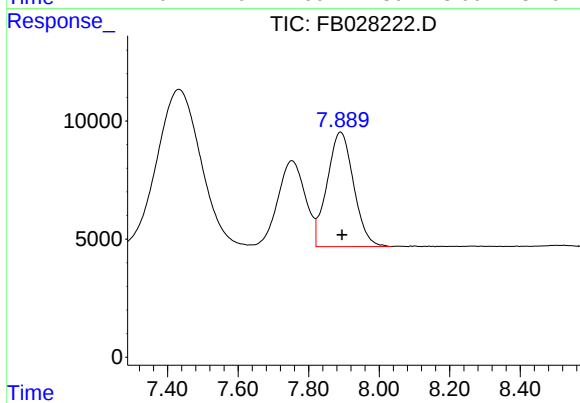

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.004 min
Response: 253329
Conc: 10.30 ng/ml

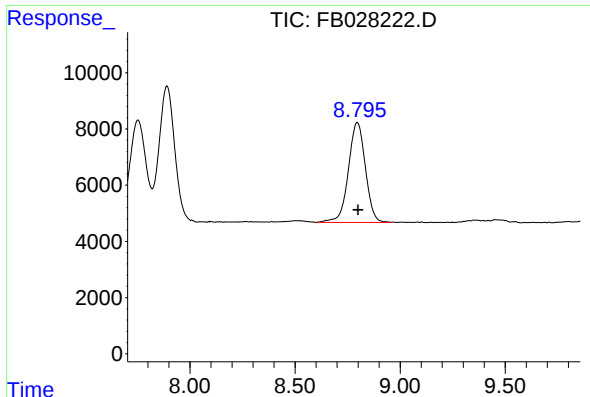

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 200207
Conc: 16.73 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-21-COMPMSD

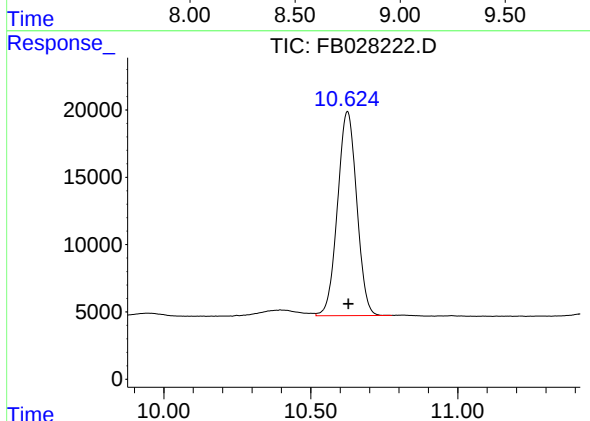


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.003 min
Response: 688508
Conc: 29.57 ng/ml

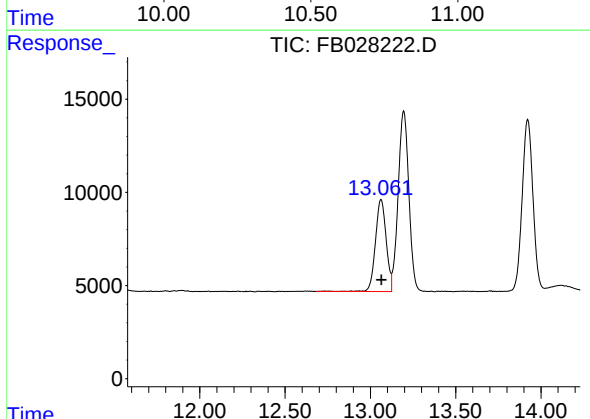


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.002 min
Response: 215243
Conc: 9.68 ng/ml

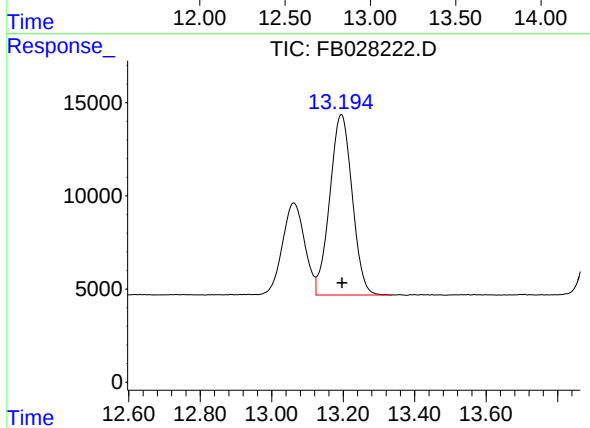

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: -0.002 min
Response: 422216
Conc: 19.35 ng/ml

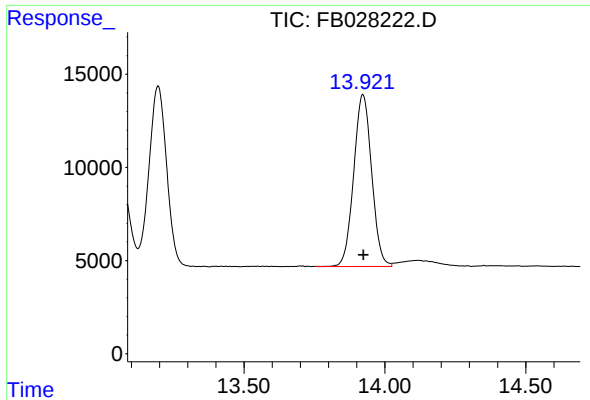

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.002 min
Response: 407880
Conc: 19.47 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-21-COMPMSD

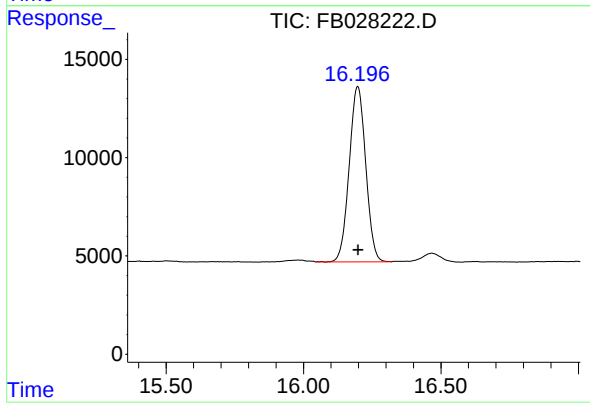

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: -0.001 min
Response: 372118
Conc: 18.51 ng/ml