Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090922\
Data File : FB028238.D
Signal(s) : FID2B.CH
Acq On : 10 Sep 2022 5:18
Operator : AJ/MA
Sample : N4530-14 50X
Misc : 5.02G/5.00 ML MEOH
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-23-COMP

Integration File: Calibration.e
Quant Time: Sep 12 01:43:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units
System Monitoring Compounds				
5) s	AAA-TFT	8.792	248961	20.801 ng/ml
Target Compounds				

(f)=RT Delta > 1/2 Window (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090922\
Data File : FB028238.D
Signal(s) : FID2B.CH
Acq On : 10 Sep 2022 5:18
Operator : AJ/MA
Sample : N4530-14 50X
Misc : 5.02G/5.00 ML MEOH
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-23-COMP

Integration File: Calibration.e
Quant Time: Sep 12 01:43:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

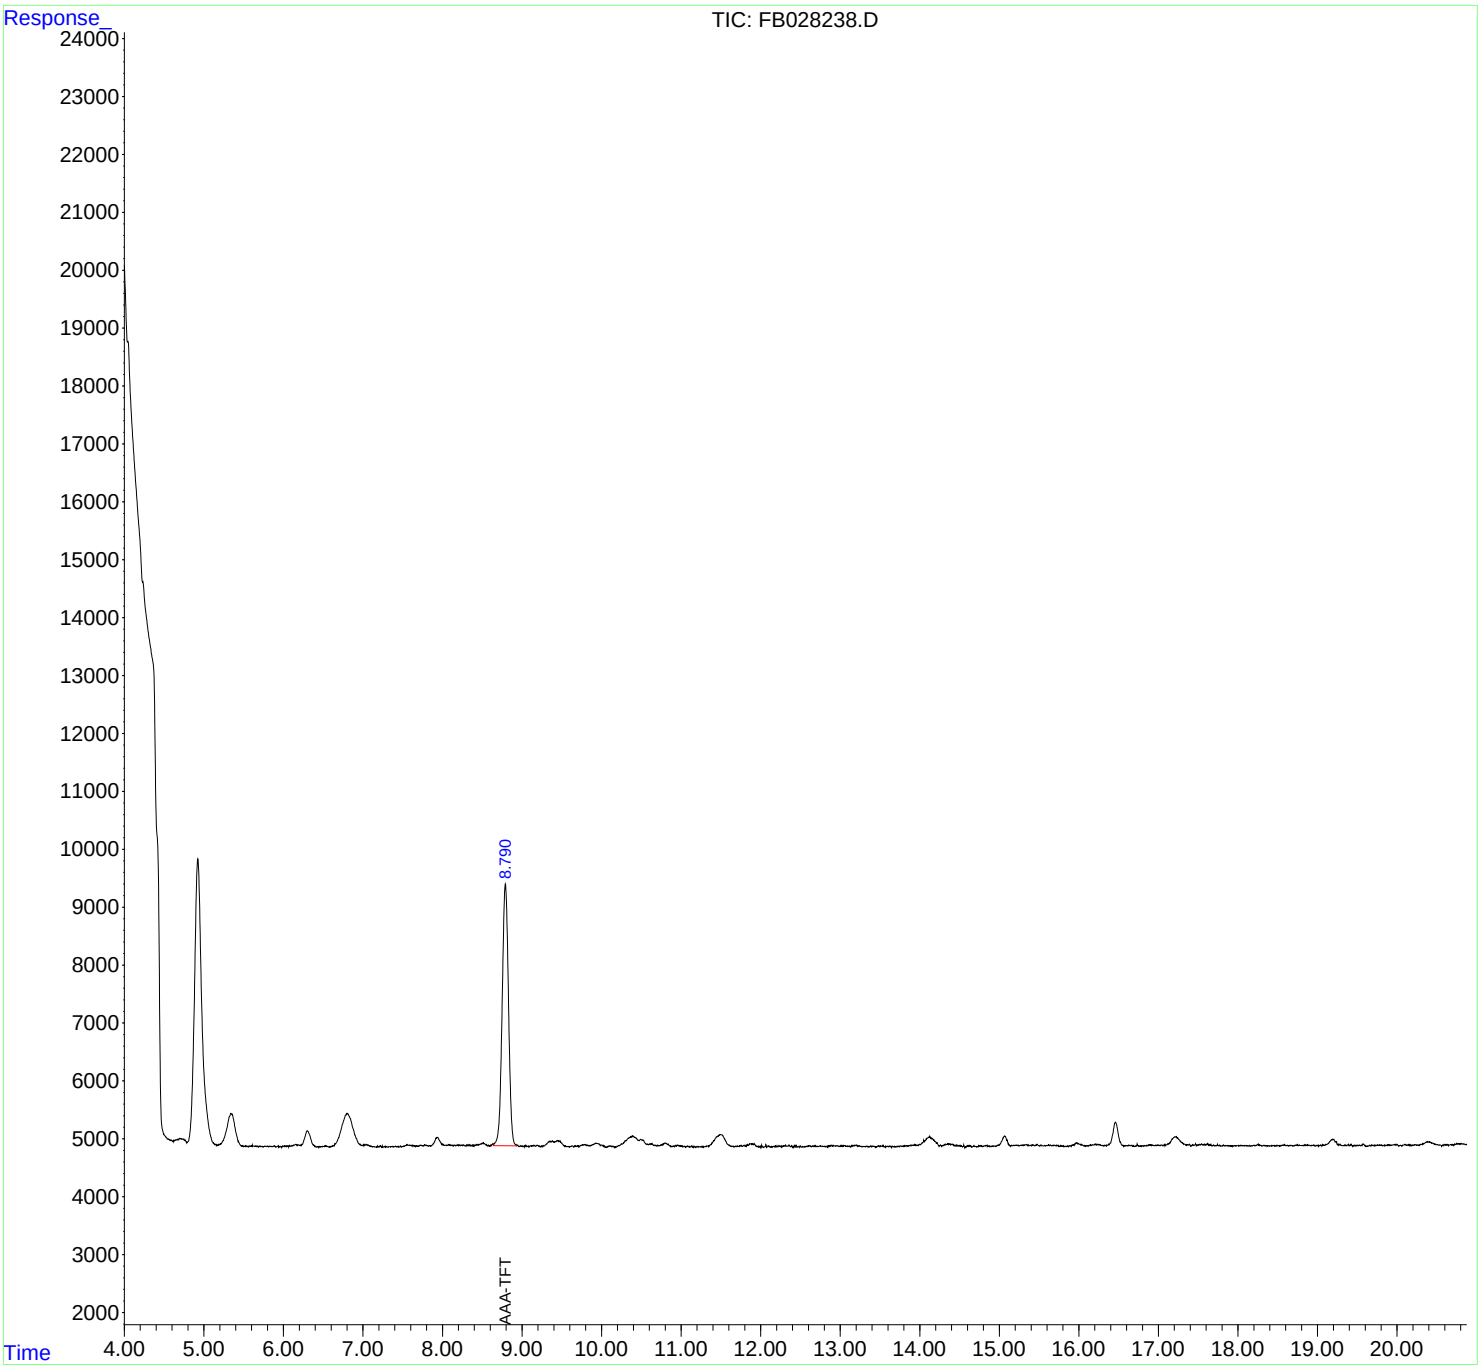

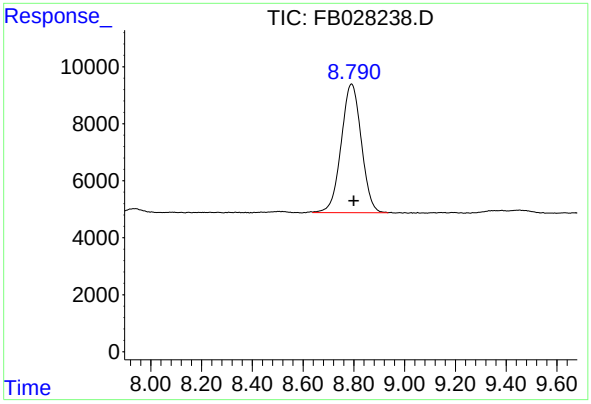

#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.008 min
Response: 248961
Conc: 20.80 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-23-COMP