

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091019\
 Data File : FB022416.D
 Signal(s) : FID2B.CH
 Acq On : 10 Sep 2019 8:58
 Operator : DD/AJ
 Sample : BSF0910S1
 Misc : 5.01g/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 11 03:53:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.967	544307	18.713 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.834	1076434	21.909 ng/ml
2) t 2,2,4-Trimethylpentane	7.586	1221454	23.654 ng/ml
3) t n-Heptane	7.925	403204	8.011 ng/ml
4) t Benzene	8.060	483468	8.146 ng/ml
6) t Toluene	10.809	1394018	29.303 ng/ml
7) t Ethylbenzene	13.255	442260	14.752 ng/ml
8) t m-Xylene	13.388	867048	32.637 ng/ml
9) t O-Xylene	14.117	812256	33.481 ng/ml
10) t 1,2,4-Trimethylbenzene	16.397	550131	21.101 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091019\
Data File : FB022416.D
Signal(s) : FID2B.CH
Acq On : 10 Sep 2019 8:58
Operator : DD/AJ
Sample : BSF0910S1
Misc : 5.01g/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 11 03:53:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

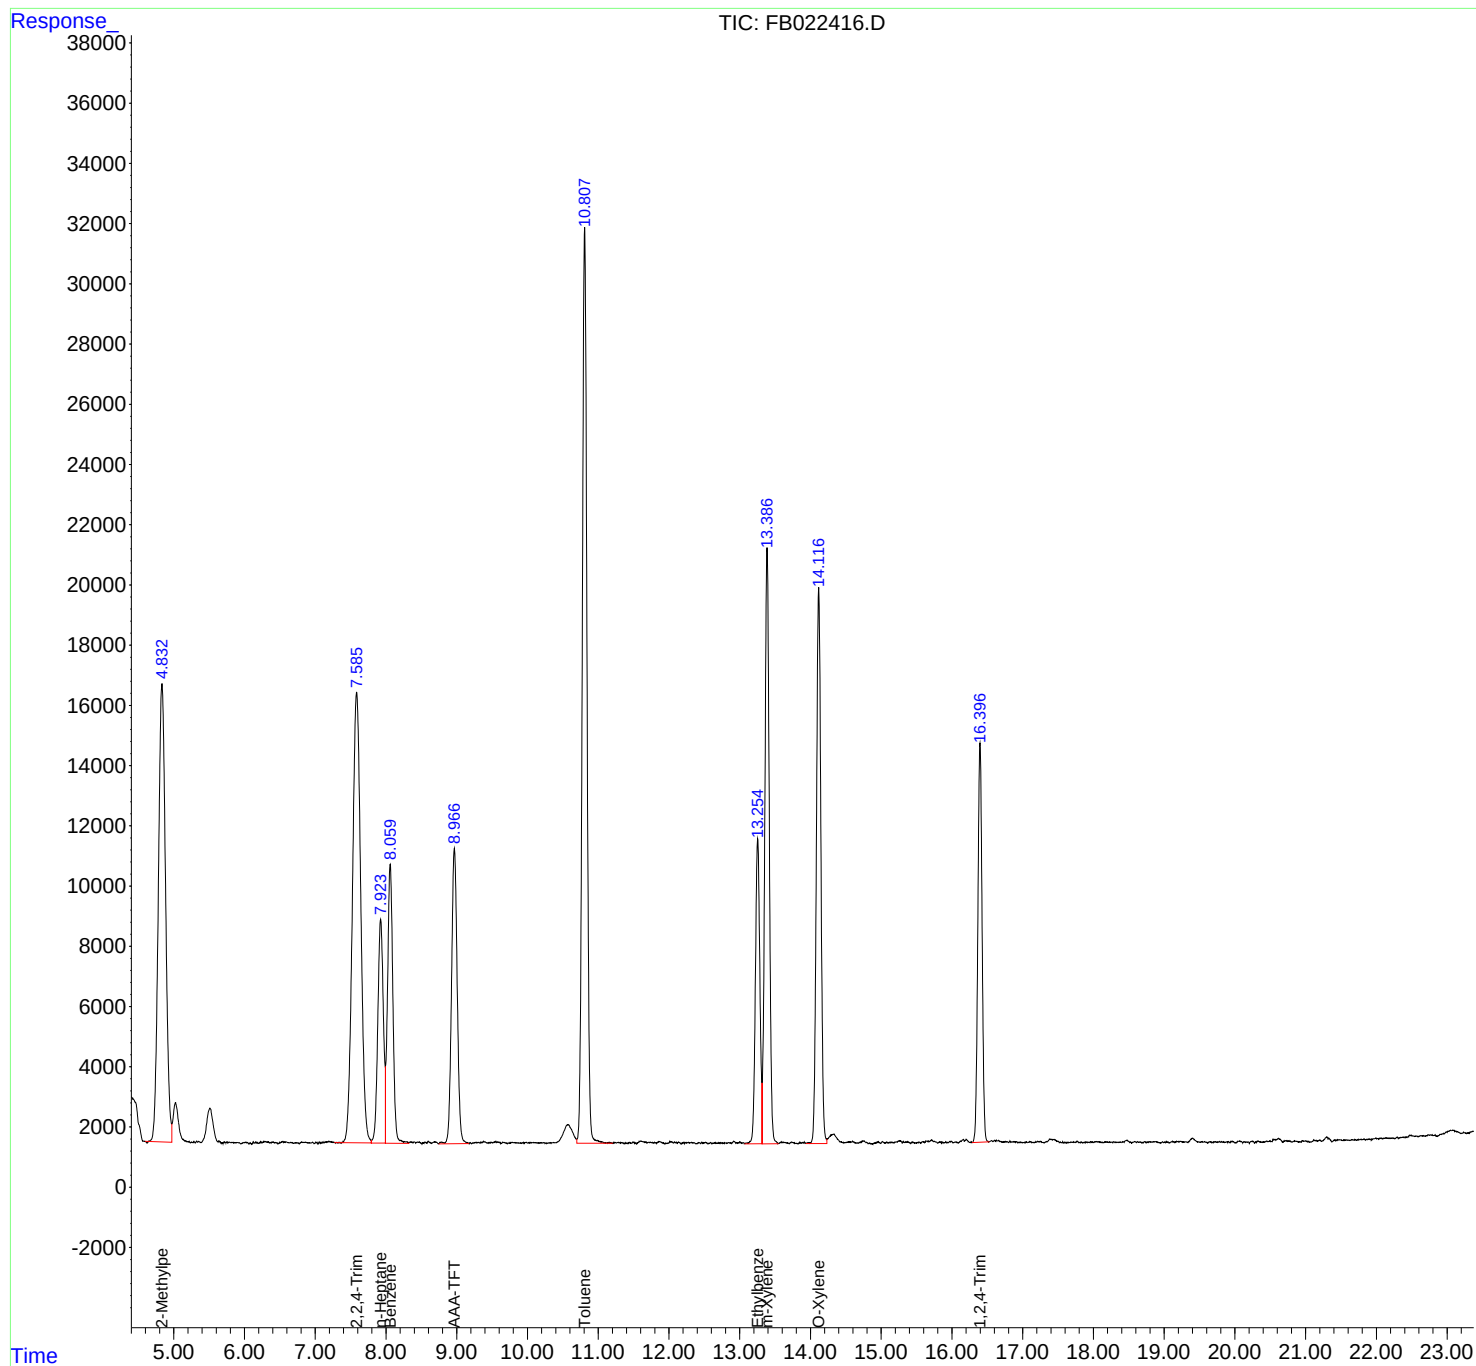

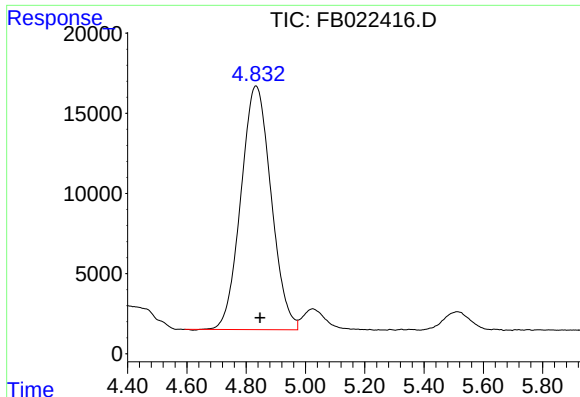


#1 2-Methylpentane

R.T.: 4.834 min
Delta R.T.: -0.013 min
Response: 1076434
Conc: 21.91 ng/ml

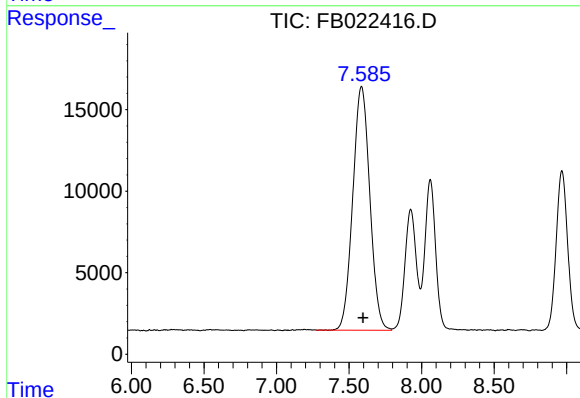


#2 2,2,4-Trimethylpentane

R.T.: 7.586 min
Delta R.T.: -0.012 min
Response: 1221454
Conc: 23.65 ng/ml

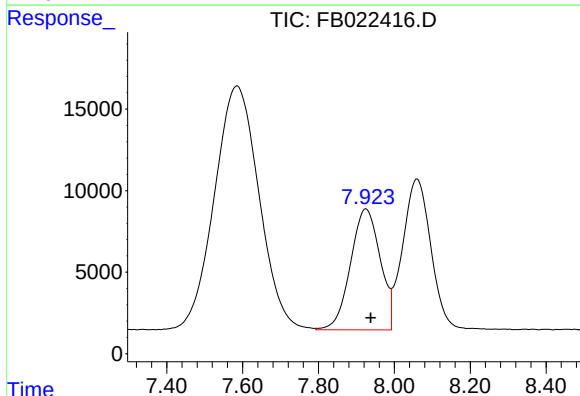


#3 n-Heptane

R.T.: 7.925 min
Delta R.T.: -0.012 min
Response: 403204
Conc: 8.01 ng/ml

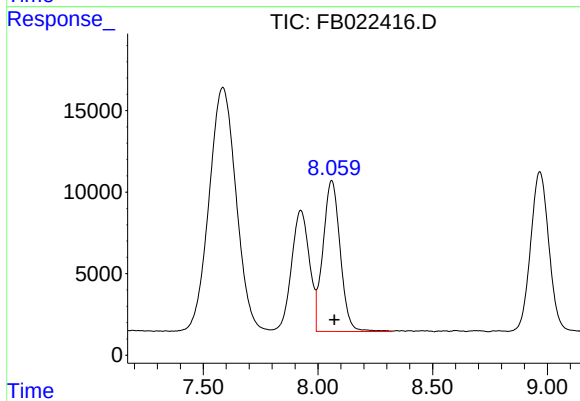


#4 Benzene

R.T.: 8.060 min
Delta R.T.: -0.012 min
Response: 483468
Conc: 8.15 ng/ml

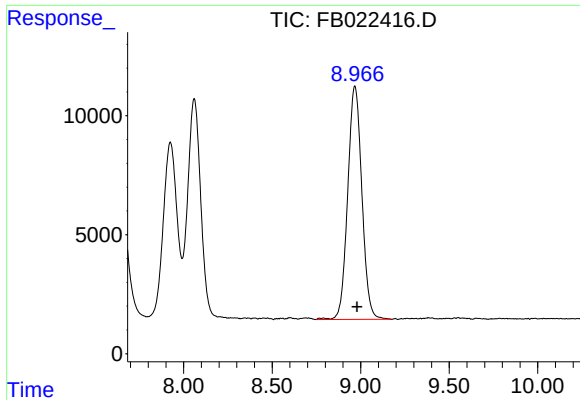


#5 AAA-TFT

R.T.: 8.967 min
 Delta R.T.: -0.012 min
 Response: 544307
 Conc: 18.71 ng/ml

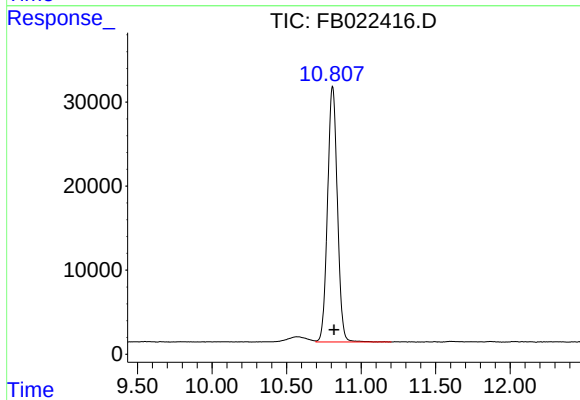


#6 Toluene

R.T.: 10.809 min
 Delta R.T.: -0.011 min
 Response: 1394018
 Conc: 29.30 ng/ml

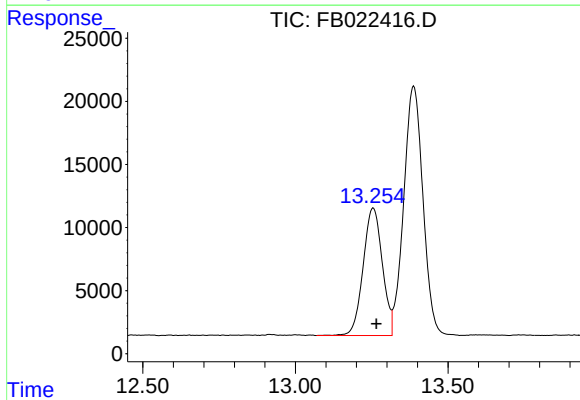


#7 Ethylbenzene

R.T.: 13.255 min
 Delta R.T.: -0.010 min
 Response: 442260
 Conc: 14.75 ng/ml

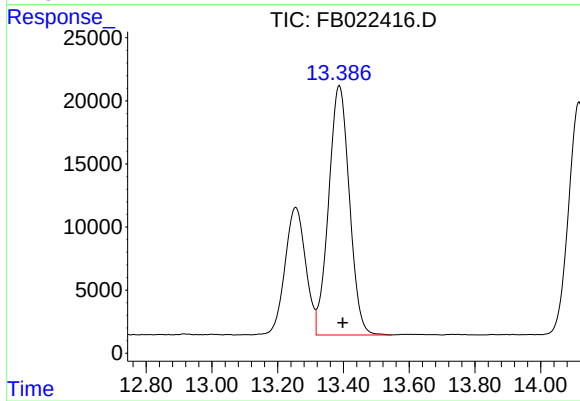

#8 m-Xylene

R.T.: 13.388 min
 Delta R.T.: -0.010 min
 Response: 867048
 Conc: 32.64 ng/ml

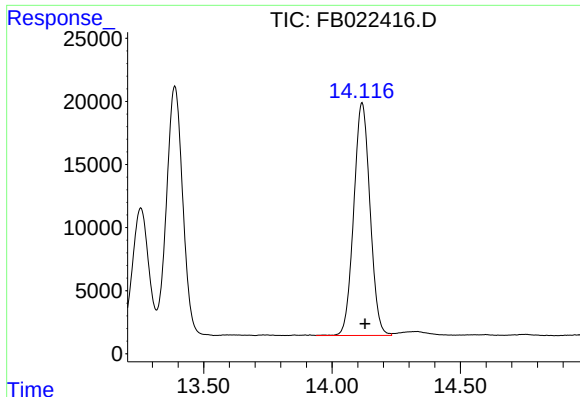


#9 O-Xylene

R.T.: 14.117 min

Delta R.T.: -0.011 min

Response: 812256

Conc: 33.48 ng/ml

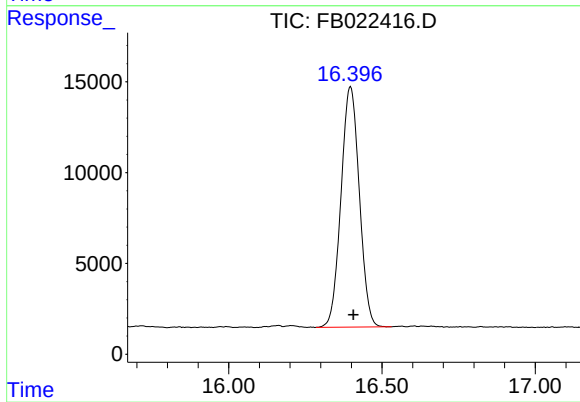

#10 1,2,4-Trimethylbenzene

R.T.: 16.397 min

Delta R.T.: -0.010 min

Response: 550131

Conc: 21.10 ng/ml