

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091019\
 Data File : FB022426.D
 Signal(s) : FID2B.CH
 Acq On : 10 Sep 2019 14:01
 Operator : DD/AJ
 Sample : K4787-02MS
 Misc : 5.02g/5.00ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 11 03:56:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.968	560465	19.268 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.835	1026058	20.883 ng/ml
2) t 2,2,4-Trimethylpentane	7.586	1191369	23.072 ng/ml
3) t n-Heptane	7.927	384873	7.647 ng/ml
4) t Benzene	8.062	472632	7.964 ng/ml
6) t Toluene	10.809	1369791	28.793 ng/ml
7) t Ethylbenzene	13.256	428370	14.289 ng/ml
8) t m-Xylene	13.388	838243	31.553 ng/ml
9) t O-Xylene	14.118	784075	32.320 ng/ml
10) t 1,2,4-Trimethylbenzene	16.398	525278	20.148 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091019\
Data File : FB022426.D
Signal(s) : FID2B.CH
Acq On : 10 Sep 2019 14:01
Operator : DD/AJ
Sample : K4787-02MS
Misc : 5.02g/5.00ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 11 03:56:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

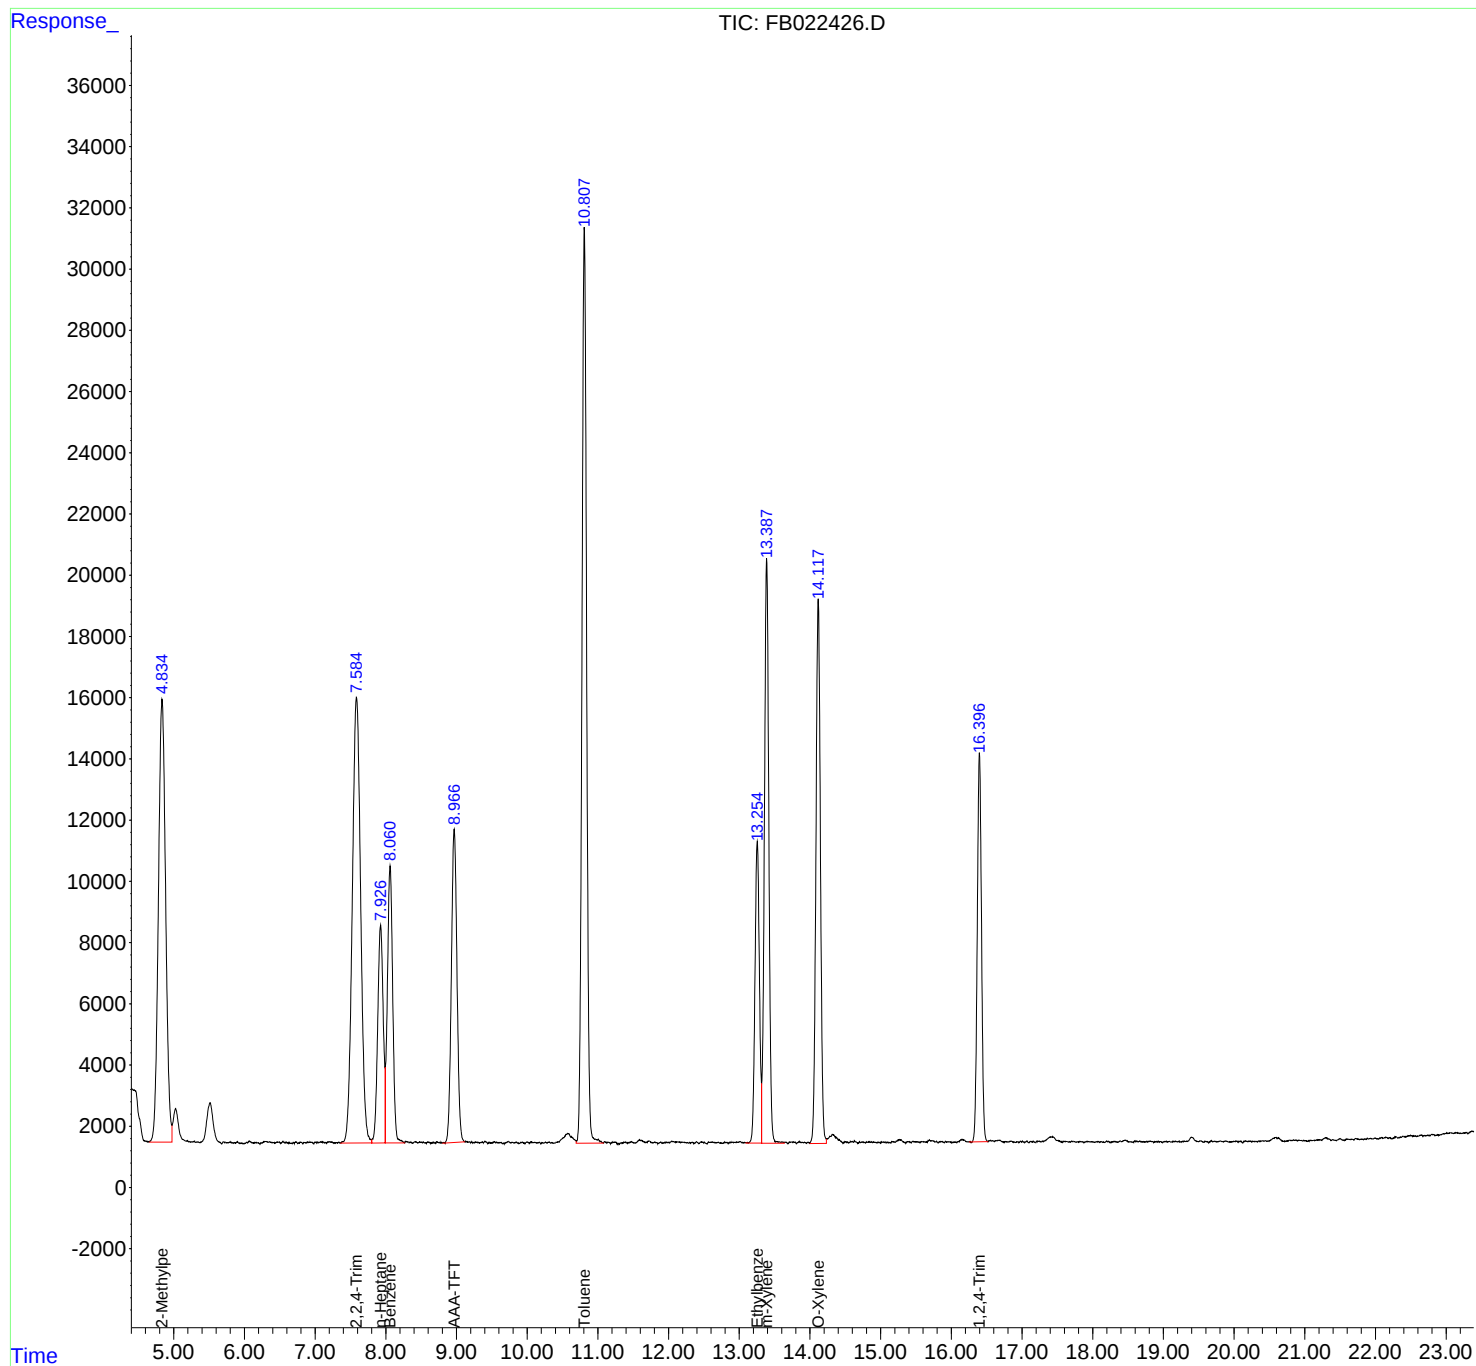

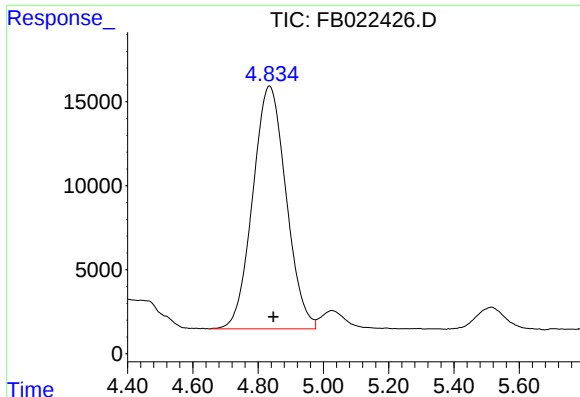


#1 2-Methylpentane

R.T.: 4.835 min
Delta R.T.: -0.012 min
Response: 1026058
Conc: 20.88 ng/ml

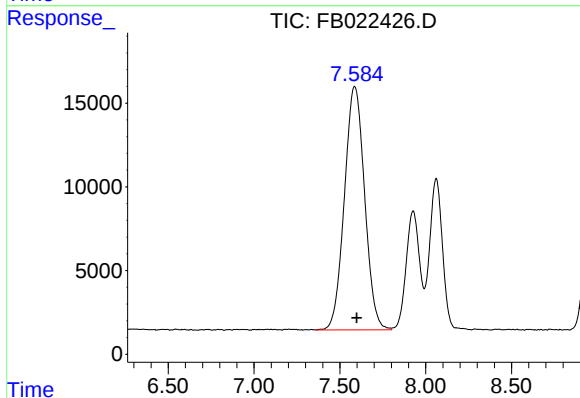


#2 2,2,4-Trimethylpentane

R.T.: 7.586 min
Delta R.T.: -0.012 min
Response: 1191369
Conc: 23.07 ng/ml

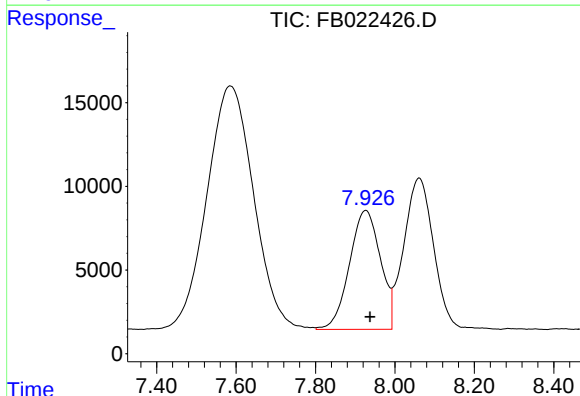


#3 n-Heptane

R.T.: 7.927 min
Delta R.T.: -0.011 min
Response: 384873
Conc: 7.65 ng/ml

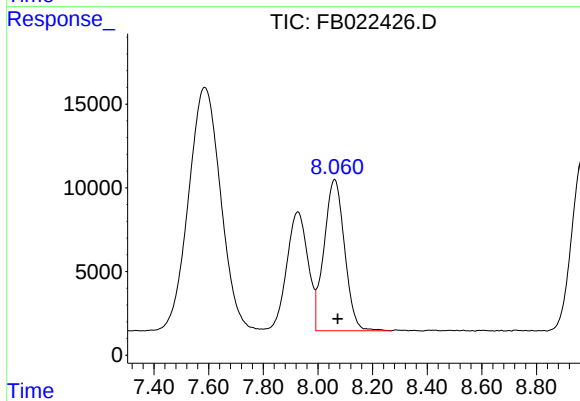


#4 Benzene

R.T.: 8.062 min
Delta R.T.: -0.011 min
Response: 472632
Conc: 7.96 ng/ml

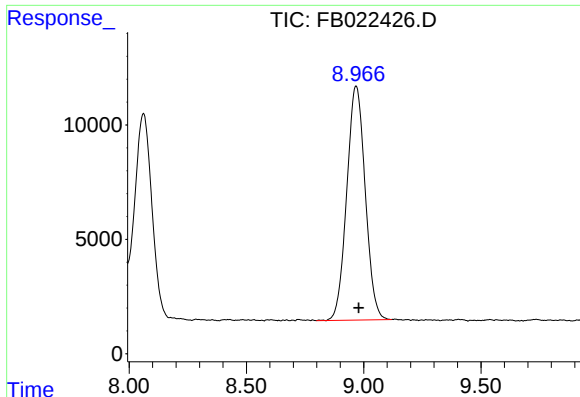


#5 AAA-TFT

R.T.: 8.968 min
Delta R.T.: -0.011 min
Response: 560465
Conc: 19.27 ng/ml

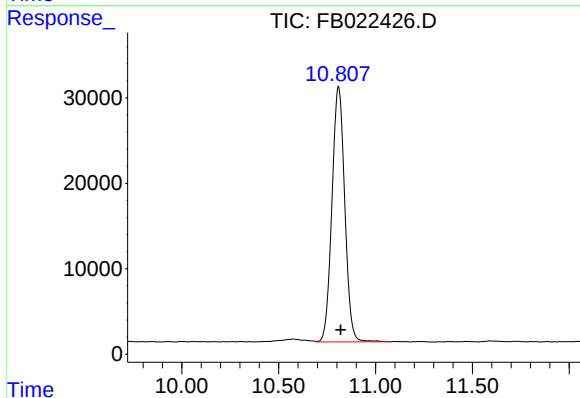


#6 Toluene

R.T.: 10.809 min
Delta R.T.: -0.011 min
Response: 1369791
Conc: 28.79 ng/ml

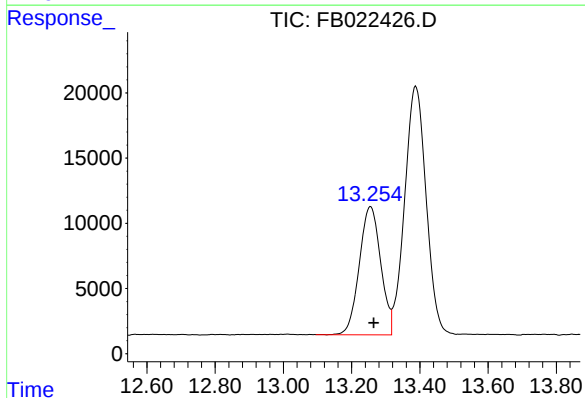


#7 Ethylbenzene

R.T.: 13.256 min
Delta R.T.: -0.010 min
Response: 428370
Conc: 14.29 ng/ml

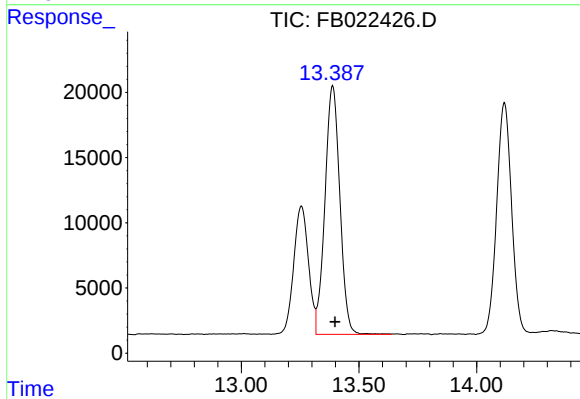


#8 m-Xylene

R.T.: 13.388 min
Delta R.T.: -0.010 min
Response: 838243
Conc: 31.55 ng/ml

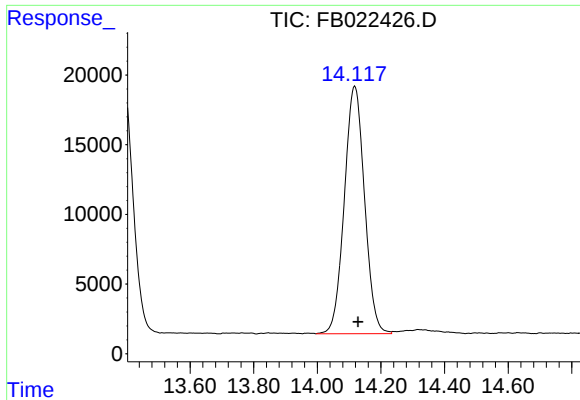

#9 O-Xylene

R.T.: 14.118 min
Delta R.T.: -0.010 min
Response: 784075
Conc: 32.32 ng/ml

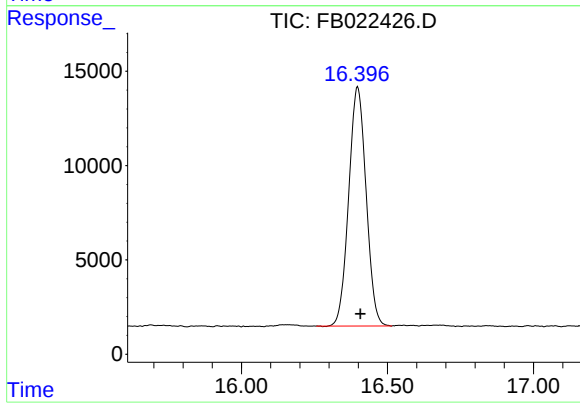

#10 1,2,4-Trimethylbenzene

R.T.: 16.398 min
Delta R.T.: -0.009 min
Response: 525278
Conc: 20.15 ng/ml