

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091019\
 Data File : FB022427.D
 Signal(s) : FID2B.CH
 Acq On : 10 Sep 2019 14:32
 Operator : DD/AJ
 Sample : K4787-02MSD
 Misc : 5.03g/5.00ML DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 11 03:56:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.968	564133	19.394 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.834	983127	20.009 ng/ml
2) t 2,2,4-Trimethylpentane	7.586	1150764	22.285 ng/ml
3) t n-Heptane	7.925	369602	7.344 ng/ml
4) t Benzene	8.061	467449	7.876 ng/ml
6) t Toluene	10.809	1360673	28.602 ng/ml
7) t Ethylbenzene	13.256	423304	14.120 ng/ml
8) t m-Xylene	13.388	837330	31.518 ng/ml
9) t O-Xylene	14.118	790309	32.577 ng/ml
10) t 1,2,4-Trimethylbenzene	16.398	515212	19.762 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091019\
Data File : FB022427.D
Signal(s) : FID2B.CH
Acq On : 10 Sep 2019 14:32
Operator : DD/AJ
Sample : K4787-02MSD
Misc : 5.03g/5.00ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 11 03:56:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

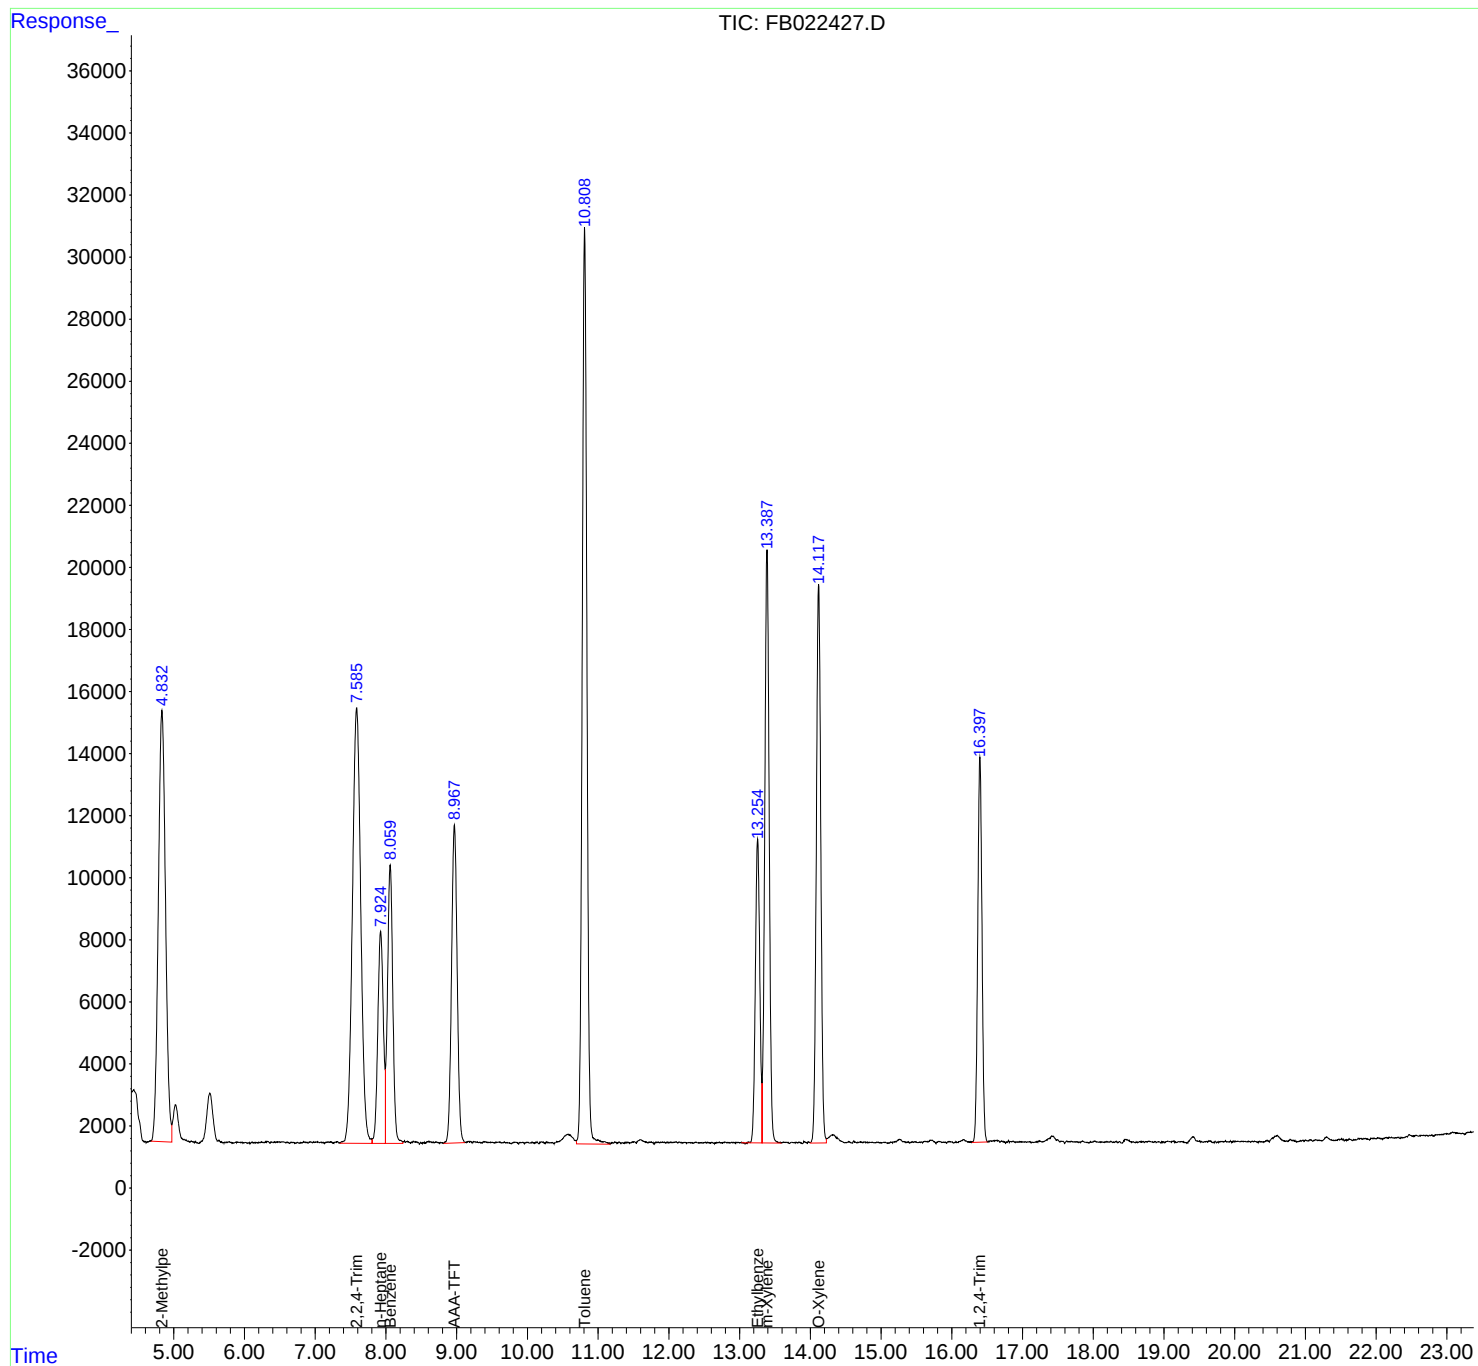

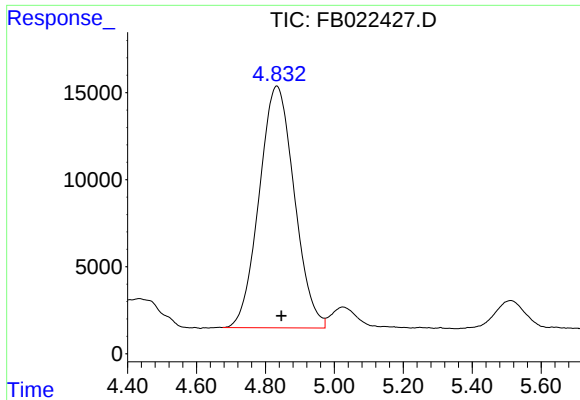


#1 2-Methylpentane

R.T.: 4.834 min
Delta R.T.: -0.013 min
Response: 983127
Conc: 20.01 ng/ml

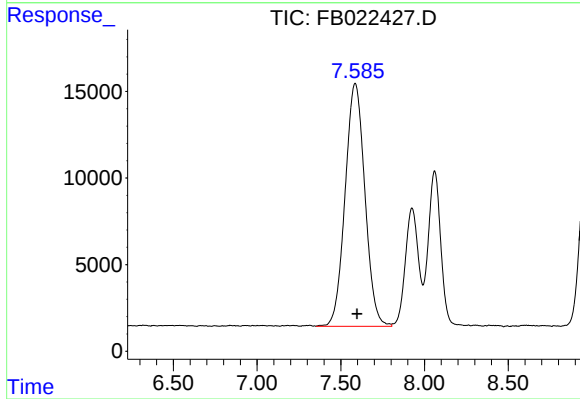


#2 2,2,4-Trimethylpentane

R.T.: 7.586 min
Delta R.T.: -0.012 min
Response: 1150764
Conc: 22.29 ng/ml

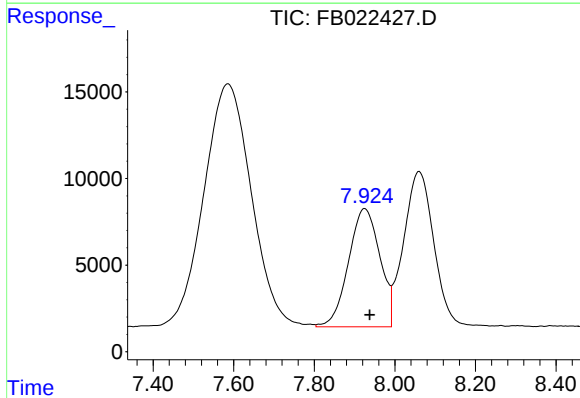


#3 n-Heptane

R.T.: 7.925 min
Delta R.T.: -0.012 min
Response: 369602
Conc: 7.34 ng/ml

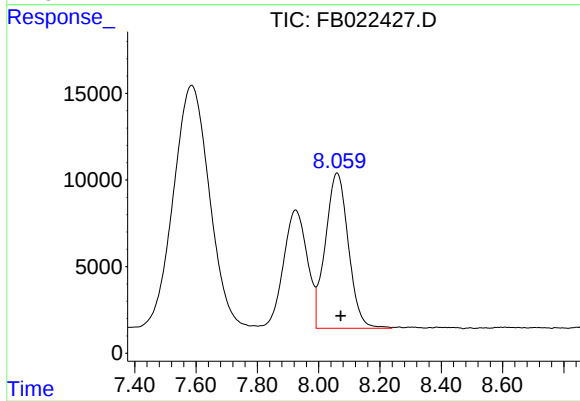


#4 Benzene

R.T.: 8.061 min
Delta R.T.: -0.012 min
Response: 467449
Conc: 7.88 ng/ml

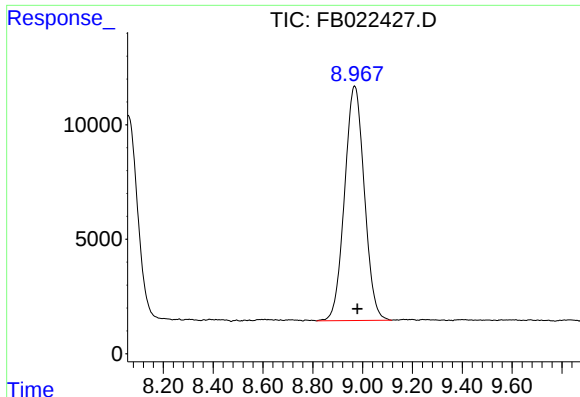


#5 AAA-TFT

R.T.: 8.968 min
Delta R.T.: -0.011 min
Response: 564133
Conc: 19.39 ng/ml

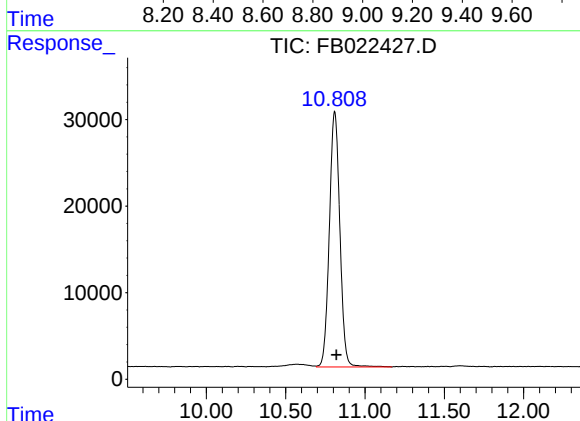


#6 Toluene

R.T.: 10.809 min
Delta R.T.: -0.011 min
Response: 1360673
Conc: 28.60 ng/ml

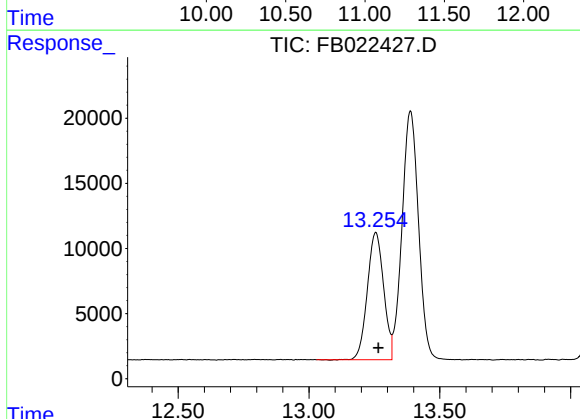


#7 Ethylbenzene

R.T.: 13.256 min
Delta R.T.: -0.010 min
Response: 423304
Conc: 14.12 ng/ml

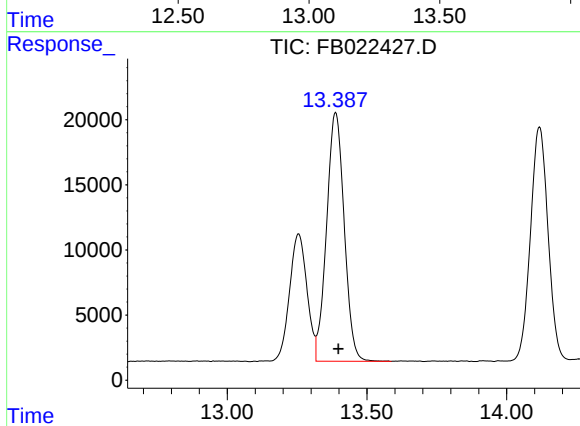


#8 m-Xylene

R.T.: 13.388 min
Delta R.T.: -0.010 min
Response: 837330
Conc: 31.52 ng/ml

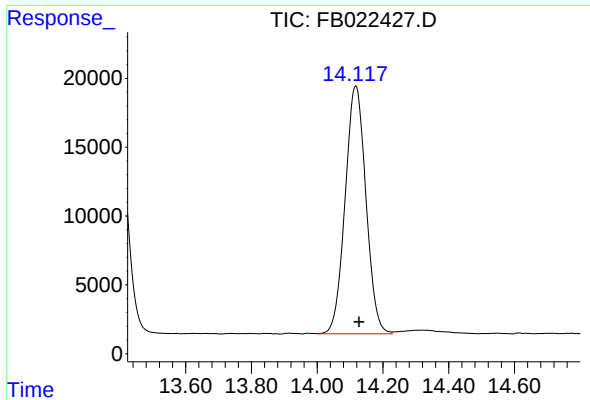

#9 O-Xylene

R.T.: 14.118 min
Delta R.T.: -0.010 min
Response: 790309
Conc: 32.58 ng/ml

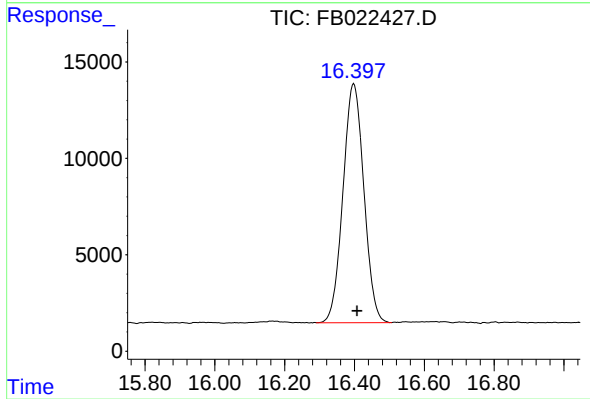

#10 1,2,4-Trimethylbenzene

R.T.: 16.398 min
Delta R.T.: -0.009 min
Response: 515212
Conc: 19.76 ng/ml