

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091019\
Data File : FB022432.D
Signal(s) : FID2B.CH
Acq On : 10 Sep 2019 17:03
Operator : DD/AJ
Sample : K4636-08
Misc : 5.28g/5.00ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 11 03:58:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.969	536685	18.451 ng/ml
Target Compounds			
6) t Toluene	10.805	5775	0.121 ng/ml
8) t m-Xylene	13.386	7207	0.271 ng/ml
9) t O-Xylene	14.119	6012	0.248 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091019\
Data File : FB022432.D
Signal(s) : FID2B.CH
Acq On : 10 Sep 2019 17:03
Operator : DD/AJ
Sample : K4636-08
Misc : 5.28g/5.00ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 11 03:58:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

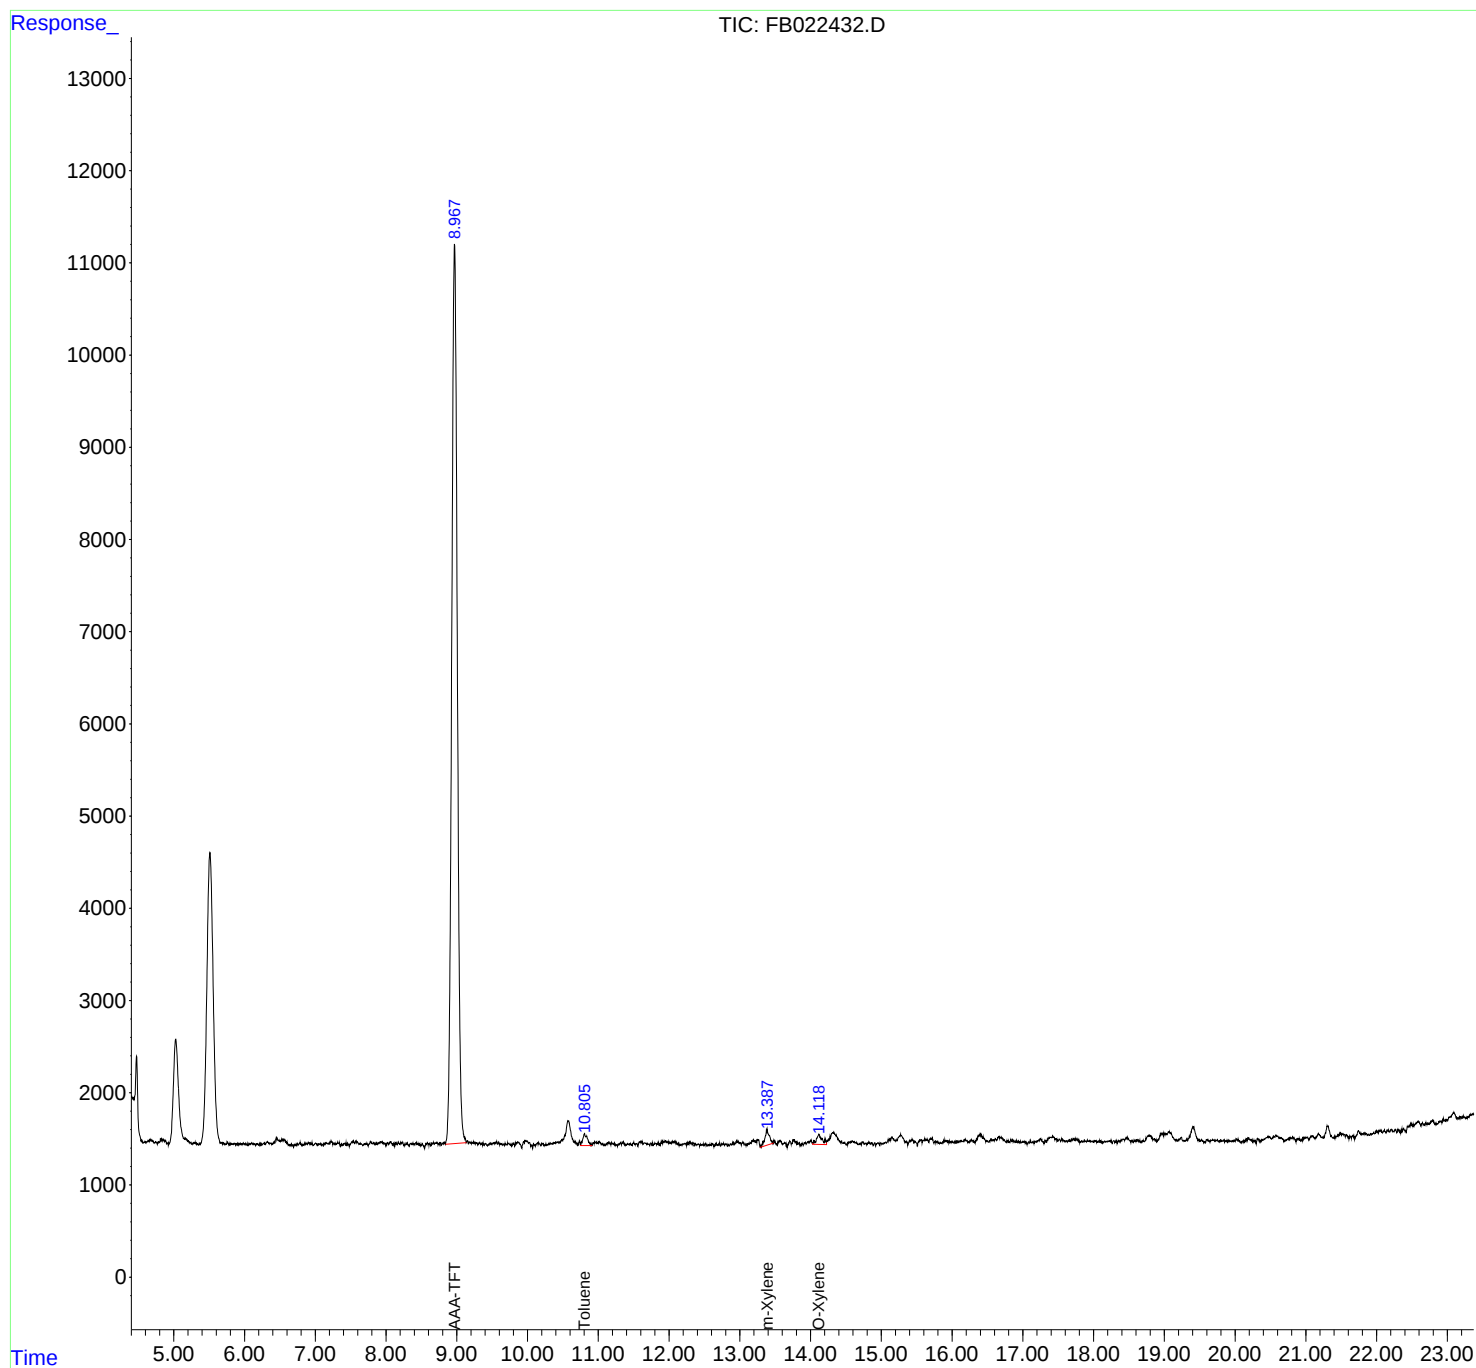

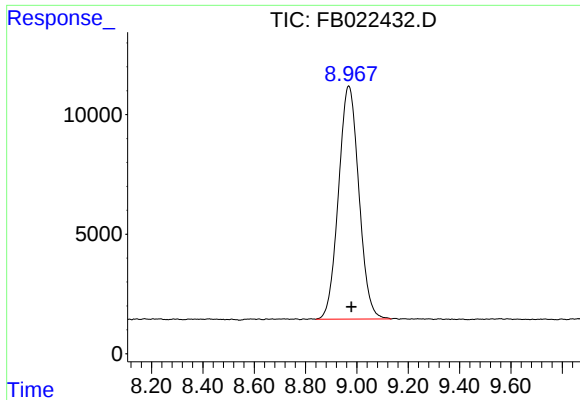


#5 AAA-TFT

R.T.: 8.969 min
Delta R.T.: -0.010 min
Response: 536685
Conc: 18.45 ng/ml

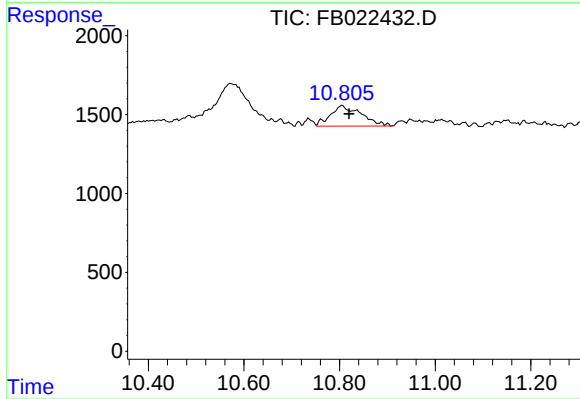


#6 Toluene

R.T.: 10.805 min
Delta R.T.: -0.014 min
Response: 5775
Conc: 0.12 ng/ml

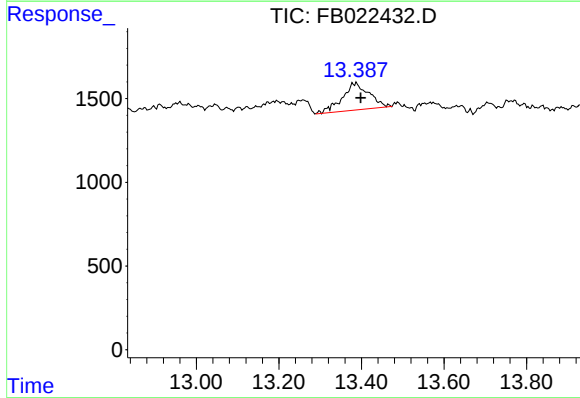

#8 m-Xylene

R.T.: 13.386 min
Delta R.T.: -0.012 min
Response: 7207
Conc: 0.27 ng/ml

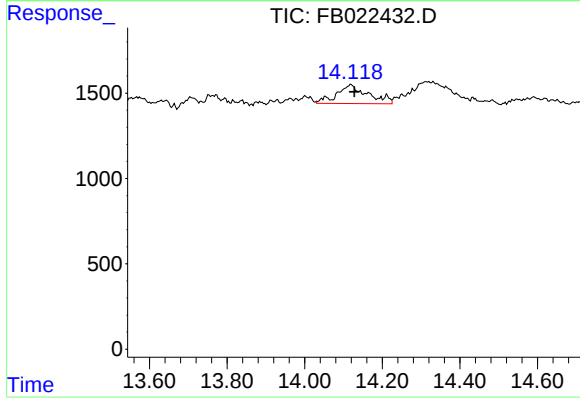

#9 O-Xylene

R.T.: 14.119 min
Delta R.T.: -0.009 min
Response: 6012
Conc: 0.25 ng/ml