

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091118\
 Data File : FB017659.D
 Signal(s) : FID2B.CH
 Acq On : 11 Sep 2018 11:26
 Operator : MJ/SJ
 Sample : BSF0911S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 12 08:53:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.110	177122	21.483 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.963	289233	20.641 ng/ml
2) t	2,2,4-Trimethylpentane	7.726	357703	25.383 ng/ml
3) t	n-Heptane	8.066	91360	6.629 ng/ml
4) t	Benzene	8.204	161698	9.171 ng/ml
6) t	Toluene	10.959	408632	28.405 ng/ml
7) t	Ethylbenzene	13.408	143885	9.757 ng/ml
8) t	m-Xylene	13.540	310281	19.960 ng/ml
9) t	O-Xylene	14.272	332630	20.263 ng/ml
10) t	1,2,4-Trimethylbenzene	16.555	389795	20.014 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091118\
Data File : FB017659.D
Signal(s) : FID2B.CH
Acq On : 11 Sep 2018 11:26
Operator : MJ/SJ
Sample : BSF0911S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 12 08:53:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

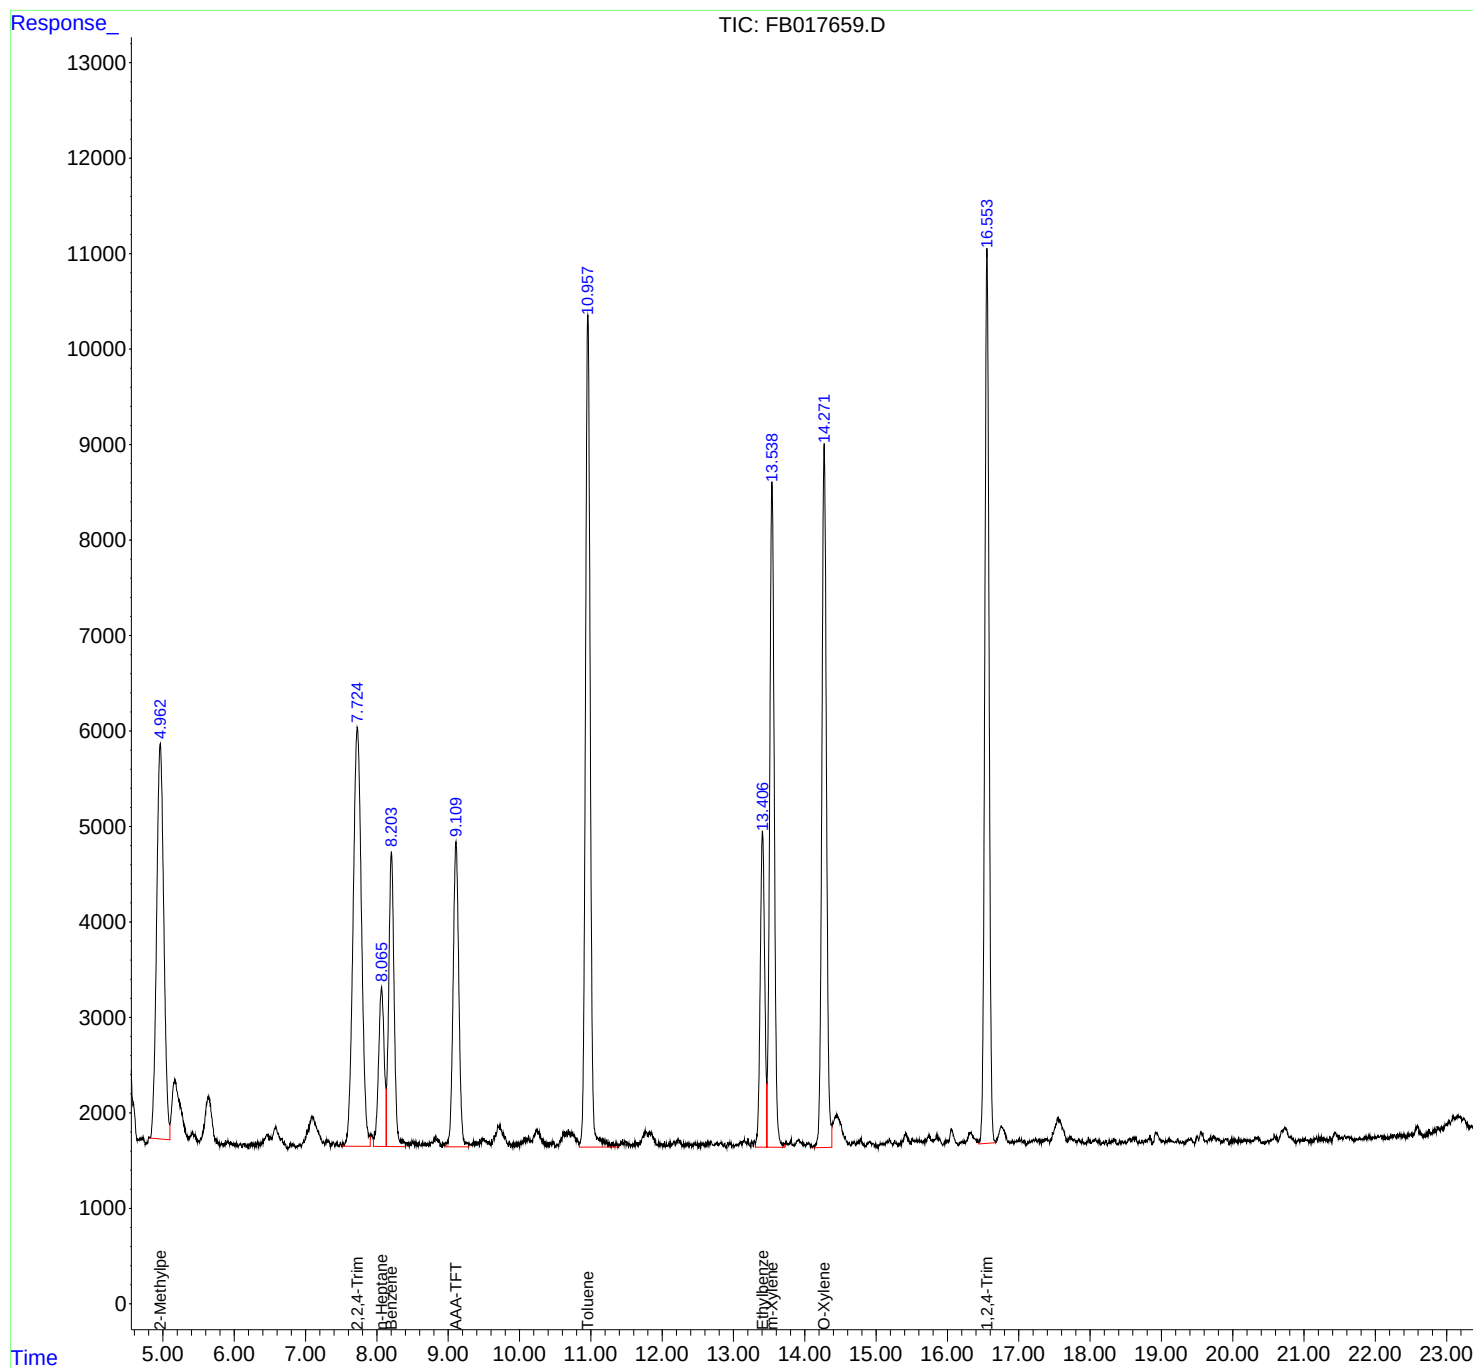

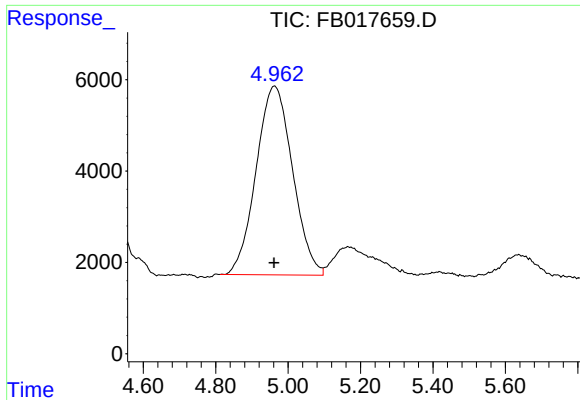


#1 2-Methylpentane

R.T.: 4.963 min
Delta R.T.: 0.002 min
Response: 289233
Conc: 20.64 ng/ml

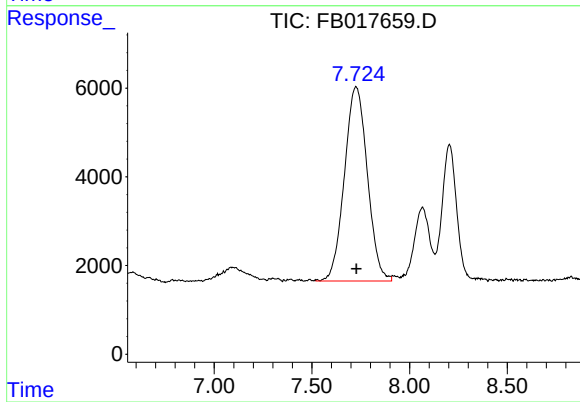


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: -0.001 min
Response: 357703
Conc: 25.38 ng/ml

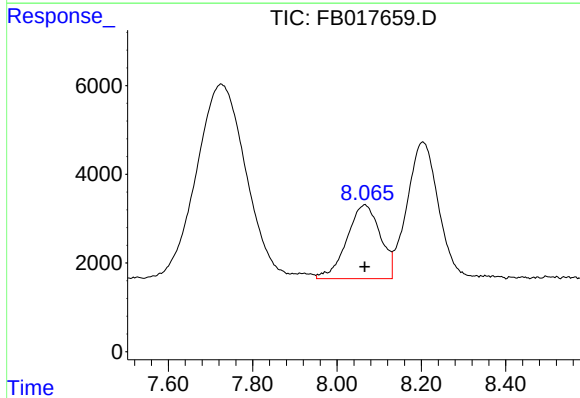


#3 n-Heptane

R.T.: 8.066 min
Delta R.T.: 0.000 min
Response: 91360
Conc: 6.63 ng/ml

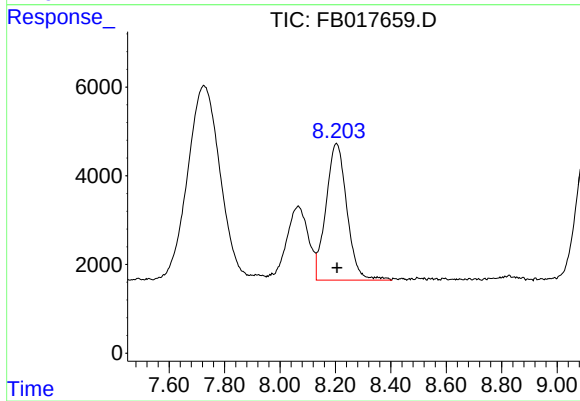


#4 Benzene

R.T.: 8.204 min
Delta R.T.: -0.001 min
Response: 161698
Conc: 9.17 ng/ml

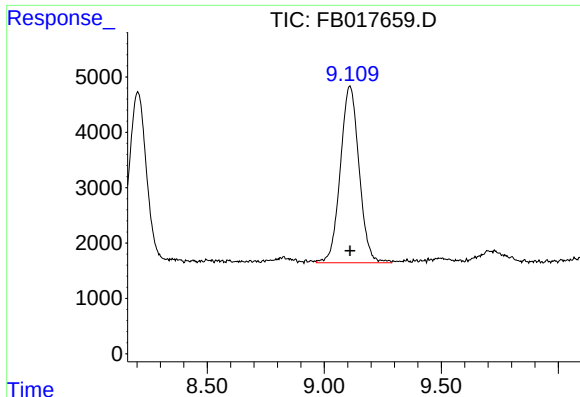


#5 AAA-TFT

R.T.: 9.110 min
Delta R.T.: -0.001 min
Response: 177122
Conc: 21.48 ng/ml

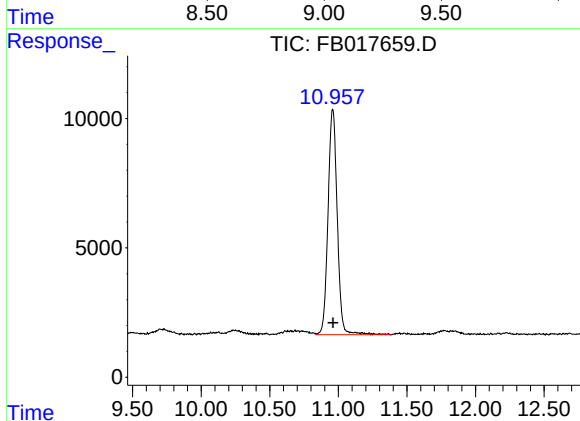


#6 Toluene

R.T.: 10.959 min
Delta R.T.: -0.001 min
Response: 408632
Conc: 28.41 ng/ml

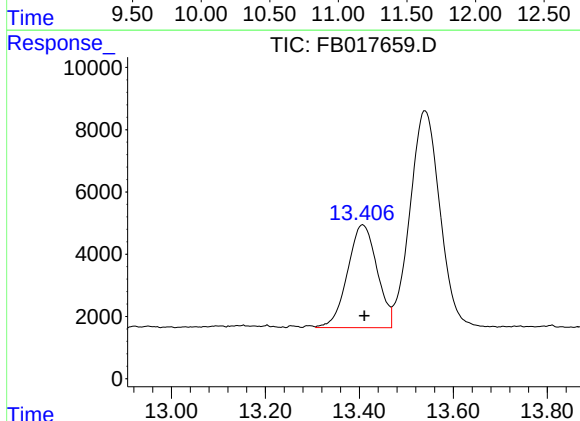


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: -0.003 min
Response: 143885
Conc: 9.76 ng/ml

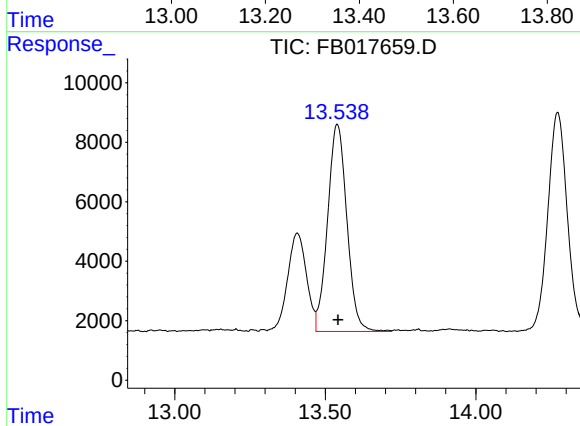


#8 m-Xylene

R.T.: 13.540 min
Delta R.T.: -0.002 min
Response: 310281
Conc: 19.96 ng/ml

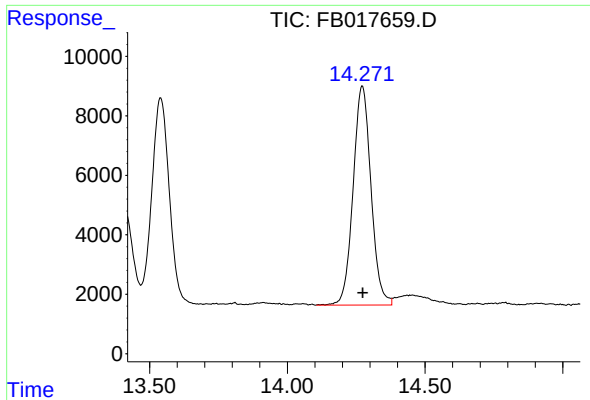

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: -0.002 min
Response: 332630
Conc: 20.26 ng/ml

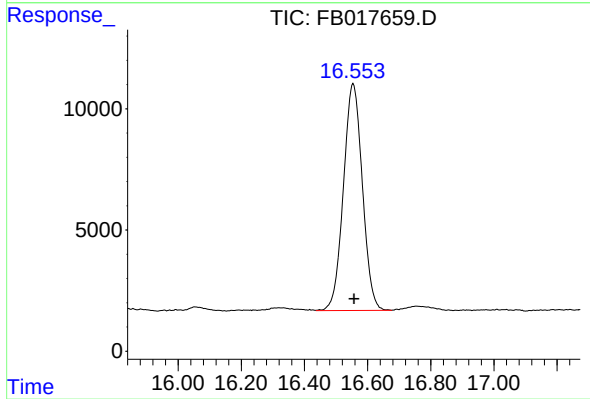

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: -0.003 min
Response: 389795
Conc: 20.01 ng/ml