

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091118\
 Data File : FB017680.D
 Signal(s) : FID2B.CH
 Acq On : 11 Sep 2018 22:43
 Operator : MJ/SJ
 Sample : J4845-01MS
 Misc : 5.05g/5.00mL DI Water
 ALS Vial : 24 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 12 08:54:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.109	160372	19.451 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.962	299331	21.362 ng/ml
2) t 2,2,4-Trimethylpentane	7.726	362898	25.752 ng/ml
3) t n-Heptane	8.064	85859	6.230 ng/ml
4) t Benzene	8.203	157703	8.945 ng/ml
6) t Toluene	10.957	391469	27.212 ng/ml
7) t Ethylbenzene	13.407	140345	9.517 ng/ml
8) t m-Xylene	13.540	296788	19.092 ng/ml
9) t O-Xylene	14.271	317753	19.357 ng/ml
10) t 1,2,4-Trimethylbenzene	16.555	372834	19.143 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091118\
Data File : FB017680.D
Signal(s) : FID2B.CH
Acq On : 11 Sep 2018 22:43
Operator : MJ/SJ
Sample : J4845-01MS
Misc : 5.05g/5.00mL DI Water
ALS Vial : 24 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 12 08:54:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

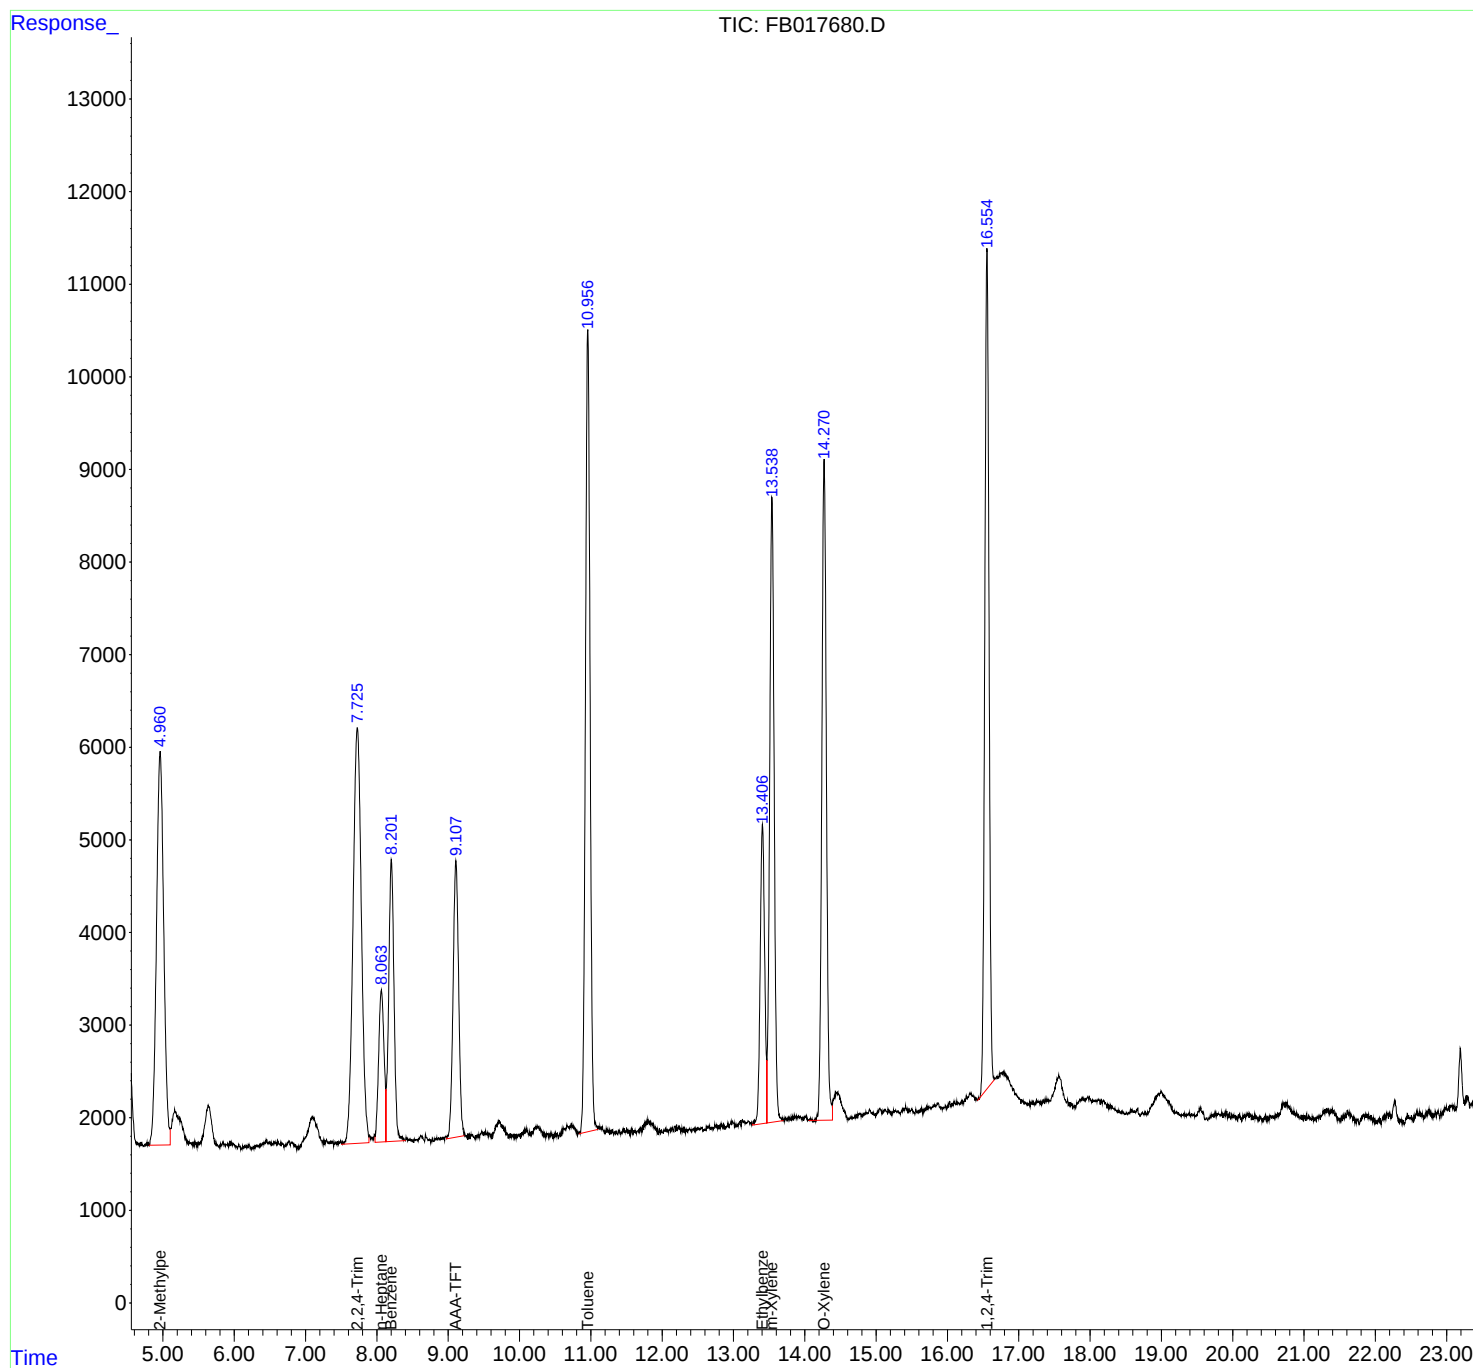

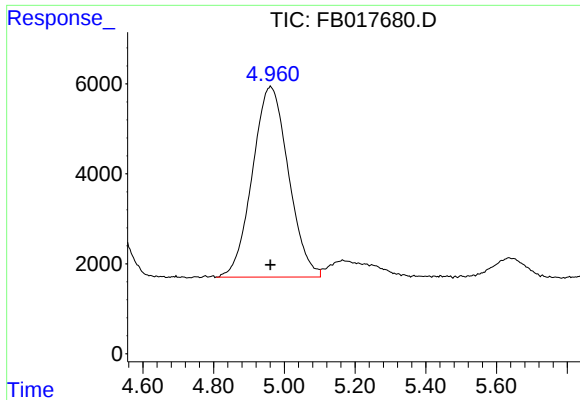


#1 2-Methylpentane

R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 299331
Conc: 21.36 ng/ml

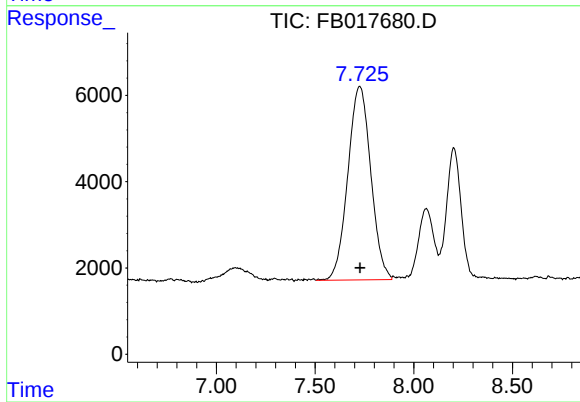


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: -0.001 min
Response: 362898
Conc: 25.75 ng/ml

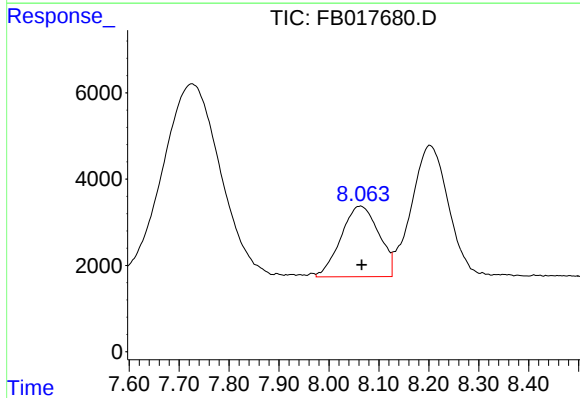


#3 n-Heptane

R.T.: 8.064 min
Delta R.T.: -0.002 min
Response: 85859
Conc: 6.23 ng/ml

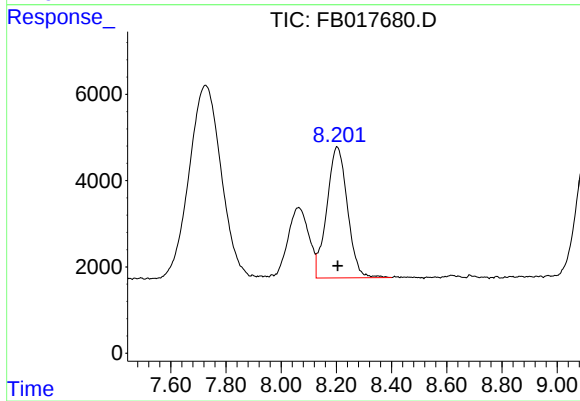


#4 Benzene

R.T.: 8.203 min
Delta R.T.: -0.002 min
Response: 157703
Conc: 8.94 ng/ml

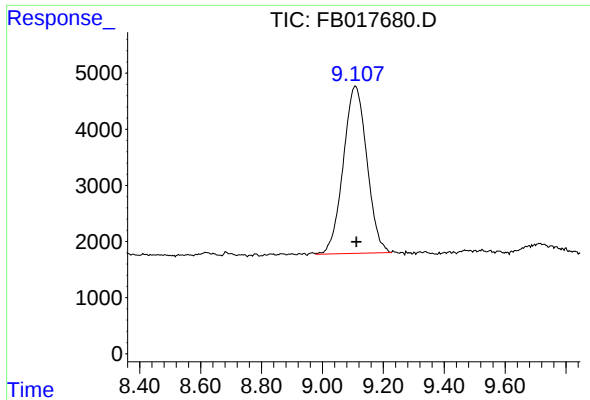


#5 AAA-TFT

R.T.: 9.109 min
Delta R.T.: -0.002 min
Response: 160372
Conc: 19.45 ng/ml

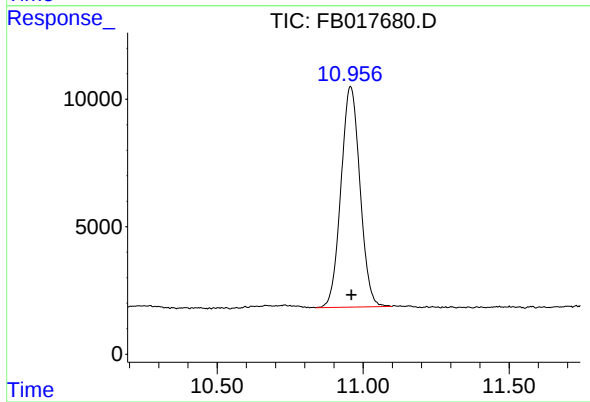


#6 Toluene

R.T.: 10.957 min
Delta R.T.: -0.003 min
Response: 391469
Conc: 27.21 ng/ml

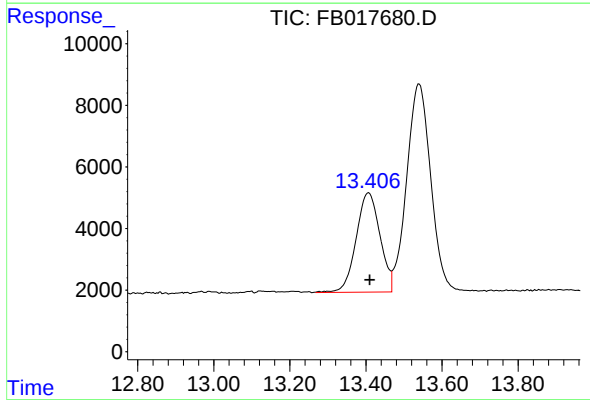


#7 Ethylbenzene

R.T.: 13.407 min
Delta R.T.: -0.004 min
Response: 140345
Conc: 9.52 ng/ml

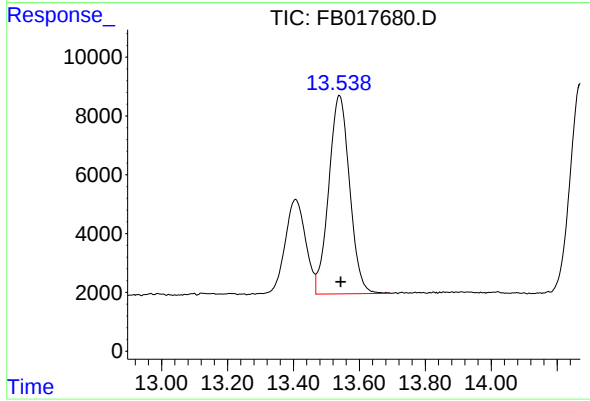


#8 m-Xylene

R.T.: 13.540 min
Delta R.T.: -0.003 min
Response: 296788
Conc: 19.09 ng/ml

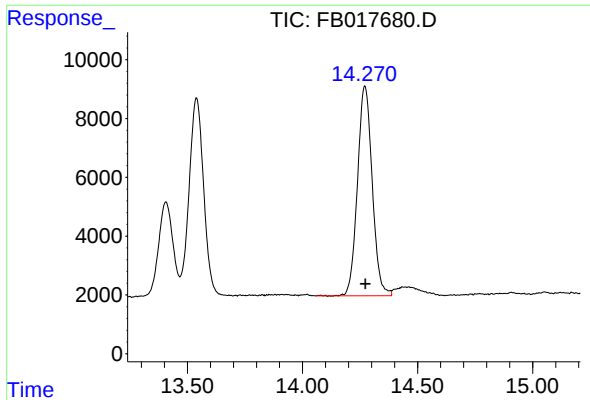

#9 O-Xylene

R.T.: 14.271 min
Delta R.T.: -0.003 min
Response: 317753
Conc: 19.36 ng/ml

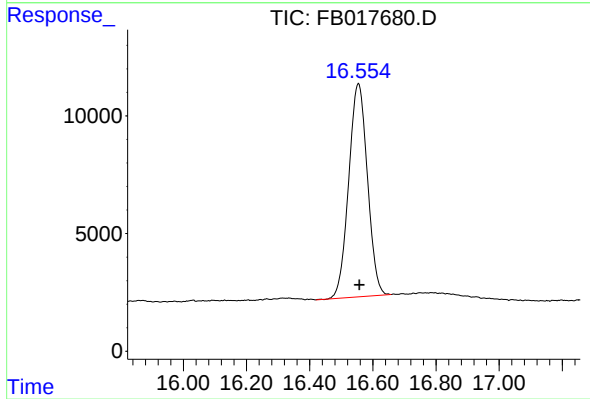

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: -0.003 min
Response: 372834
Conc: 19.14 ng/ml