

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091119\
 Data File : FB022450.D
 Signal(s) : FID2B.CH
 Acq On : 11 Sep 2019 17:30
 Operator : DD/AJ
 Sample : K4825-09MSD
 Misc : 5.02g/5.00ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 CSA-4-2MSD

Integration File: Calibration.e
 Quant Time: Sep 12 06:25:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.971	481114	16.540 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.838	687399	13.991 ng/ml
2) t 2,2,4-Trimethylpentane	7.588	699963	13.555 ng/ml
3) t n-Heptane	7.929	228500	4.540 ng/ml
4) t Benzene	8.063	412448	6.949 ng/ml
6) t Toluene	10.812	1138323	23.928 ng/ml
7) t Ethylbenzene	13.258	335757	11.200 ng/ml
8) t m-Xylene	13.391	655262	24.665 ng/ml
9) t O-Xylene	14.121	611706	25.215 ng/ml
10) t 1,2,4-Trimethylbenzene	16.401	369807	14.184 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091119\
Data File : FB022450.D
Signal(s) : FID2B.CH
Acq On : 11 Sep 2019 17:30
Operator : DD/AJ
Sample : K4825-09MSD
Misc : 5.02g/5.00ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
CSA-4-2MSD

Integration File: Calibration.e
Quant Time: Sep 12 06:25:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

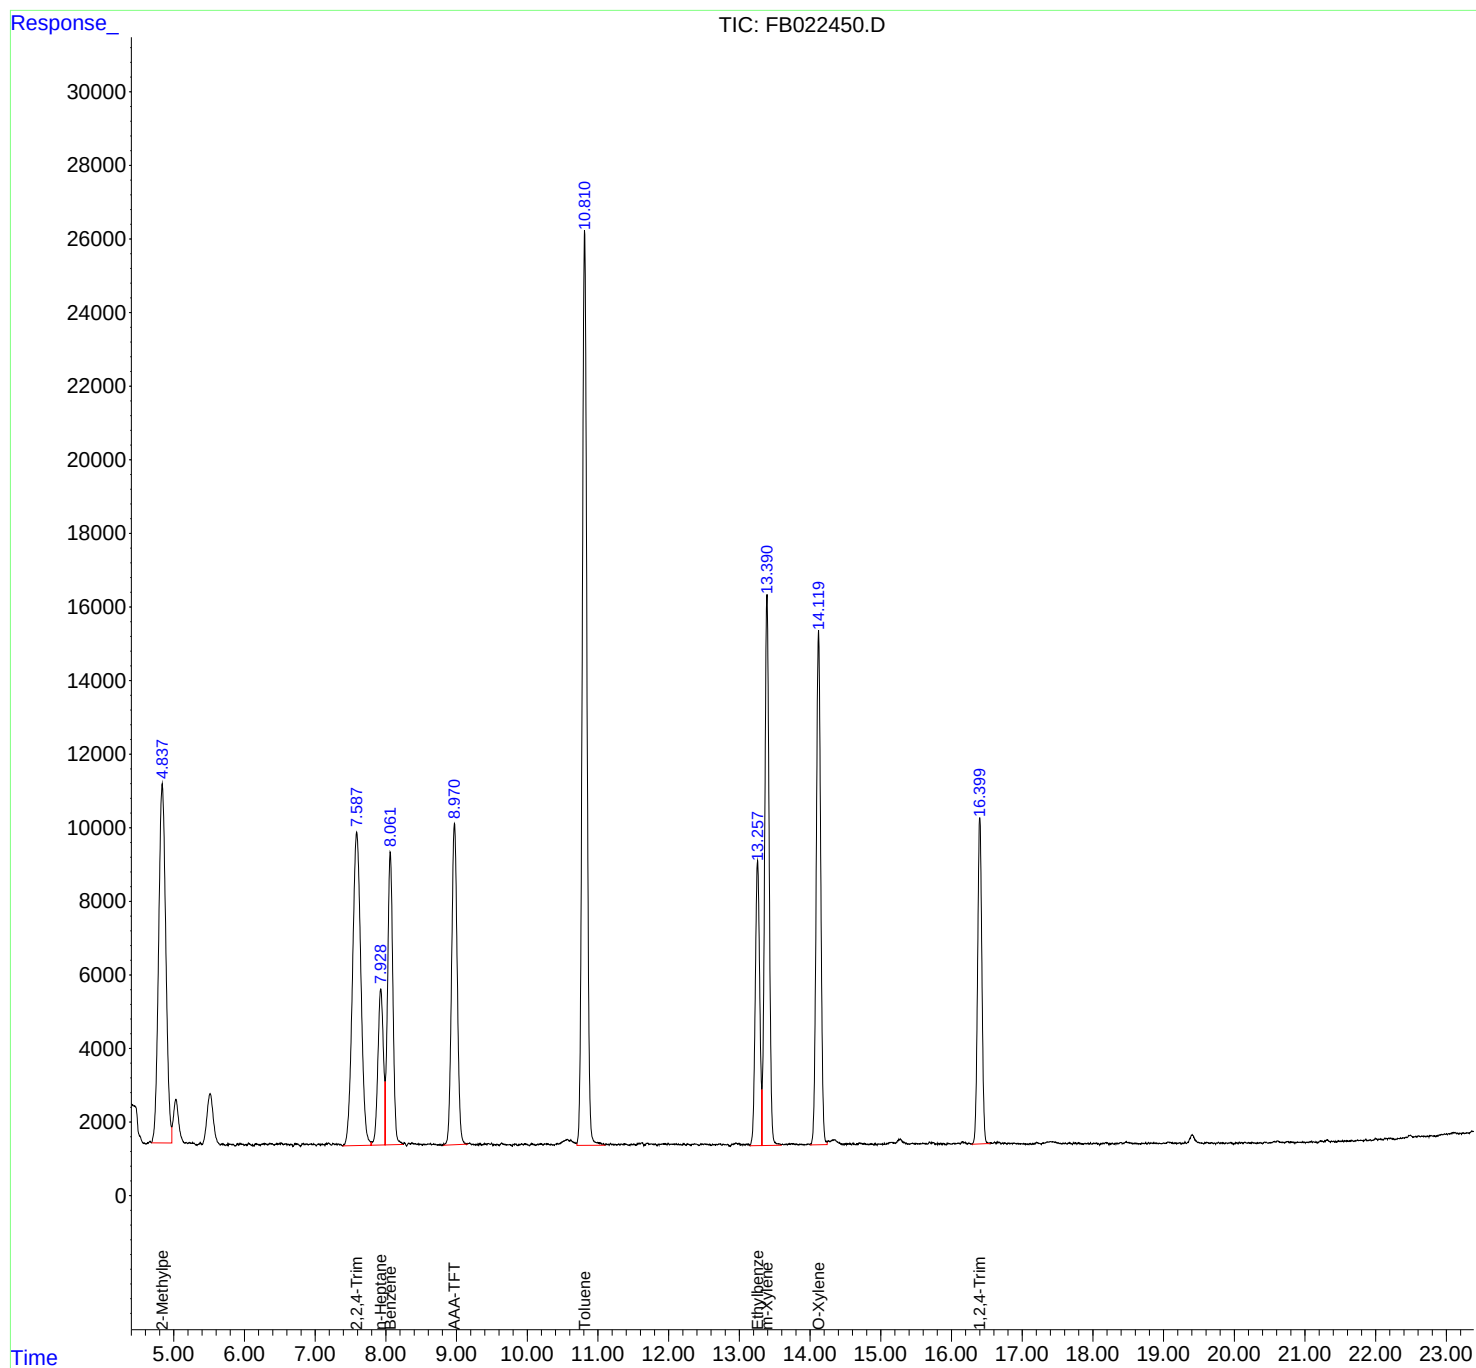


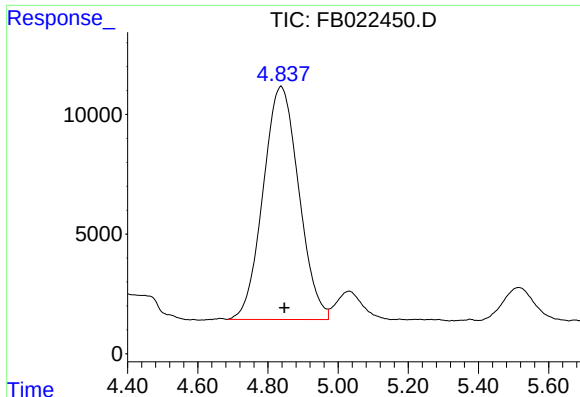

#1 2-Methylpentane


R.T.: 4.838 min
Delta R.T.: -0.009 min
Response: 687399
Conc: 13.99 ng/ml

Instrument :
FID_B
ClientSampleId :
CSA-4-2MSD

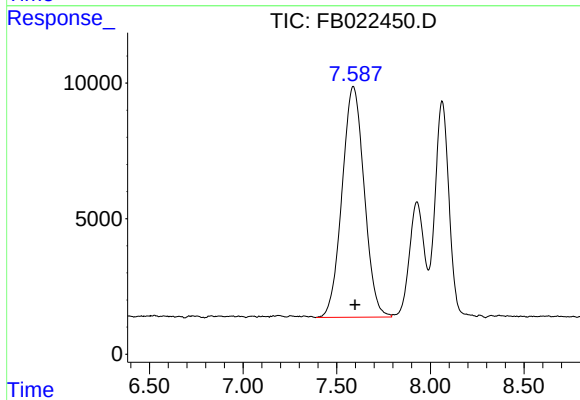


#2 2,2,4-Trimethylpentane

R.T.: 7.588 min
Delta R.T.: -0.009 min
Response: 699963
Conc: 13.56 ng/ml

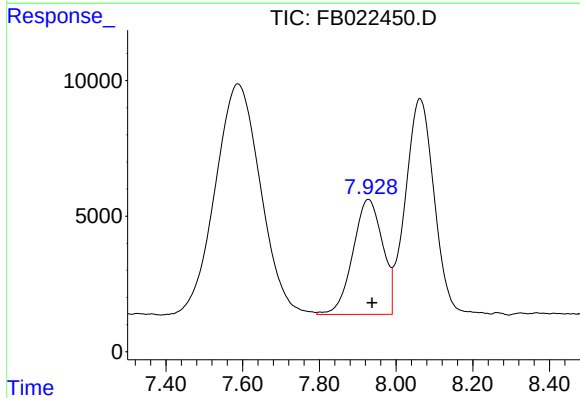


#3 n-Heptane

R.T.: 7.929 min
Delta R.T.: -0.009 min
Response: 228500
Conc: 4.54 ng/ml

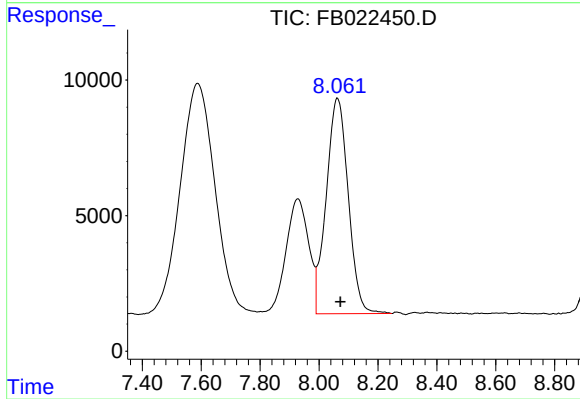

#4 Benzene


R.T.: 8.063 min
Delta R.T.: -0.009 min
Response: 412448
Conc: 6.95 ng/ml

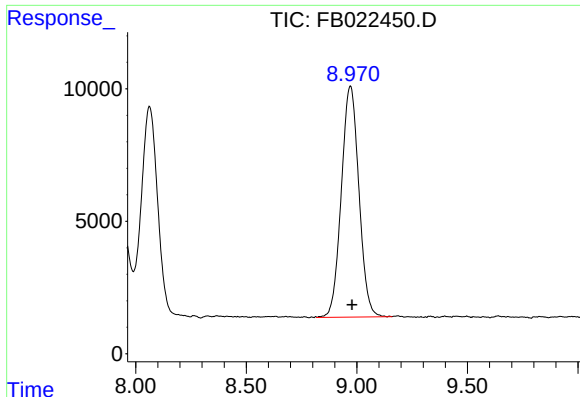

#5 AAA-TFT


R.T.: 8.971 min
Delta R.T.: -0.008 min
Response: 481114
Conc: 16.54 ng/ml

Instrument :
FID_B
ClientSampleId :
CSA-4-2MSD

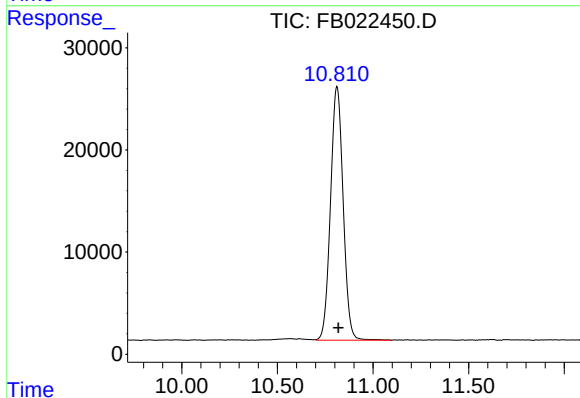


#6 Toluene

R.T.: 10.812 min
Delta R.T.: -0.008 min
Response: 1138323
Conc: 23.93 ng/ml

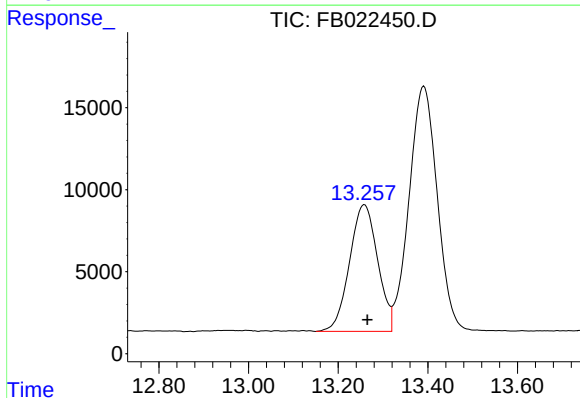


#7 Ethylbenzene

R.T.: 13.258 min
Delta R.T.: -0.007 min
Response: 335757
Conc: 11.20 ng/ml

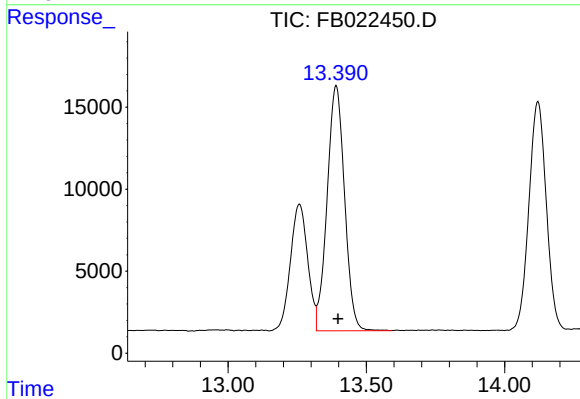

#8 m-Xylene


R.T.: 13.391 min
Delta R.T.: -0.007 min
Response: 655262
Conc: 24.67 ng/ml

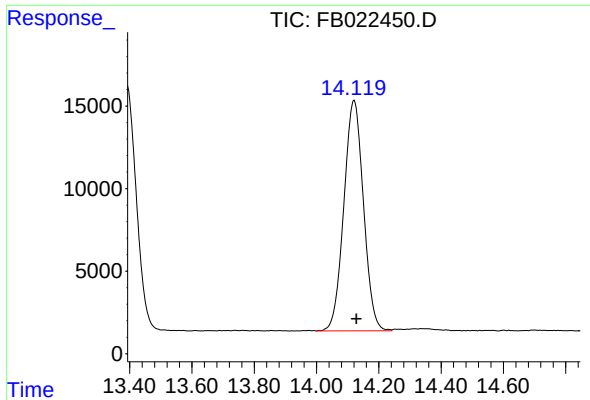

#9 O-Xylene

R.T.: 14.121 min
Delta R.T.: -0.007 min
Response: 611706
Conc: 25.21 ng/ml

Instrument :
FID_B
ClientSampleId :
CSA-4-2MSD

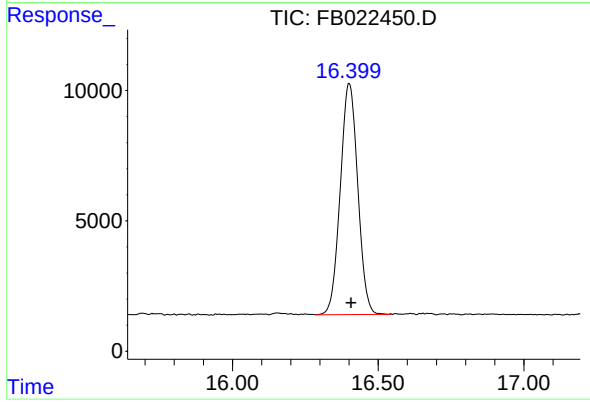

#10 1,2,4-Trimethylbenzene

R.T.: 16.401 min
Delta R.T.: -0.006 min
Response: 369807
Conc: 14.18 ng/ml