

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091119\
 Data File : FB022445.D
 Signal(s) : FID2B.CH
 Acq On : 11 Sep 2019 9:39
 Operator : DD/AJ
 Sample : BSF0911S1
 Misc : 5.01g/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0911S1

Integration File: Calibration.e
 Quant Time: Sep 12 06:25:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.969	538831	18.525 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.833	1103523	22.460 ng/ml
2) t 2,2,4-Trimethylpentane	7.586	1243409	24.079 ng/ml
3) t n-Heptane	7.926	405172	8.050 ng/ml
4) t Benzene	8.060	484538	8.164 ng/ml
6) t Toluene	10.810	1421901	29.889 ng/ml
7) t Ethylbenzene	13.256	450940	15.042 ng/ml
8) t m-Xylene	13.389	893137	33.619 ng/ml
9) t O-Xylene	14.118	839029	34.585 ng/ml
10) t 1,2,4-Trimethylbenzene	16.399	566914	21.745 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091119\
Data File : FB022445.D
Signal(s) : FID2B.CH
Acq On : 11 Sep 2019 9:39
Operator : DD/AJ
Sample : BSF0911S1
Misc : 5.01g/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0911S1

Integration File: Calibration.e
Quant Time: Sep 12 06:25:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

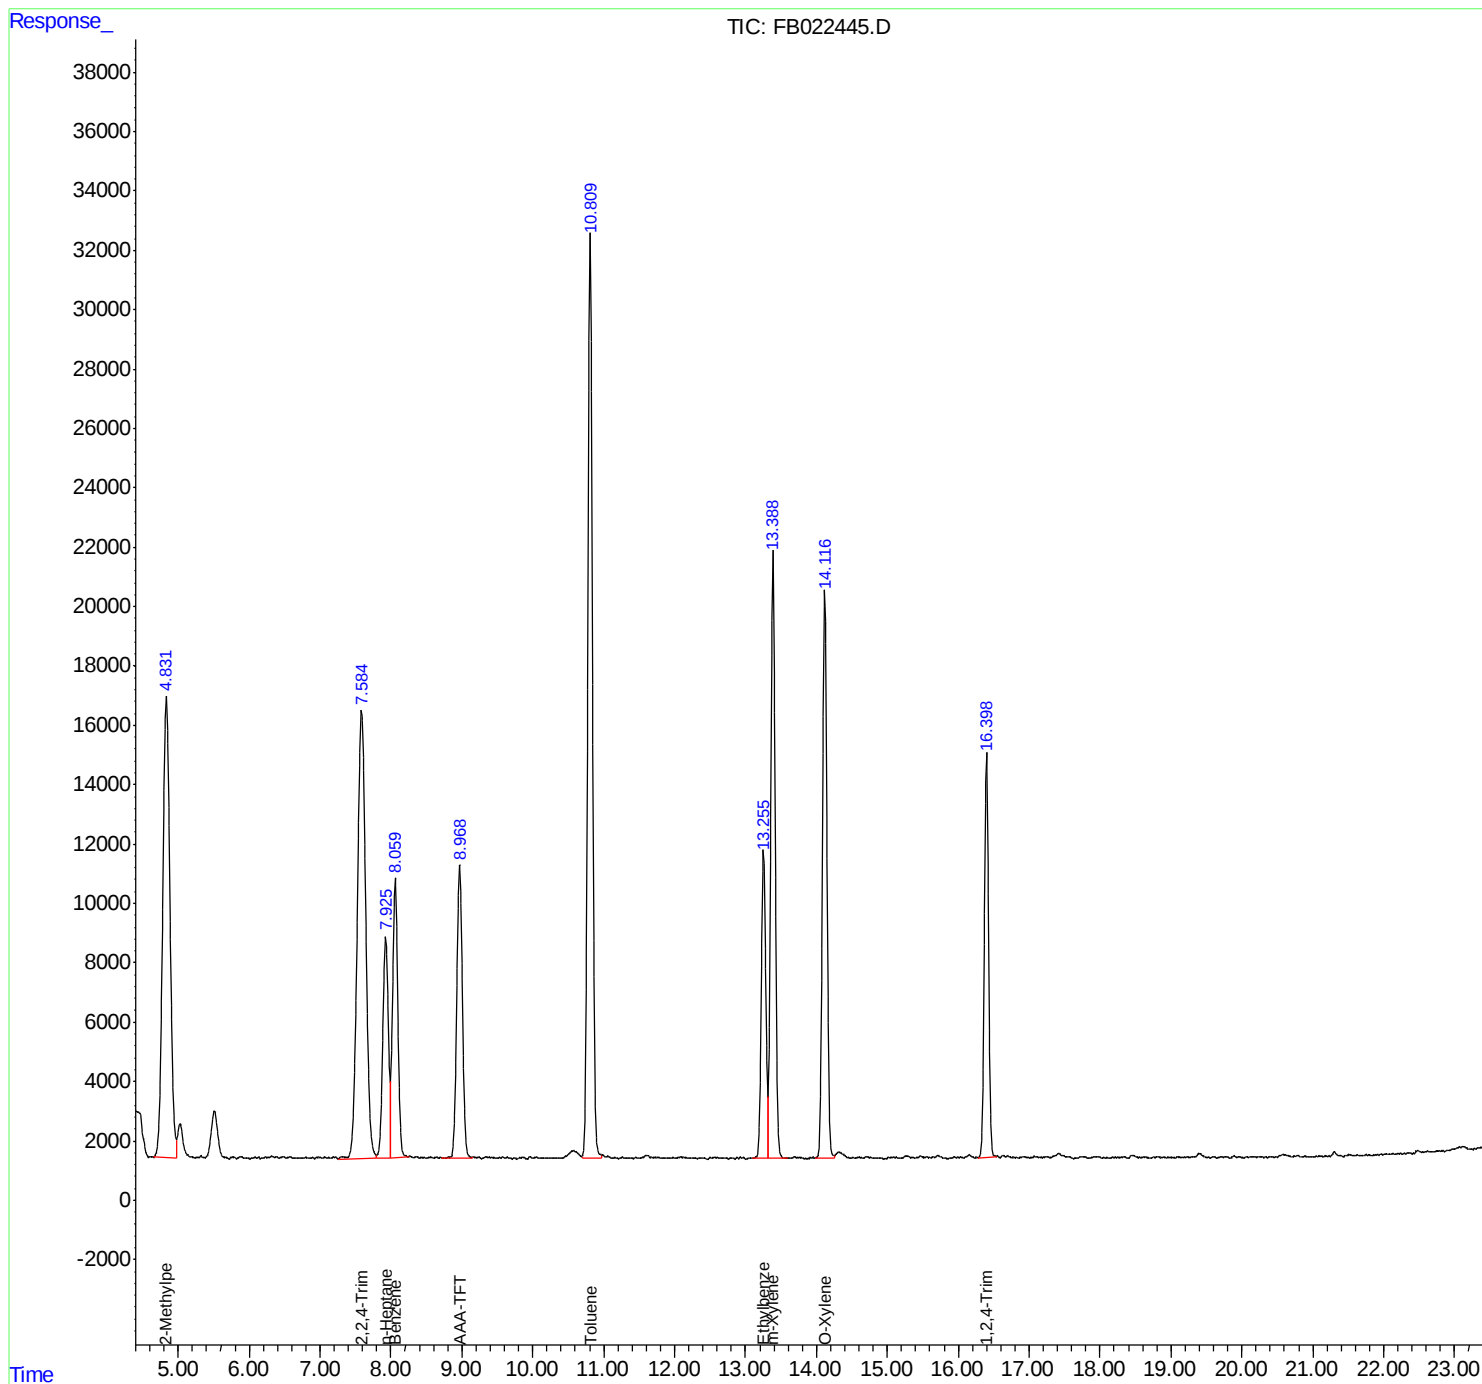


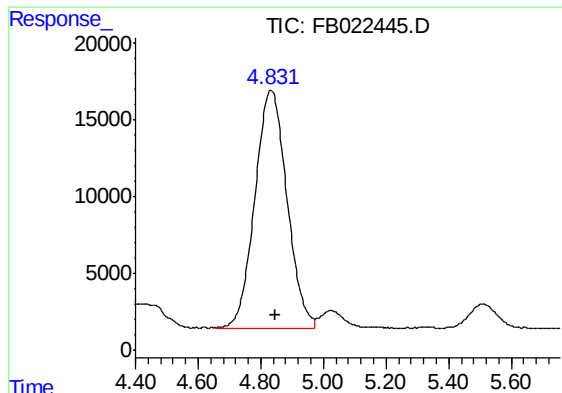

#1 2-Methylpentane


R.T.: 4.833 min
Delta R.T.: -0.014 min
Response: 1103523
Conc: 22.46 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0911S1

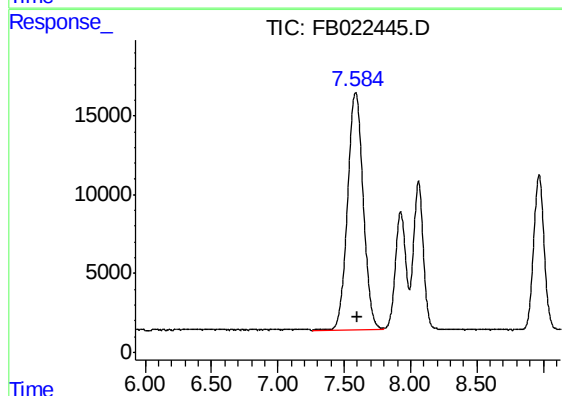


#2 2,2,4-Trimethylpentane

R.T.: 7.586 min
Delta R.T.: -0.012 min
Response: 1243409
Conc: 24.08 ng/ml

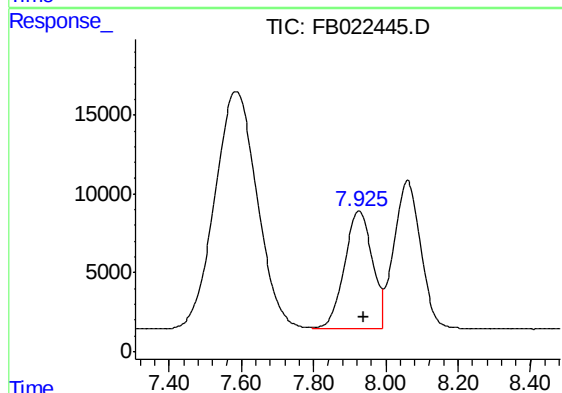


#3 n-Heptane

R.T.: 7.926 min
Delta R.T.: -0.012 min
Response: 405172
Conc: 8.05 ng/ml

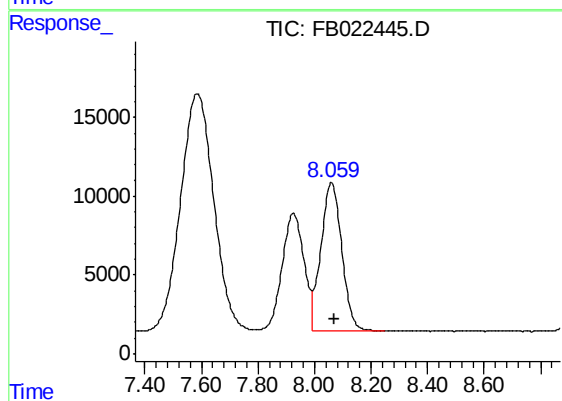

#4 Benzene


R.T.: 8.060 min
Delta R.T.: -0.012 min
Response: 484538
Conc: 8.16 ng/ml

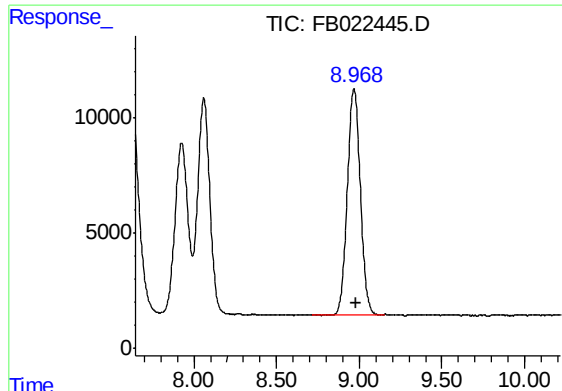

#5 AAA-TFT


R.T.: 8.969 min
Delta R.T.: -0.010 min
Response: 538831
Conc: 18.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0911S1

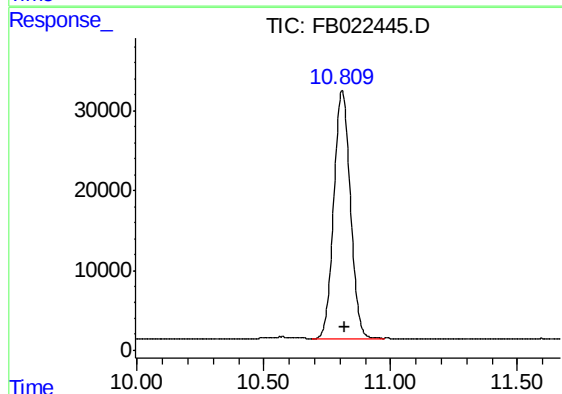


#6 Toluene

R.T.: 10.810 min
Delta R.T.: -0.010 min
Response: 1421901
Conc: 29.89 ng/ml

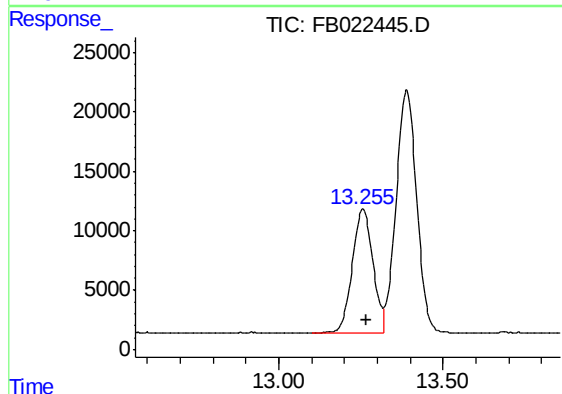


#7 Ethylbenzene

R.T.: 13.256 min
Delta R.T.: -0.009 min
Response: 450940
Conc: 15.04 ng/ml

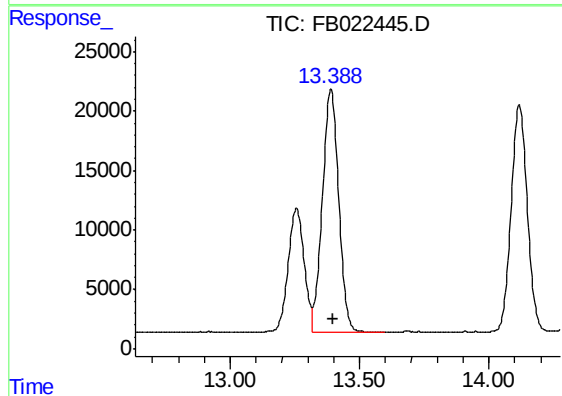

#8 m-Xylene


R.T.: 13.389 min
Delta R.T.: -0.009 min
Response: 893137
Conc: 33.62 ng/ml

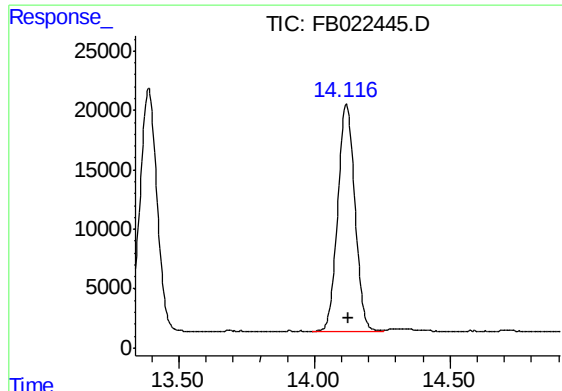

#9 O-Xylene

R.T.: 14.118 min
Delta R.T.: -0.010 min
Response: 839029
Conc: 34.58 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0911S1

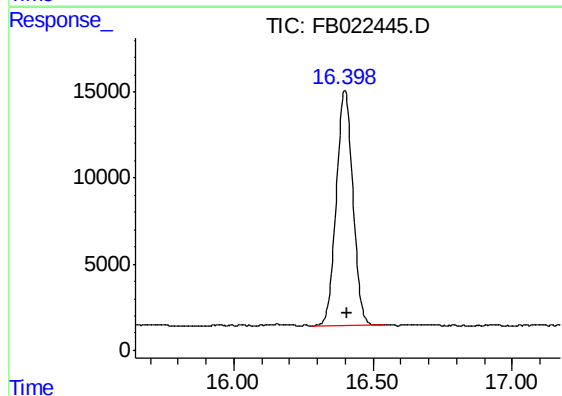

#10 1,2,4-Trimethylbenzene

R.T.: 16.399 min
Delta R.T.: -0.008 min
Response: 566914
Conc: 21.74 ng/ml