

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091219\
 Data File : FB022455.D
 Signal(s) : FID2B.CH
 Acq On : 12 Sep 2019 9:02
 Operator : DD/AJ
 Sample : BSF0912S1
 Misc : 5.01g/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 13 01:26:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.968	581811	20.002 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.834	1149489	23.395 ng/ml
2) t 2,2,4-Trimethylpentane	7.586	1289945	24.981 ng/ml
3) t n-Heptane	7.926	425171	8.448 ng/ml
4) t Benzene	8.061	519752	8.758 ng/ml
6) t Toluene	10.810	1519918	31.949 ng/ml
7) t Ethylbenzene	13.256	483036	16.112 ng/ml
8) t m-Xylene	13.389	954646	35.934 ng/ml
9) t O-Xylene	14.119	897389	36.990 ng/ml
10) t 1,2,4-Trimethylbenzene	16.400	609887	23.393 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091219\
Data File : FB022455.D
Signal(s) : FID2B.CH
Acq On : 12 Sep 2019 9:02
Operator : DD/AJ
Sample : BSF0912S1
Misc : 5.01g/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 13 01:26:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

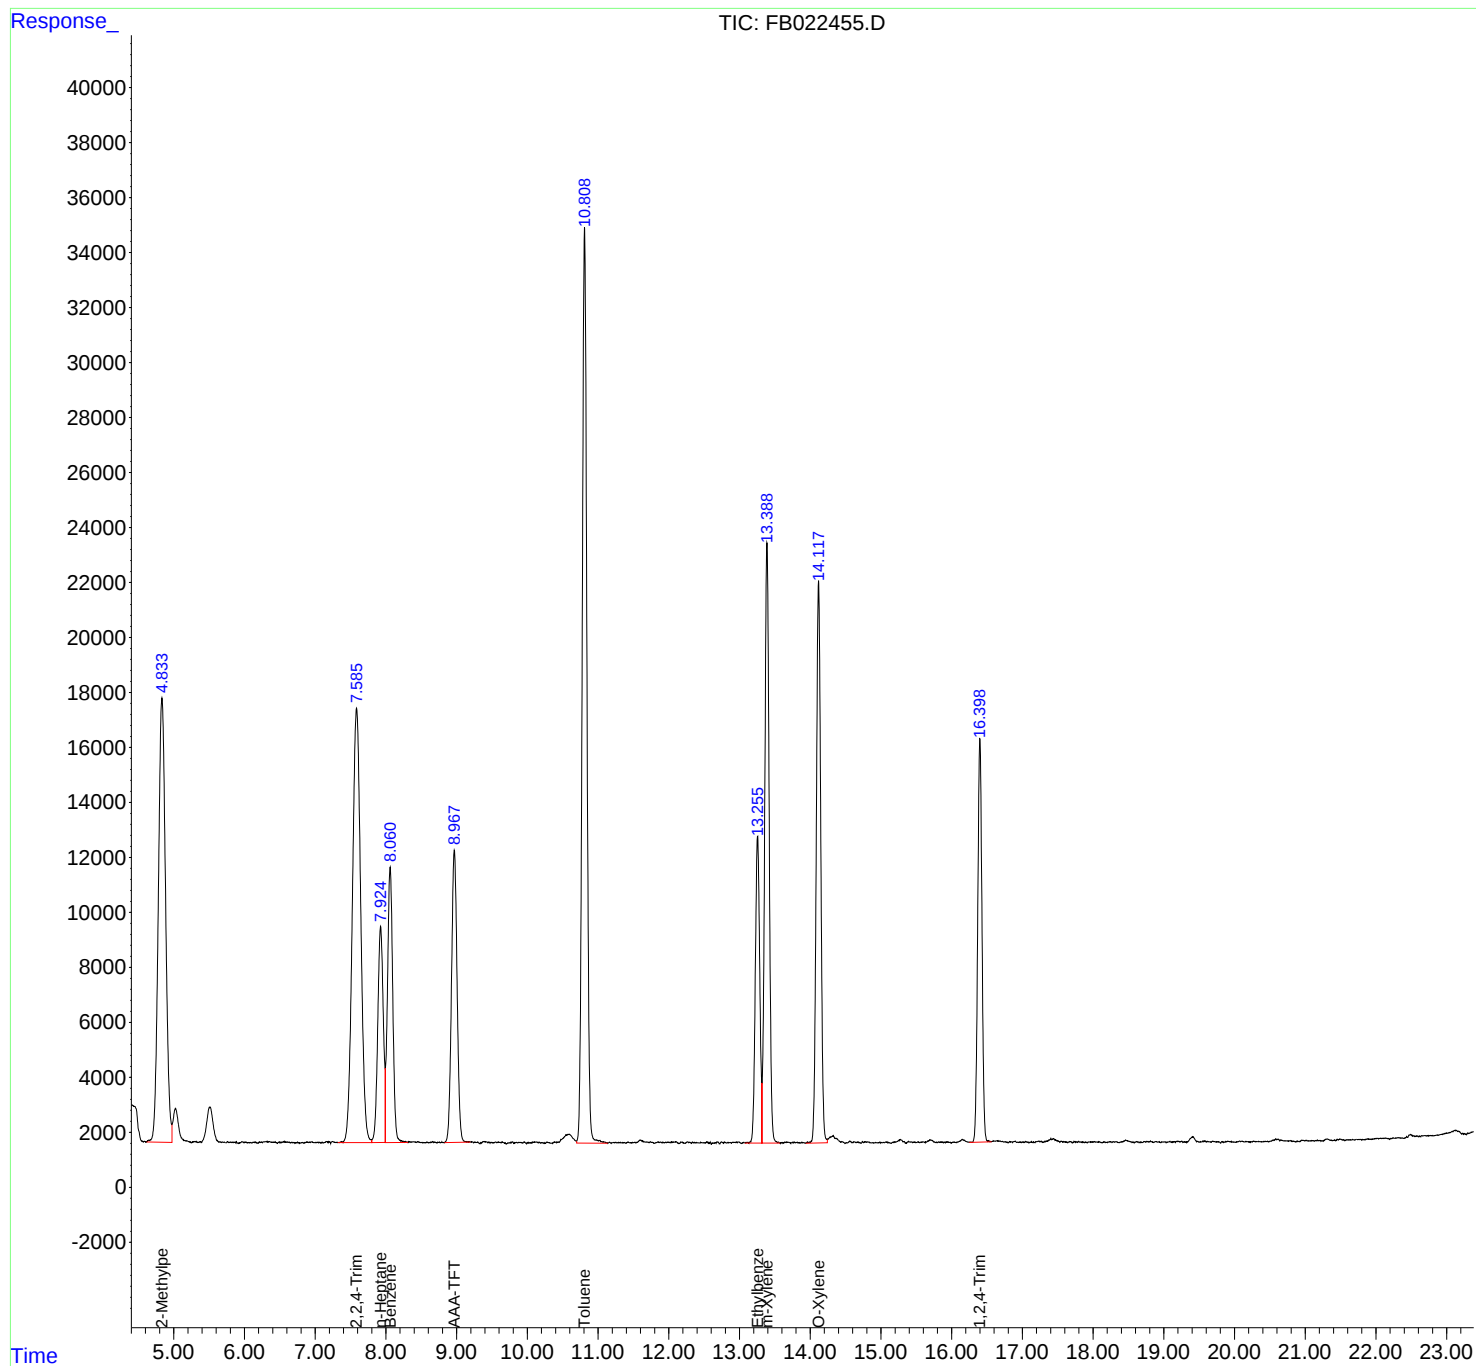

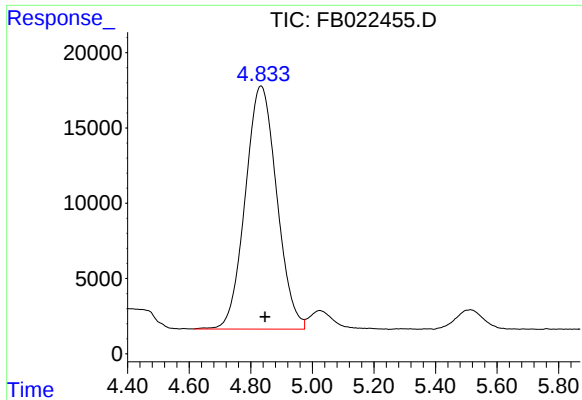


#1 2-Methylpentane

R.T.: 4.834 min
Delta R.T.: -0.013 min
Response: 1149489
Conc: 23.40 ng/ml

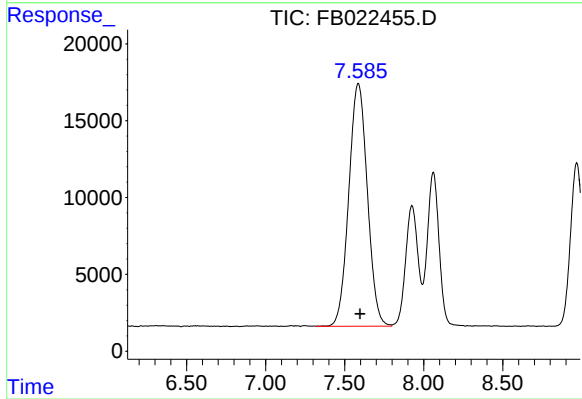


#2 2,2,4-Trimethylpentane

R.T.: 7.586 min
Delta R.T.: -0.012 min
Response: 1289945
Conc: 24.98 ng/ml

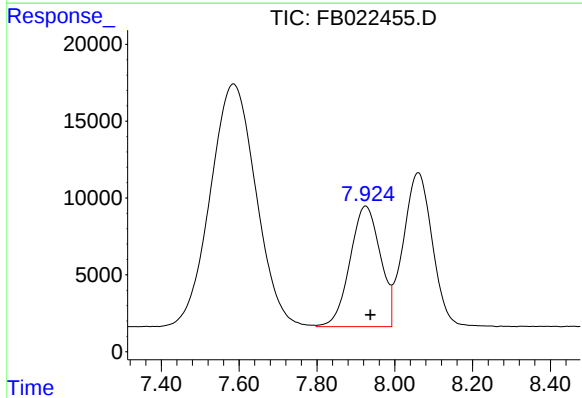


#3 n-Heptane

R.T.: 7.926 min
Delta R.T.: -0.012 min
Response: 425171
Conc: 8.45 ng/ml

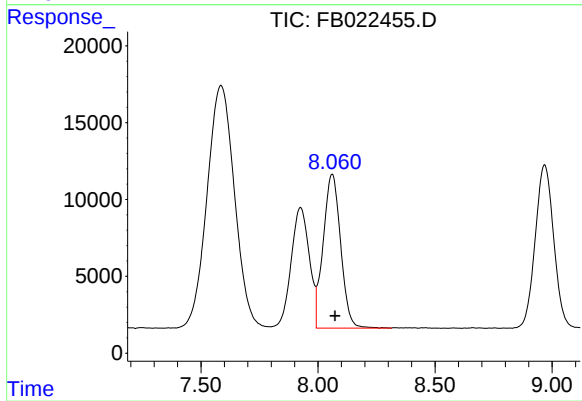


#4 Benzene

R.T.: 8.061 min
Delta R.T.: -0.012 min
Response: 519752
Conc: 8.76 ng/ml

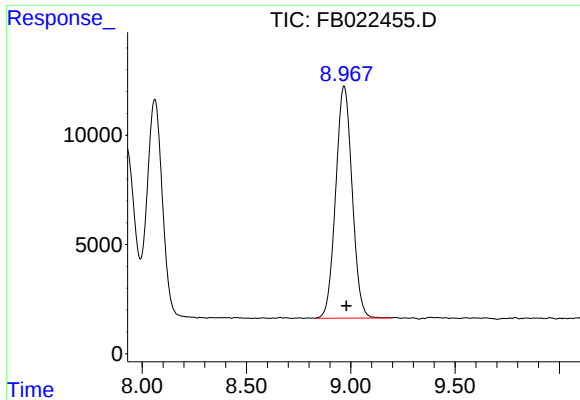


#5 AAA-TFT

R.T.: 8.968 min
Delta R.T.: -0.011 min
Response: 581811
Conc: 20.00 ng/ml

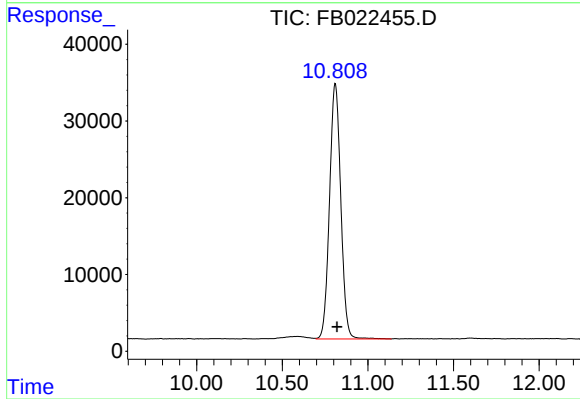


#6 Toluene

R.T.: 10.810 min
Delta R.T.: -0.010 min
Response: 1519918
Conc: 31.95 ng/ml

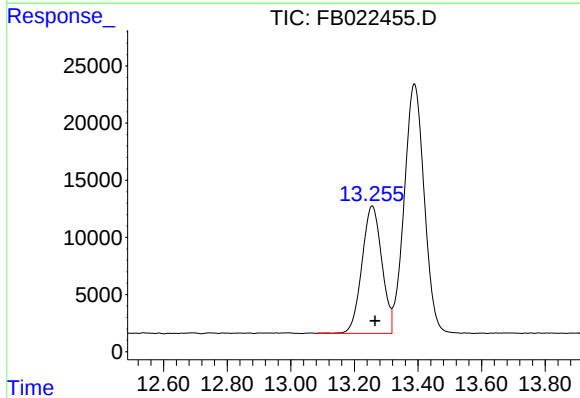


#7 Ethylbenzene

R.T.: 13.256 min
Delta R.T.: -0.009 min
Response: 483036
Conc: 16.11 ng/ml

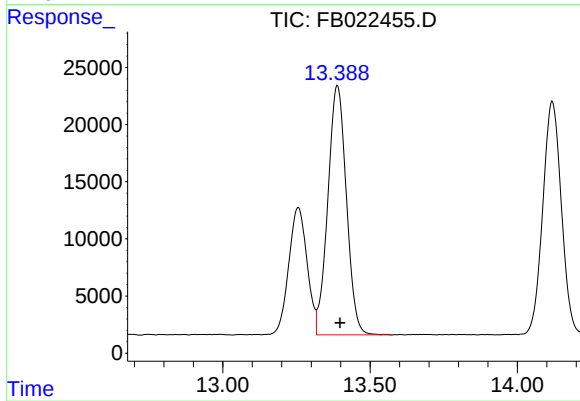

#8 m-Xylene

R.T.: 13.389 min
Delta R.T.: -0.009 min
Response: 954646
Conc: 35.93 ng/ml

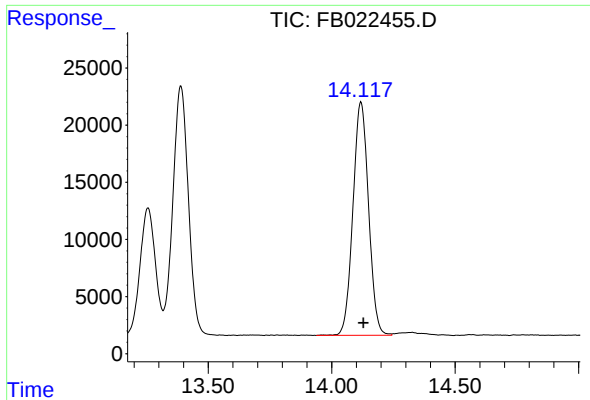


#9 O-Xylene

R.T.: 14.119 min

Delta R.T.: -0.009 min

Response: 897389

Conc: 36.99 ng/ml

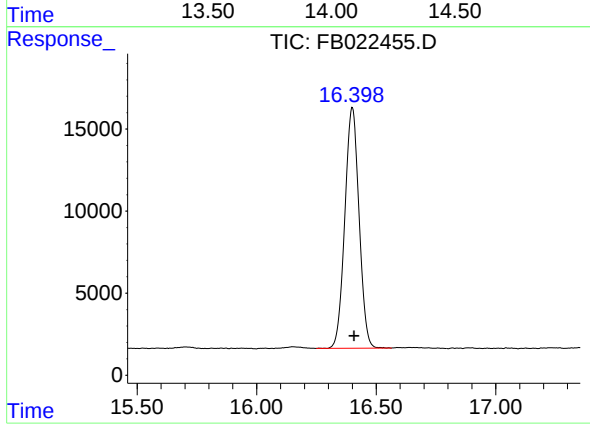

#10 1,2,4-Trimethylbenzene

R.T.: 16.400 min

Delta R.T.: -0.007 min

Response: 609887

Conc: 23.39 ng/ml