

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091219\
 Data File : FB022466.D
 Signal(s) : FID2B.CH
 Acq On : 12 Sep 2019 14:37
 Operator : DD/AJ
 Sample : K4857-02MS
 Misc : 5.03g/5.00ML DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 13 01:29:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.968	548444	18.855 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.836	1063367	21.643 ng/ml
2) t 2,2,4-Trimethylpentane	7.586	1171729	22.691 ng/ml
3) t n-Heptane	7.925	384403	7.638 ng/ml
4) t Benzene	8.061	489746	8.252 ng/ml
6) t Toluene	10.809	1421197	29.874 ng/ml
7) t Ethylbenzene	13.256	452755	15.102 ng/ml
8) t m-Xylene	13.389	884133	33.280 ng/ml
9) t O-Xylene	14.118	826830	34.082 ng/ml
10) t 1,2,4-Trimethylbenzene	16.400	562050	21.558 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091219\
Data File : FB022466.D
Signal(s) : FID2B.CH
Acq On : 12 Sep 2019 14:37
Operator : DD/AJ
Sample : K4857-02MS
Misc : 5.03g/5.00ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 13 01:29:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

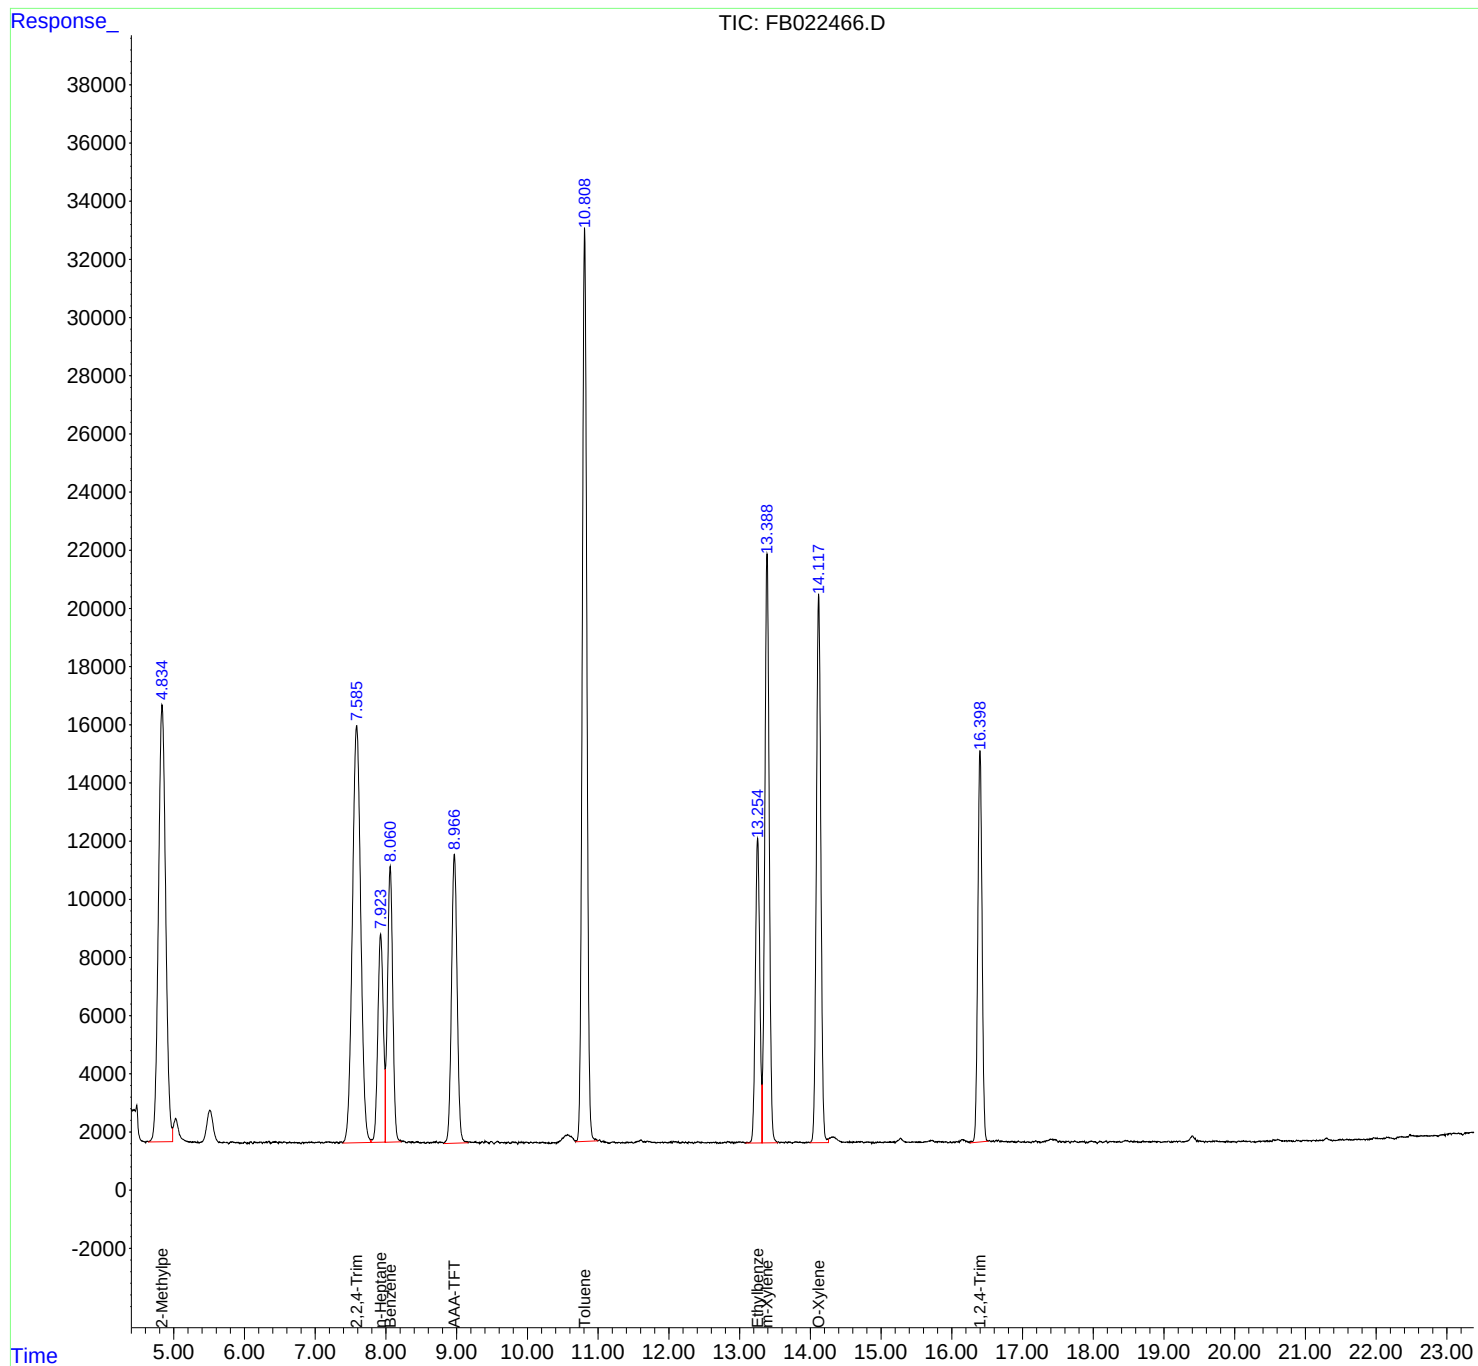

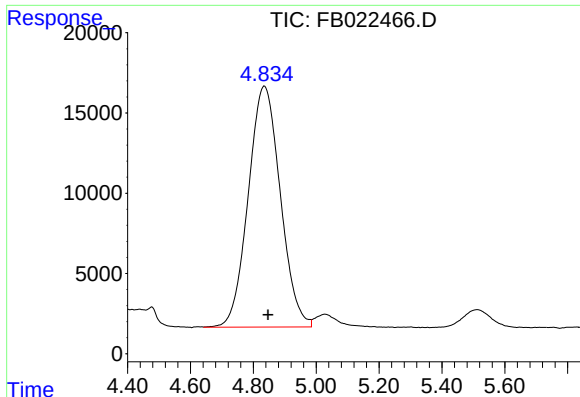


#1 2-Methylpentane

R.T.: 4.836 min
Delta R.T.: -0.011 min
Response: 1063367
Conc: 21.64 ng/ml

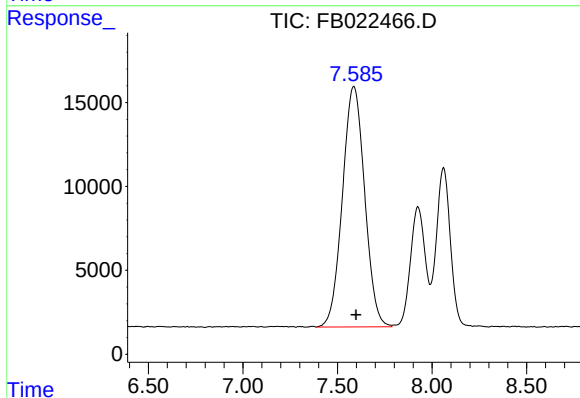


#2 2,2,4-Trimethylpentane

R.T.: 7.586 min
Delta R.T.: -0.011 min
Response: 1171729
Conc: 22.69 ng/ml

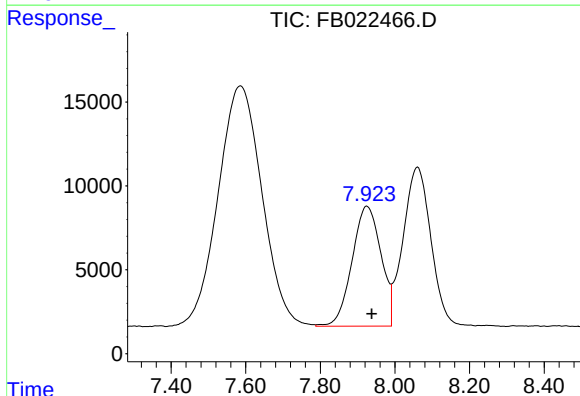


#3 n-Heptane

R.T.: 7.925 min
Delta R.T.: -0.012 min
Response: 384403
Conc: 7.64 ng/ml

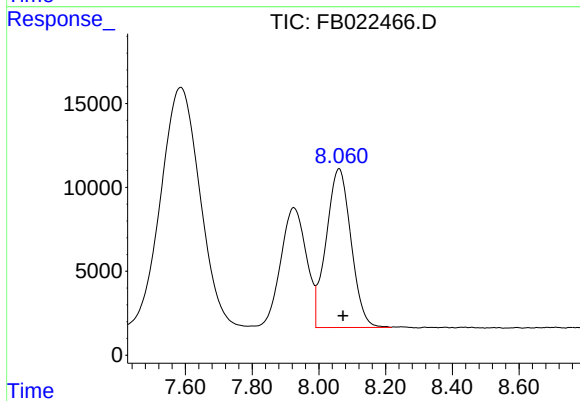


#4 Benzene

R.T.: 8.061 min
Delta R.T.: -0.012 min
Response: 489746
Conc: 8.25 ng/ml

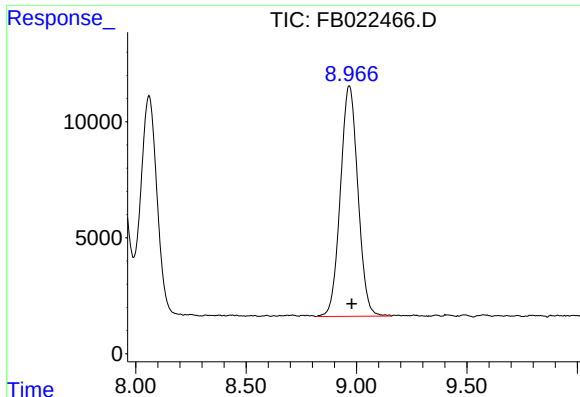


#5 AAA-TFT

R.T.: 8.968 min
Delta R.T.: -0.011 min
Response: 548444
Conc: 18.85 ng/ml

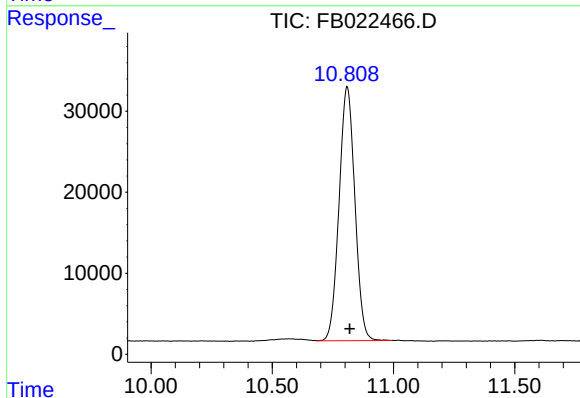


#6 Toluene

R.T.: 10.809 min
Delta R.T.: -0.010 min
Response: 1421197
Conc: 29.87 ng/ml

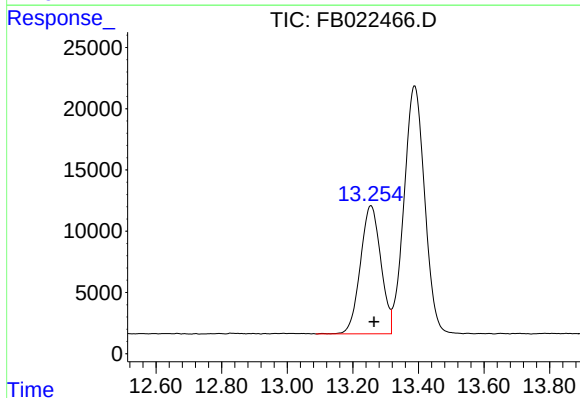


#7 Ethylbenzene

R.T.: 13.256 min
Delta R.T.: -0.009 min
Response: 452755
Conc: 15.10 ng/ml

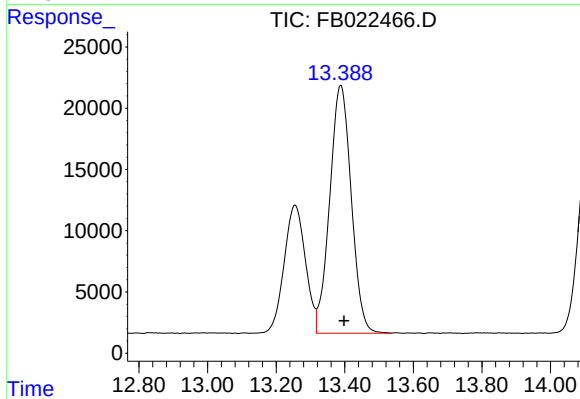


#8 m-Xylene

R.T.: 13.389 min
Delta R.T.: -0.009 min
Response: 884133
Conc: 33.28 ng/ml

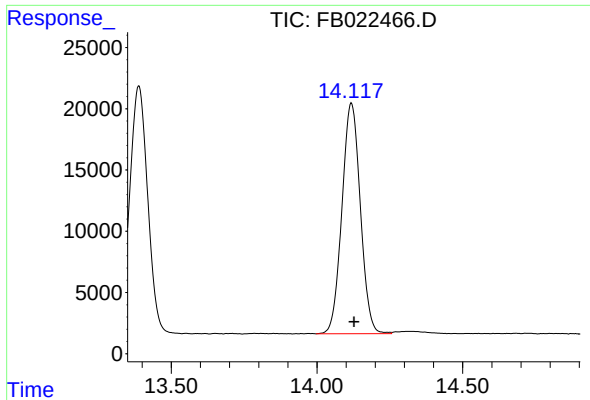

#9 O-Xylene

R.T.: 14.118 min
Delta R.T.: -0.010 min
Response: 826830
Conc: 34.08 ng/ml

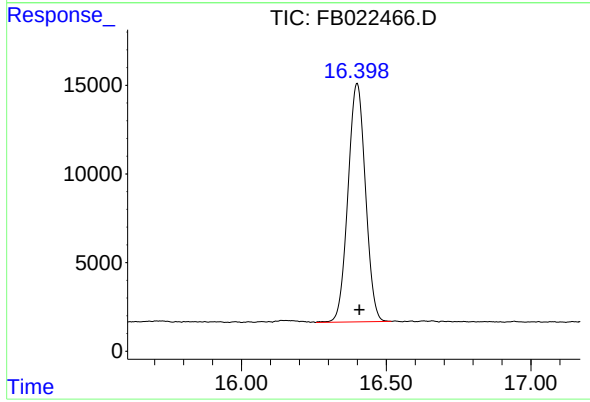

#10 1,2,4-Trimethylbenzene

R.T.: 16.400 min
Delta R.T.: -0.008 min
Response: 562050
Conc: 21.56 ng/ml