

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091219\
 Data File : FB022467.D
 Signal(s) : FID2B.CH
 Acq On : 12 Sep 2019 15:07
 Operator : DD/AJ
 Sample : K4857-02MSD
 Misc : 5.05g/5.00ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 13 01:29:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.969	561243	19.295 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.836	1026945	20.901 ng/ml
2) t 2,2,4-Trimethylpentane	7.587	1220996	23.645 ng/ml
3) t n-Heptane	7.927	397133	7.891 ng/ml
4) t Benzene	8.061	472912	7.968 ng/ml
6) t Toluene	10.810	1427991	30.017 ng/ml
7) t Ethylbenzene	13.257	458564	15.296 ng/ml
8) t m-Xylene	13.390	902324	33.965 ng/ml
9) t O-Xylene	14.119	843549	34.771 ng/ml
10) t 1,2,4-Trimethylbenzene	16.400	558485	21.421 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091219\
Data File : FB022467.D
Signal(s) : FID2B.CH
Acq On : 12 Sep 2019 15:07
Operator : DD/AJ
Sample : K4857-02MSD
Misc : 5.05g/5.00ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 13 01:29:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

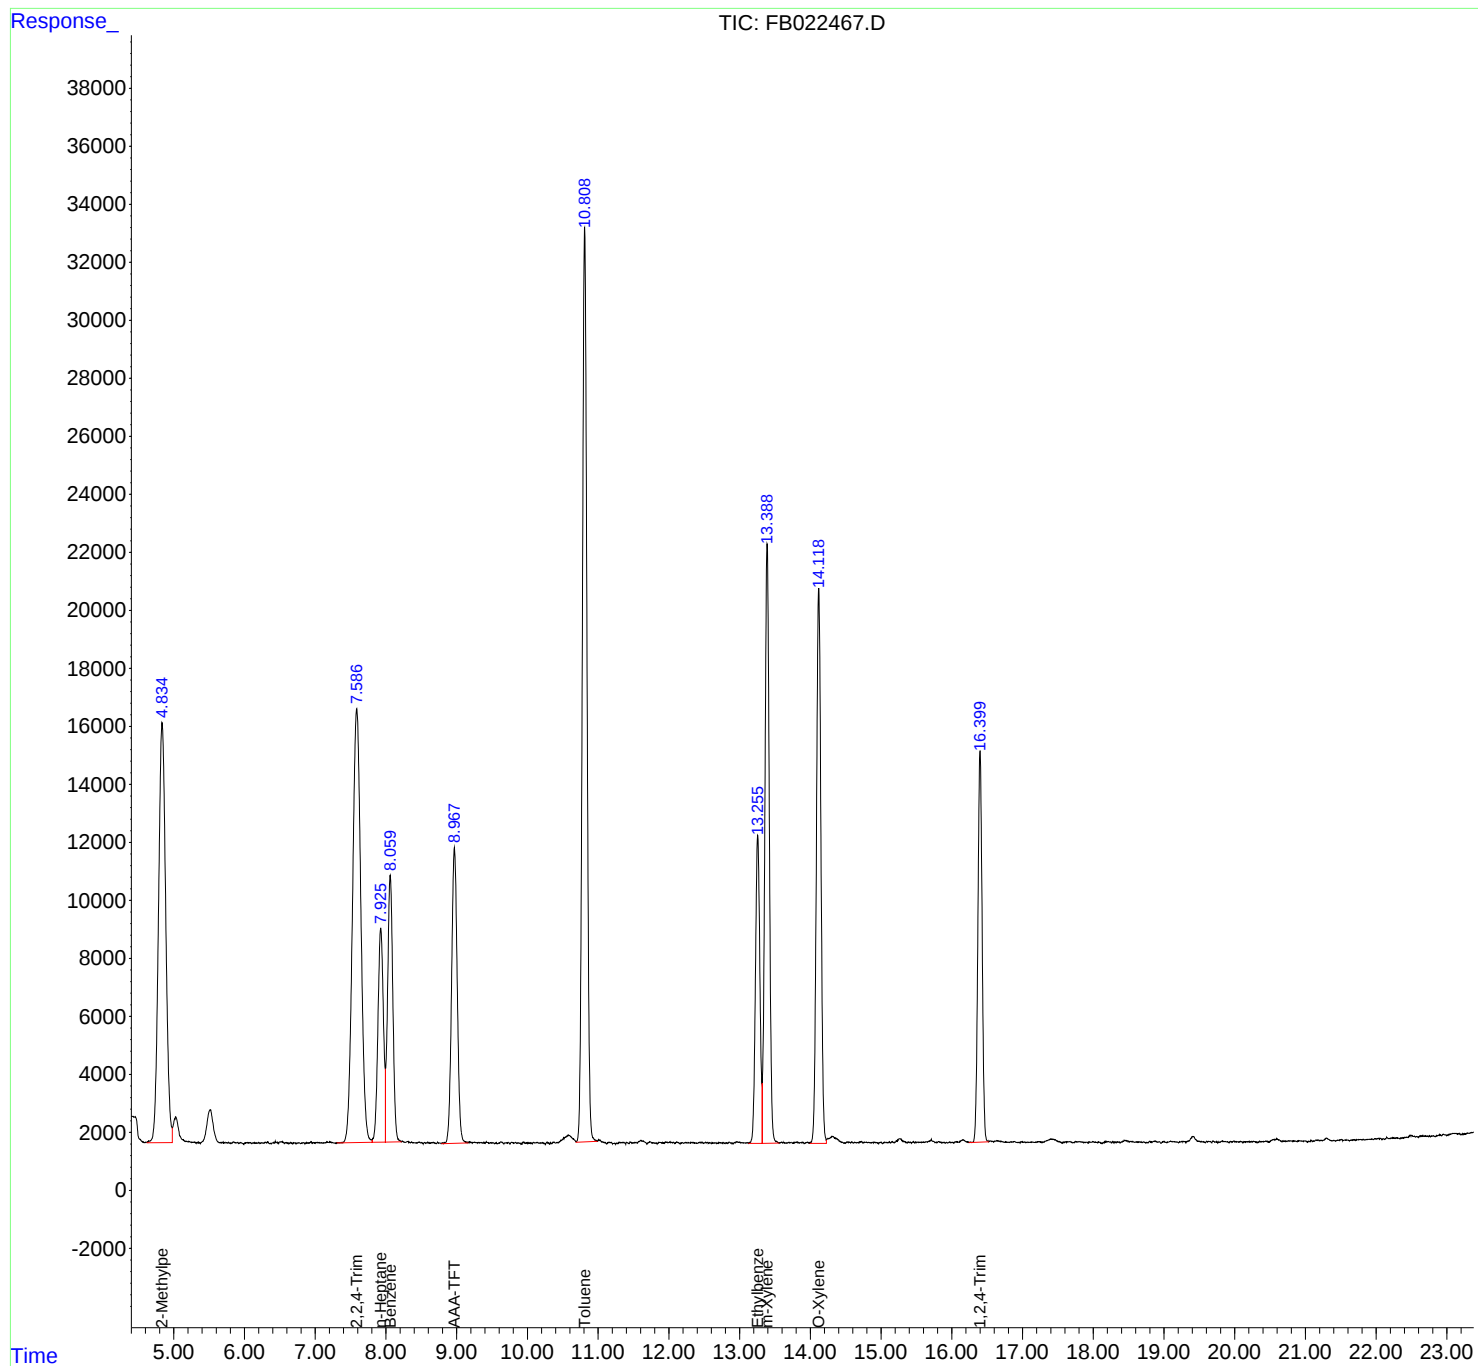

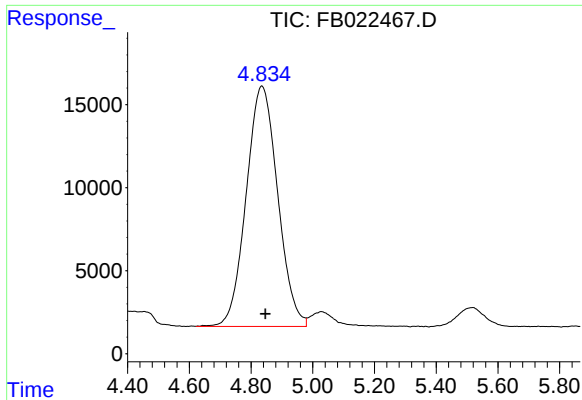


#1 2-Methylpentane

R.T.: 4.836 min
Delta R.T.: -0.011 min
Response: 1026945
Conc: 20.90 ng/ml

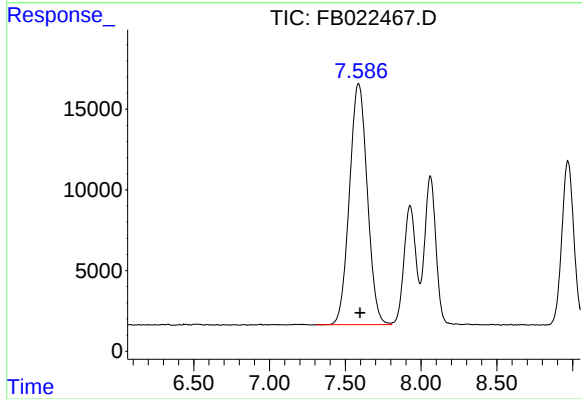


#2 2,2,4-Trimethylpentane

R.T.: 7.587 min
Delta R.T.: -0.010 min
Response: 1220996
Conc: 23.65 ng/ml

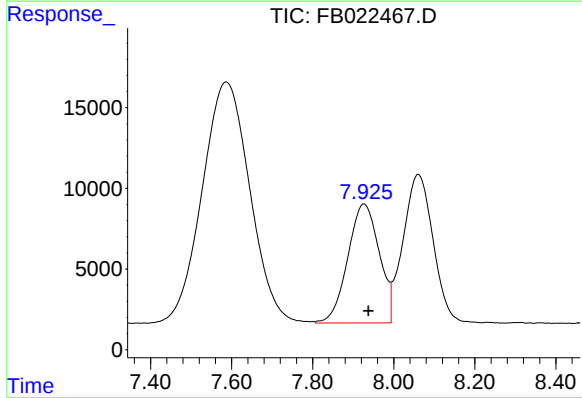


#3 n-Heptane

R.T.: 7.927 min
Delta R.T.: -0.011 min
Response: 397133
Conc: 7.89 ng/ml

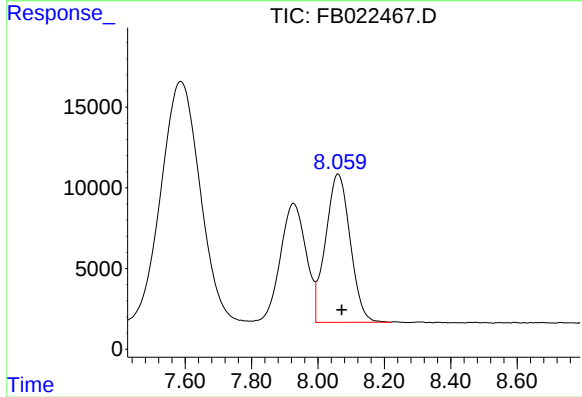


#4 Benzene

R.T.: 8.061 min
Delta R.T.: -0.011 min
Response: 472912
Conc: 7.97 ng/ml

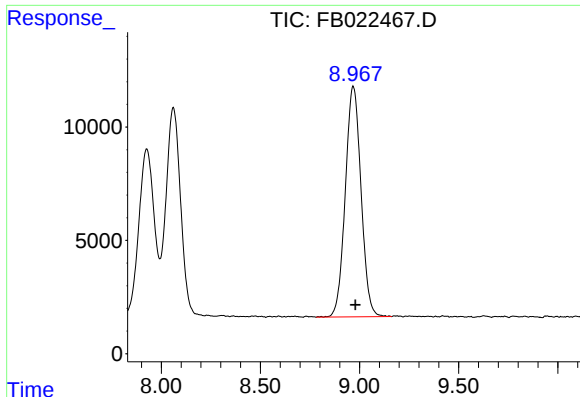


#5 AAA-TFT

R.T.: 8.969 min
Delta R.T.: -0.011 min
Response: 561243
Conc: 19.30 ng/ml

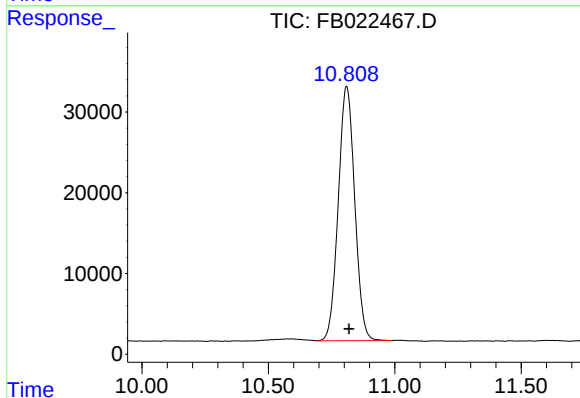


#6 Toluene

R.T.: 10.810 min
Delta R.T.: -0.010 min
Response: 1427991
Conc: 30.02 ng/ml

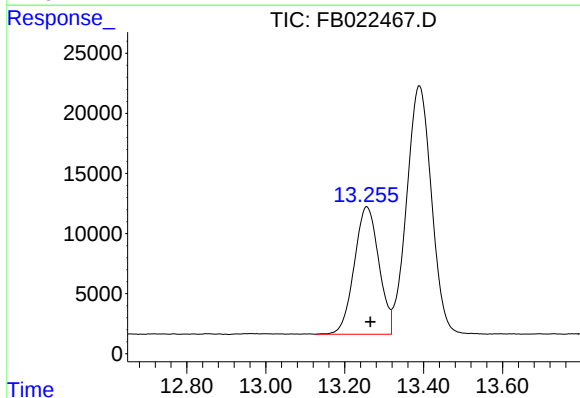


#7 Ethylbenzene

R.T.: 13.257 min
Delta R.T.: -0.008 min
Response: 458564
Conc: 15.30 ng/ml

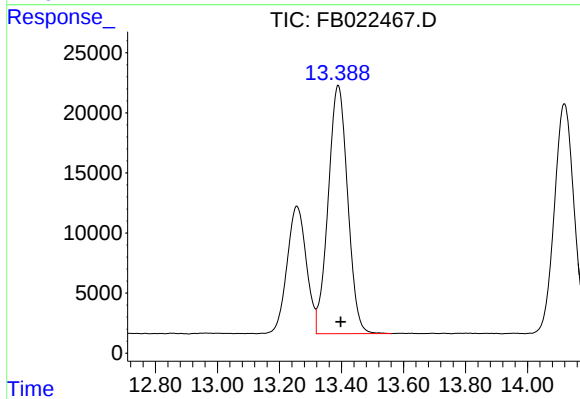


#8 m-Xylene

R.T.: 13.390 min
Delta R.T.: -0.008 min
Response: 902324
Conc: 33.96 ng/ml

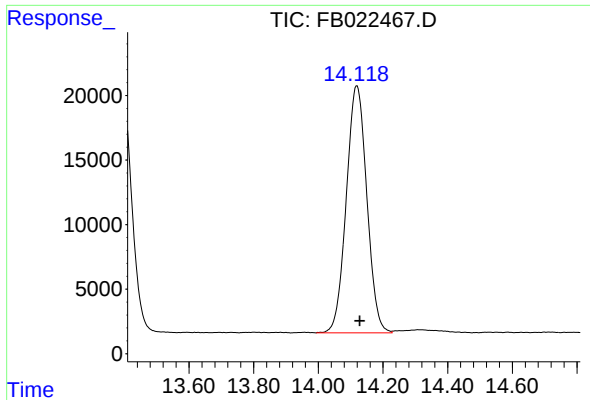

#9 O-Xylene

R.T.: 14.119 min
Delta R.T.: -0.009 min
Response: 843549
Conc: 34.77 ng/ml

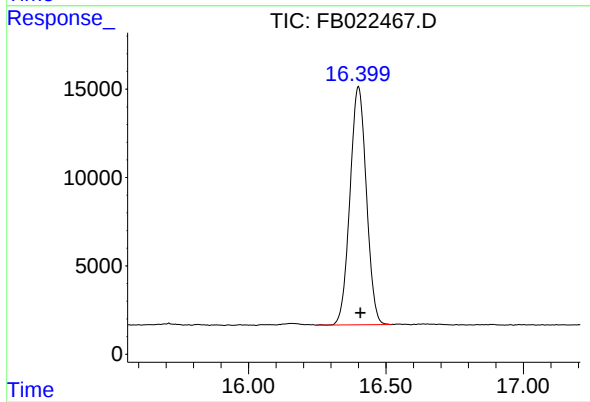

#10 1,2,4-Trimethylbenzene

R.T.: 16.400 min
Delta R.T.: -0.007 min
Response: 558485
Conc: 21.42 ng/ml