

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091322\
 Data File : FB028245.D
 Signal(s) : FID2B.CH
 Acq On : 13 Sep 2022 10:59
 Operator : AJ/MA
 Sample : BSF0913S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0913S1

Integration File: Calibration.e
 Quant Time: Sep 14 12:36:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	229144	19.145 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	585265	28.906 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	612419	29.113 ng/ml
3) t n-Heptane	7.758	200507	9.327 ng/ml
4) t Benzene	7.895	237227	9.643 ng/ml
6) t Toluene	10.628	684535	29.403 ng/ml
7) t Ethylbenzene	13.065	210560	9.468 ng/ml
8) t m-Xylene	13.197	419965	19.245 ng/ml
9) t O-Xylene	13.924	406770	19.414 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	398694	19.829 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091322\
Data File : FB028245.D
Signal(s) : FID2B.CH
Acq On : 13 Sep 2022 10:59
Operator : AJ/MA
Sample : BSF0913S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0913S1

Integration File: Calibration.e
Quant Time: Sep 14 12:36:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

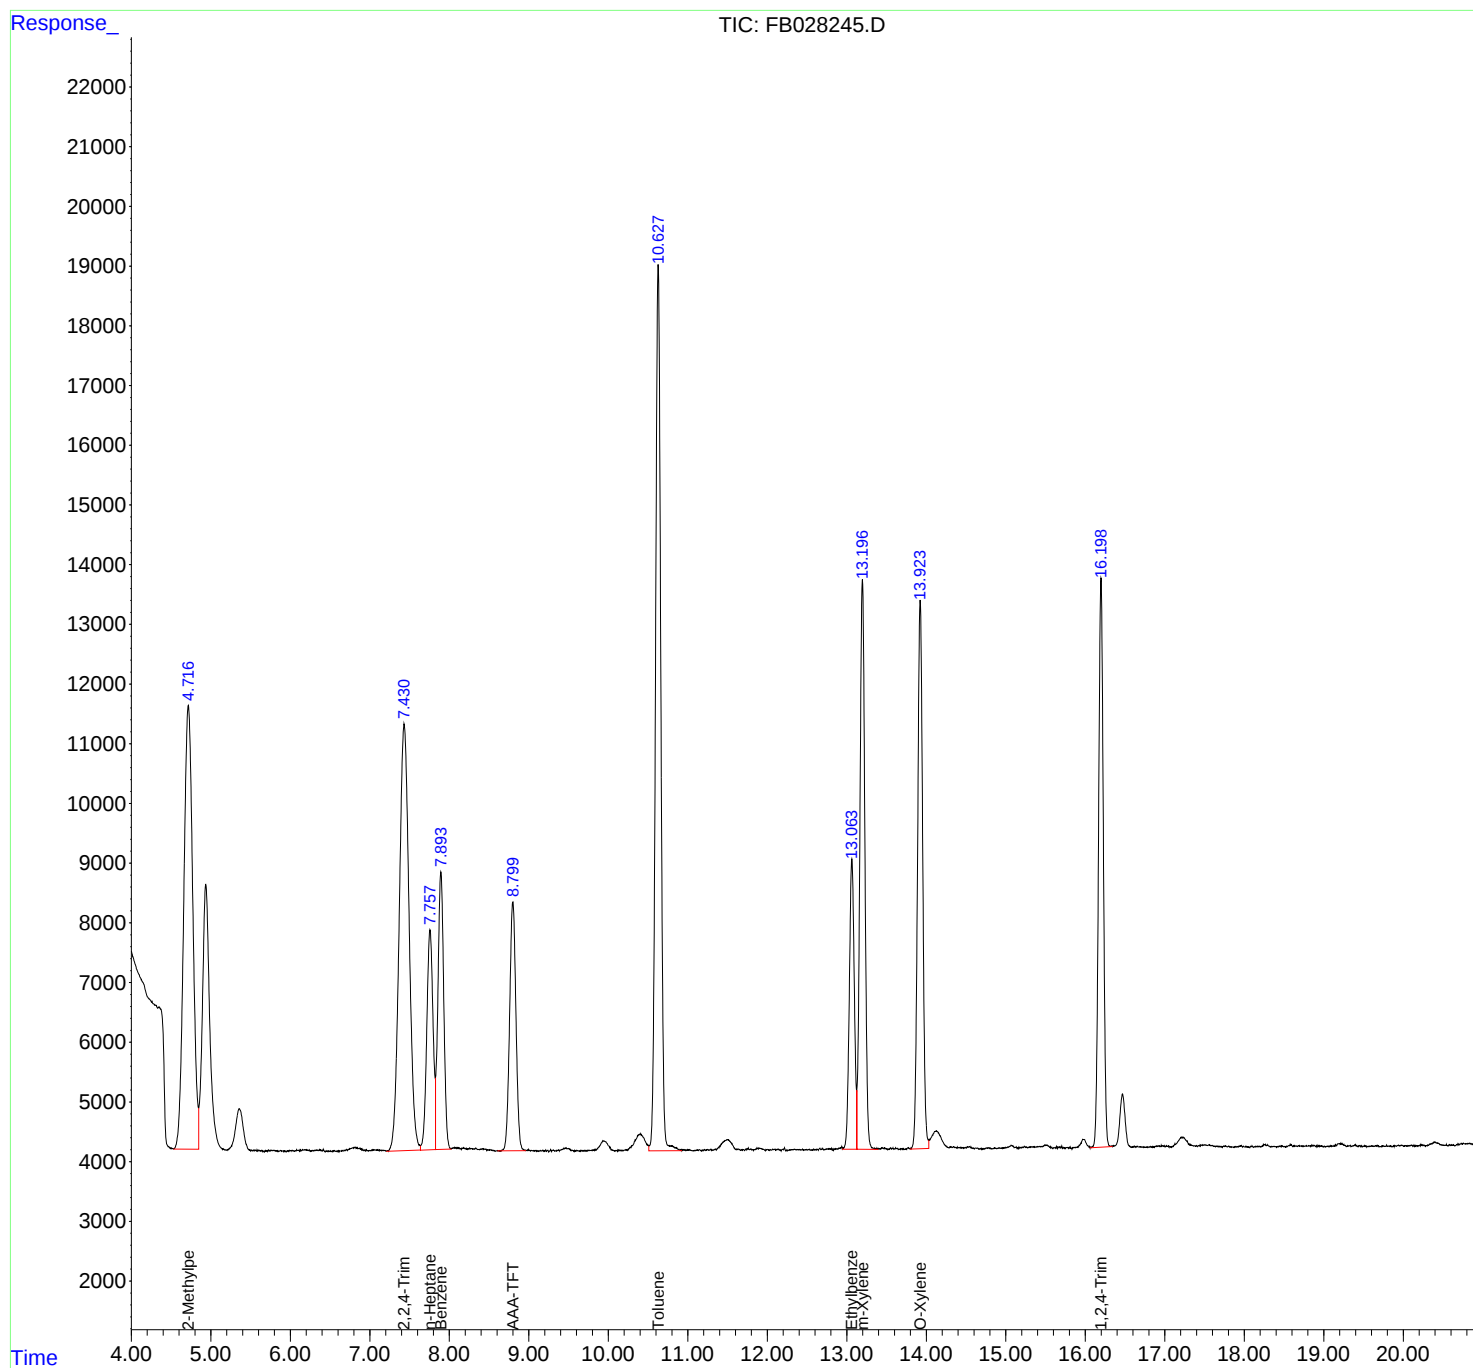


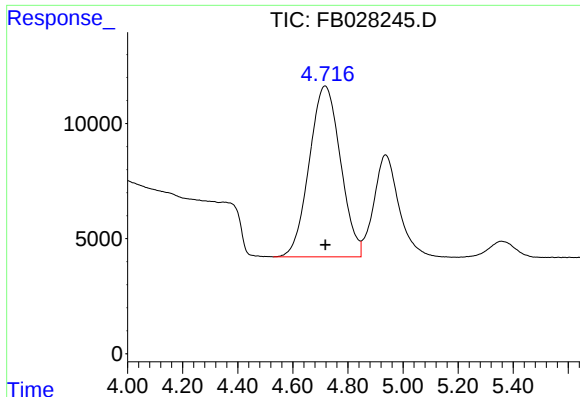

#1 2-Methylpentane


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 585265
Conc: 28.91 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0913S1

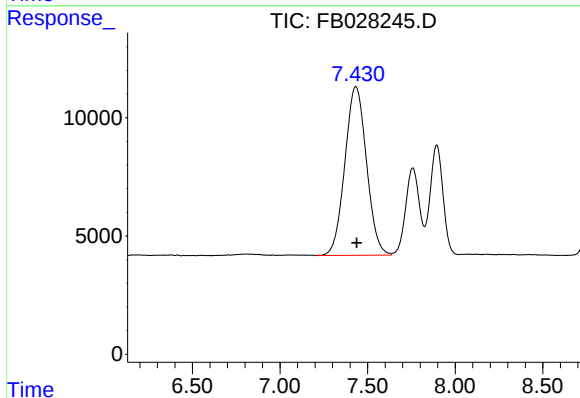


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
Delta R.T.: -0.005 min
Response: 612419
Conc: 29.11 ng/ml

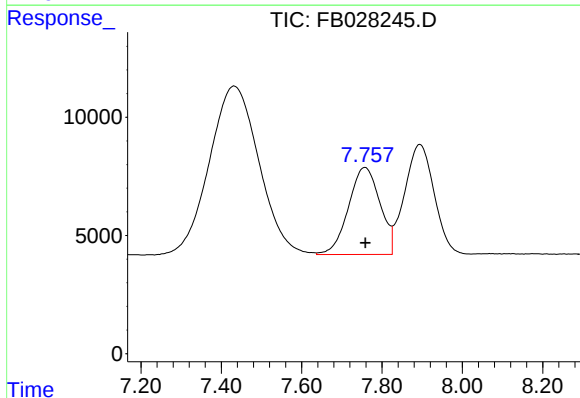


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 200507
Conc: 9.33 ng/ml

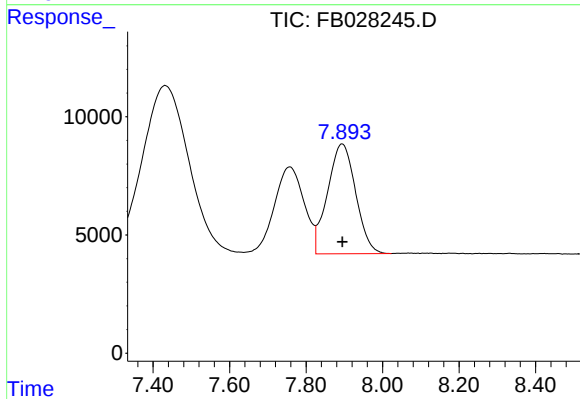

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 237227
Conc: 9.64 ng/ml

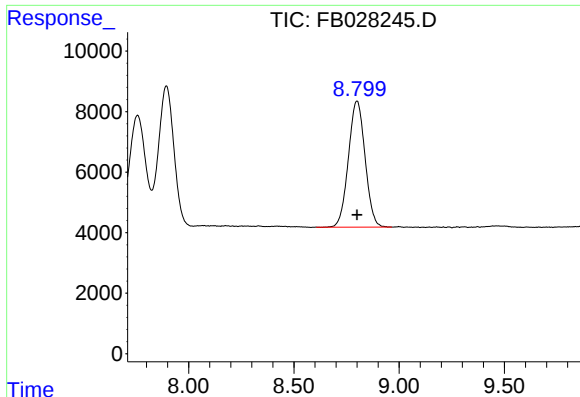

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 229144
Conc: 19.15 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0913S1

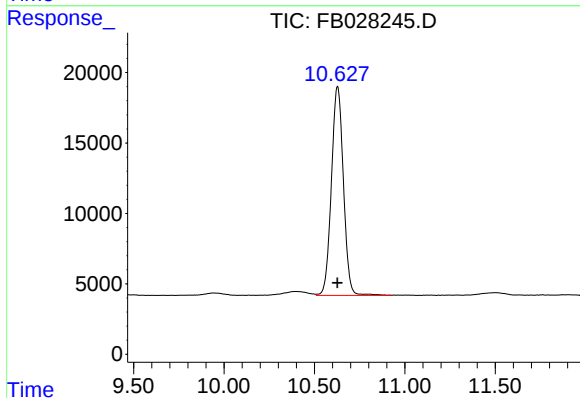


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 684535
Conc: 29.40 ng/ml

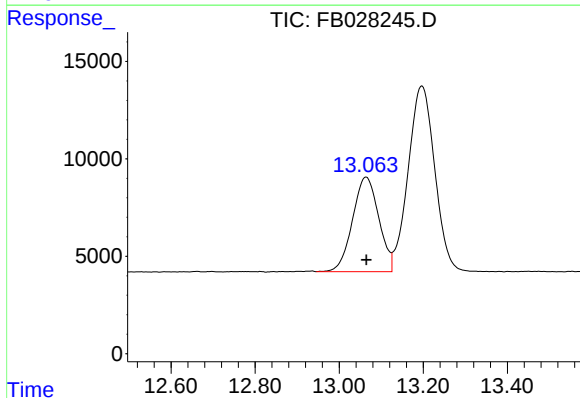


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: 0.000 min
Response: 210560
Conc: 9.47 ng/ml

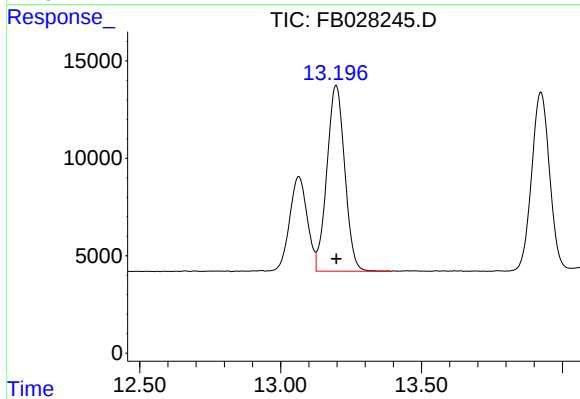

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.000 min
Response: 419965
Conc: 19.24 ng/ml

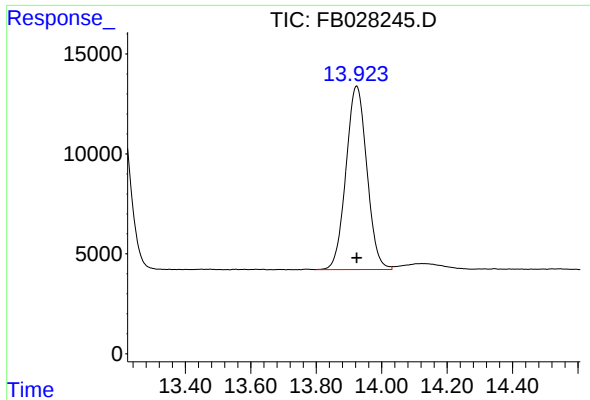

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.000 min
Response: 406770
Conc: 19.41 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0913S1

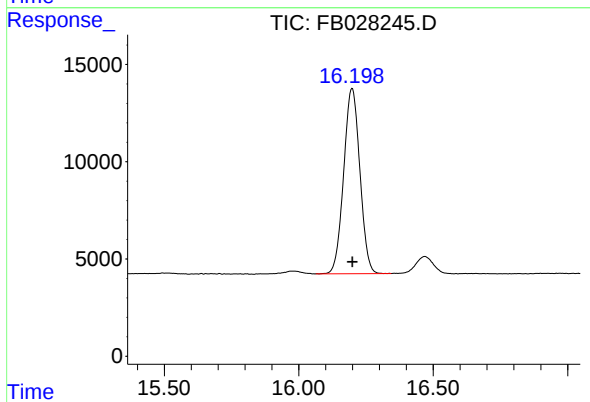

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.000 min
Response: 398694
Conc: 19.83 ng/ml