

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091322\
 Data File : FB028253.D
 Signal(s) : FID2B.CH
 Acq On : 13 Sep 2022 20:48
 Operator : AJ/MA
 Sample : N4569-02MS 50X
 Misc : 5.02G/5.00 ML MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-T-6-(5-10)MS

Integration File: Calibration.e
 Quant Time: Sep 14 12:37:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	214876	17.953 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	536393	26.492 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	581993	27.666 ng/ml
3) t n-Heptane	7.754	195288	9.085 ng/ml
4) t Benzene	7.891	263133	10.696 ng/ml
6) t Toluene	10.626	706491	30.346 ng/ml
7) t Ethylbenzene	13.064	217785	9.793 ng/ml
8) t m-Xylene	13.197	428396	19.631 ng/ml
9) t O-Xylene	13.924	418712	19.984 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	380514	18.924 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091322\
Data File : FB028253.D
Signal(s) : FID2B.CH
Acq On : 13 Sep 2022 20:48
Operator : AJ/MA
Sample : N4569-02MS 50X
Misc : 5.02G/5.00 ML MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-T-6-(5-10)MS

Integration File: Calibration.e
Quant Time: Sep 14 12:37:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

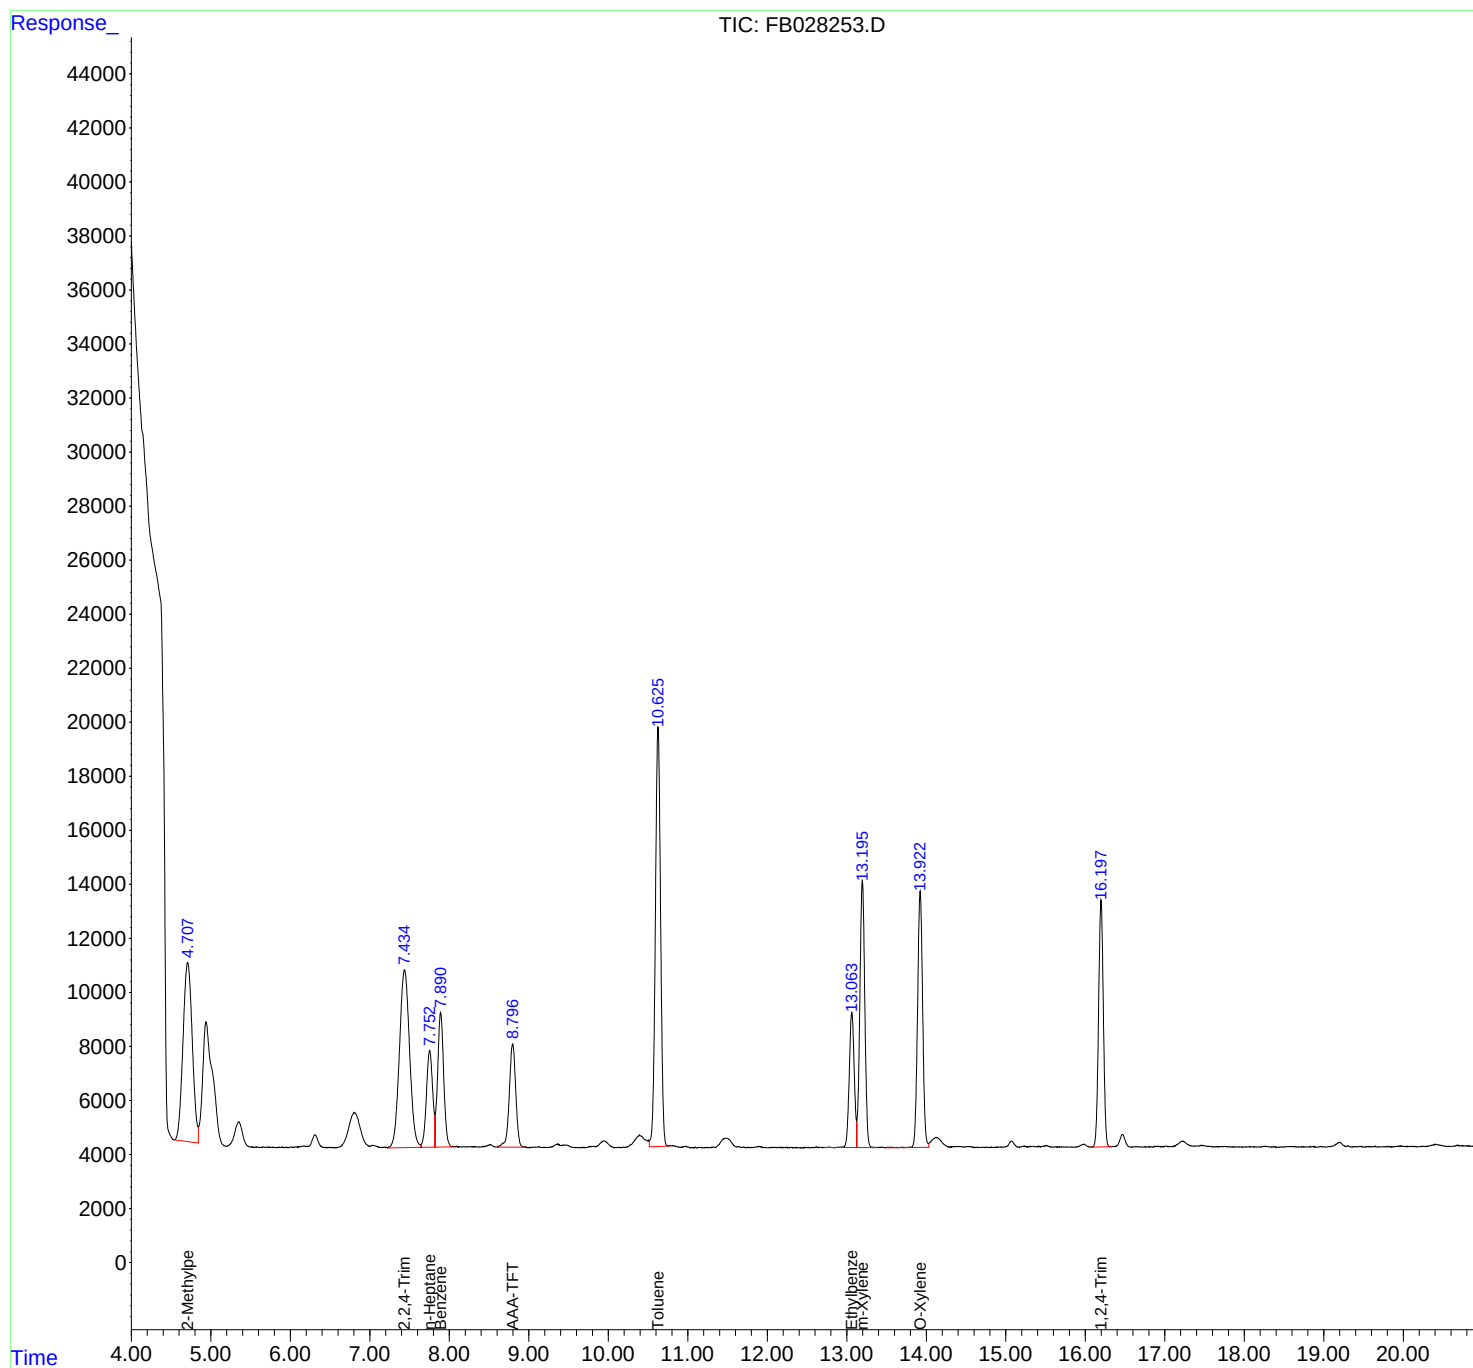


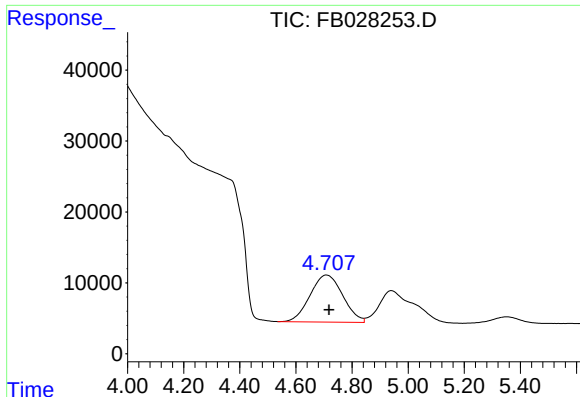

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: -0.009 min
Response: 536393
Conc: 26.49 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-6-(5-10)MS

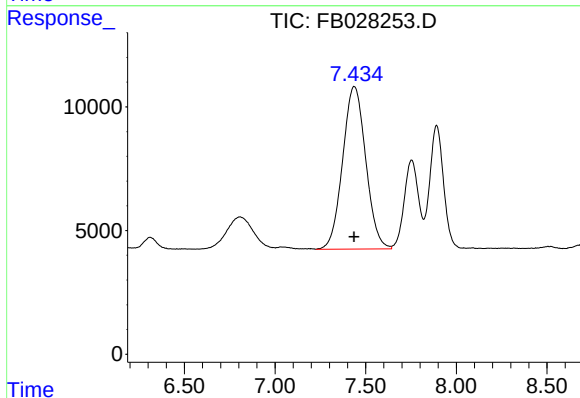


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: -0.002 min
Response: 581993
Conc: 27.67 ng/ml

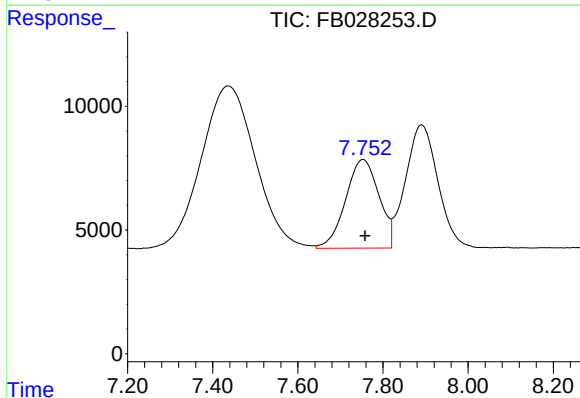


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 195288
Conc: 9.08 ng/ml

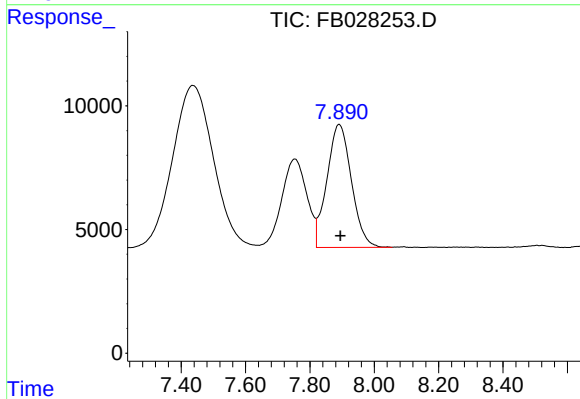

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.004 min
Response: 263133
Conc: 10.70 ng/ml

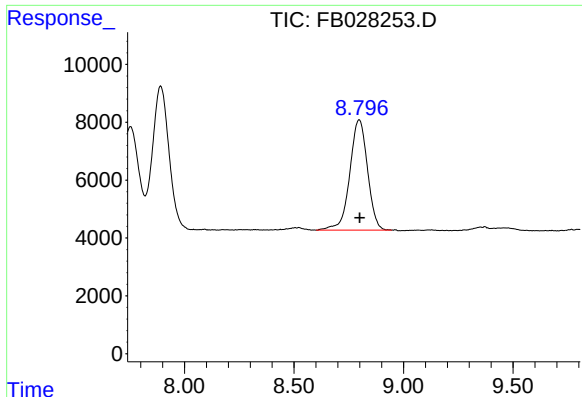

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.002 min
Response: 214876
Conc: 17.95 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-6-(5-10)MS

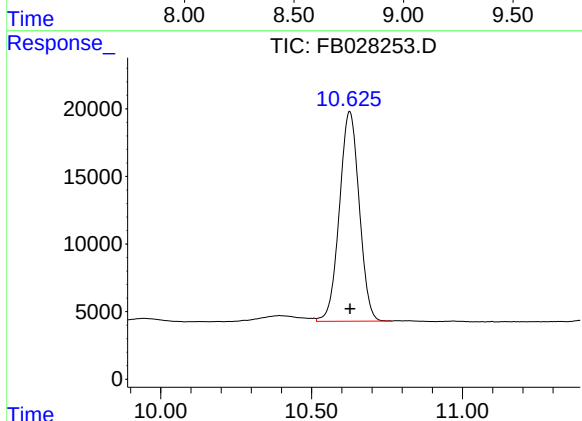


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.002 min
Response: 706491
Conc: 30.35 ng/ml

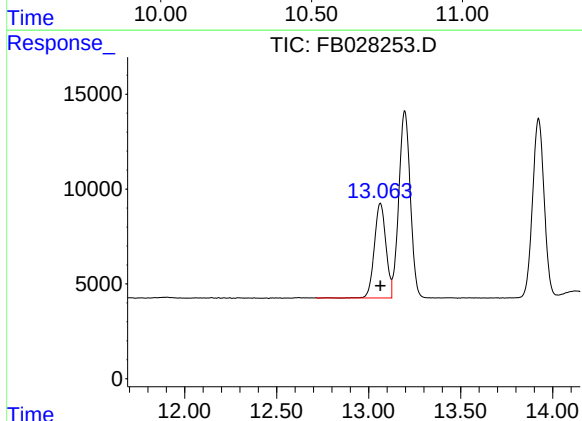


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.000 min
Response: 217785
Conc: 9.79 ng/ml

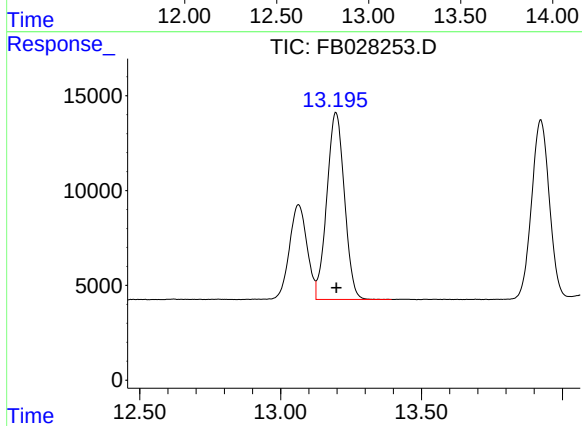

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.000 min
Response: 428396
Conc: 19.63 ng/ml

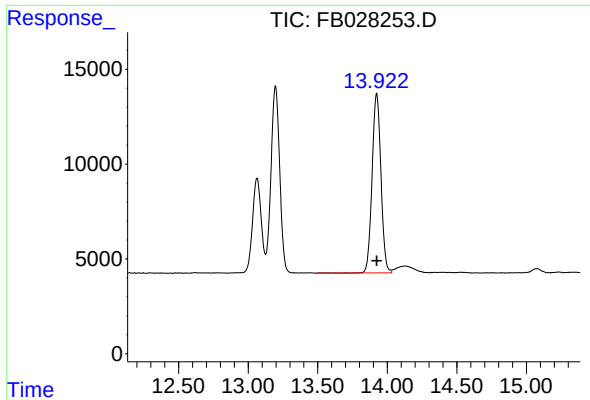

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.000 min
Response: 418712
Conc: 19.98 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-6-(5-10)MS

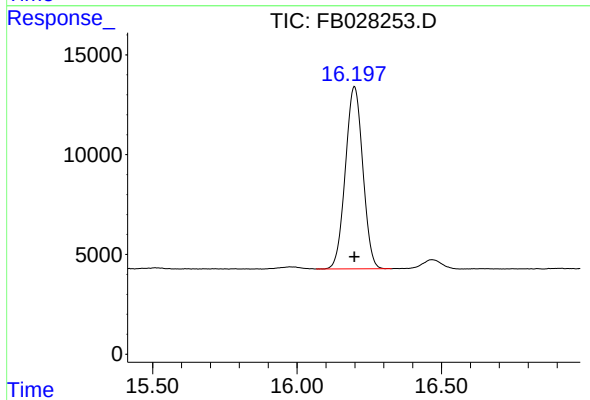

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.000 min
Response: 380514
Conc: 18.92 ng/ml