

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091418\
 Data File : FB017714.D
 Signal(s) : FID2B.CH
 Acq On : 14 Sep 2018 15:08
 Operator : MJ/SJ
 Sample : BSF0914S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 17 07:48:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.109	178088	21.053 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.961	492574	30.930 ng/ml
2) t 2,2,4-Trimethylpentane	7.726	470958	29.595 ng/ml
3) t n-Heptane	8.065	152692	9.908 ng/ml
4) t Benzene	8.204	196176	10.305 ng/ml
6) t Toluene	10.959	473126	29.895 ng/ml
7) t Ethylbenzene	13.409	167070	10.225 ng/ml
8) t m-Xylene	13.541	356977	20.635 ng/ml
9) t O-Xylene	14.273	374766	20.623 ng/ml
10) t 1,2,4-Trimethylbenzene	16.555	431256	20.274 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091418\
Data File : FB017714.D
Signal(s) : FID2B.CH
Acq On : 14 Sep 2018 15:08
Operator : MJ/SJ
Sample : BSF0914S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 17 07:48:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

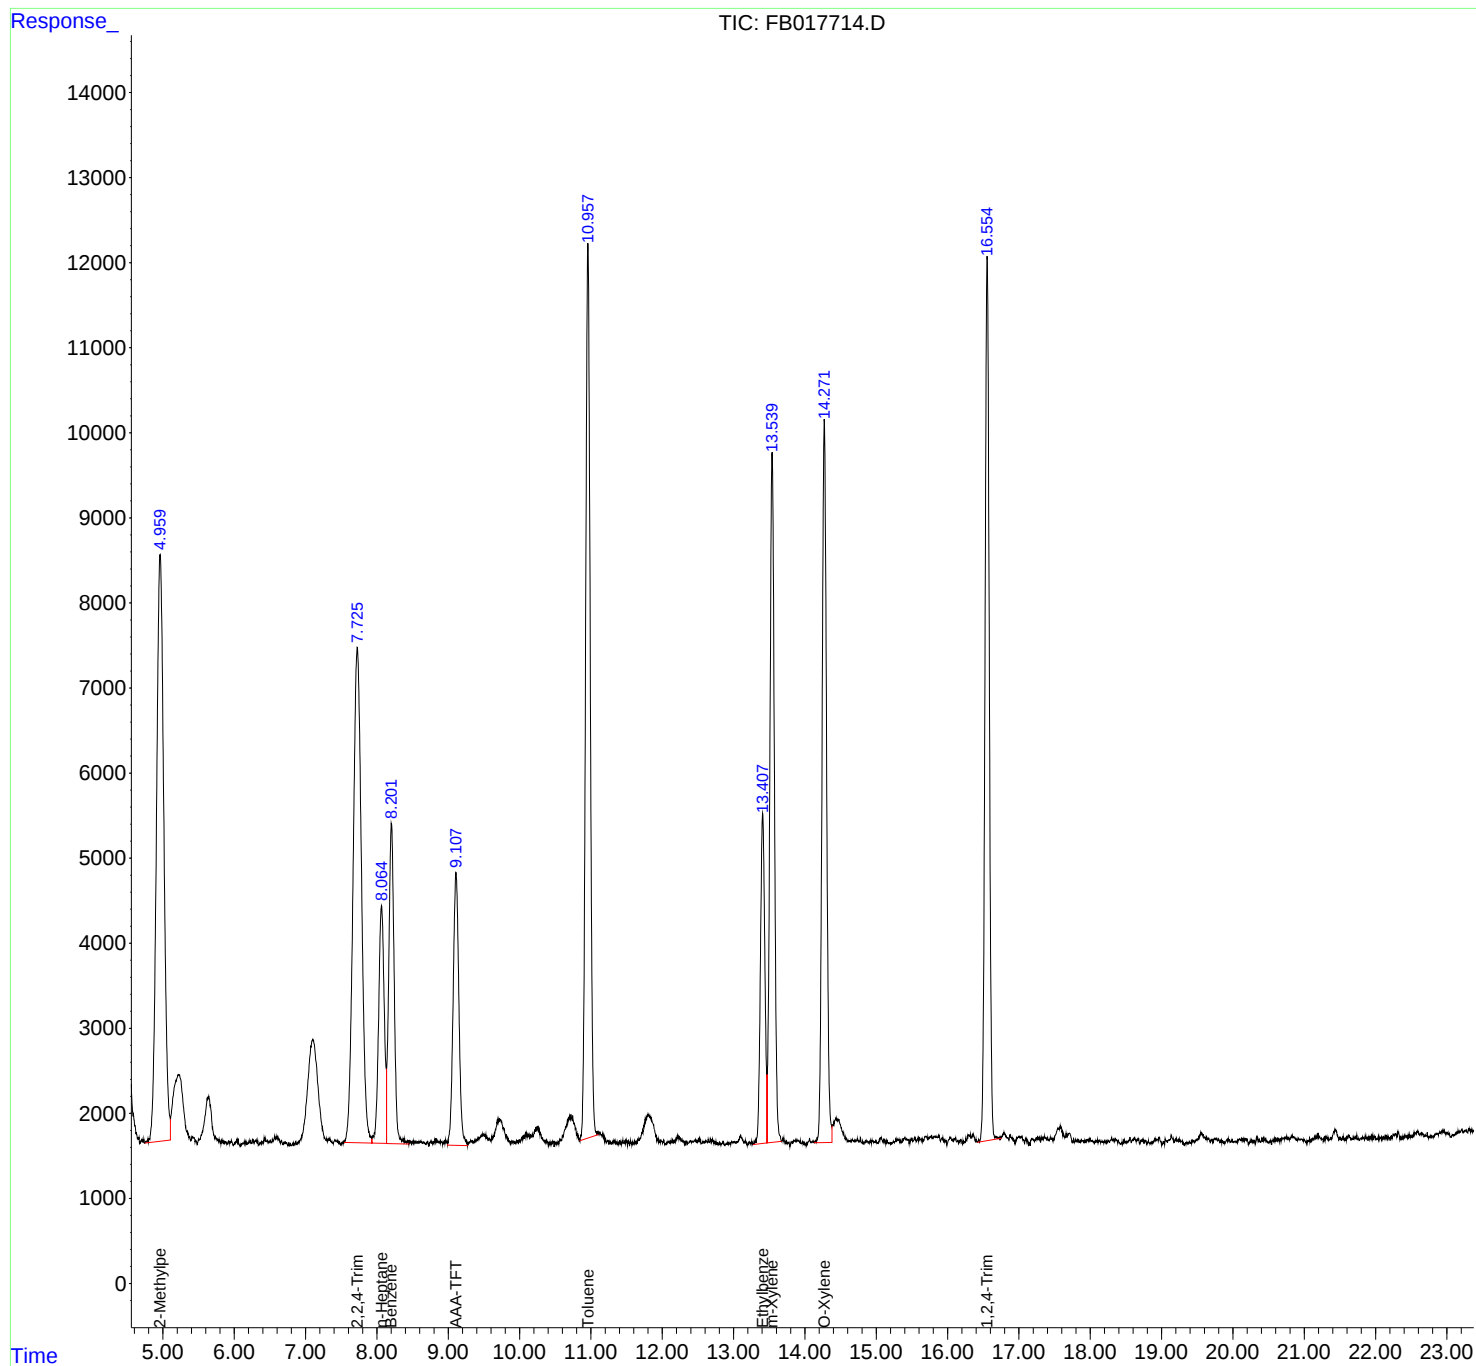

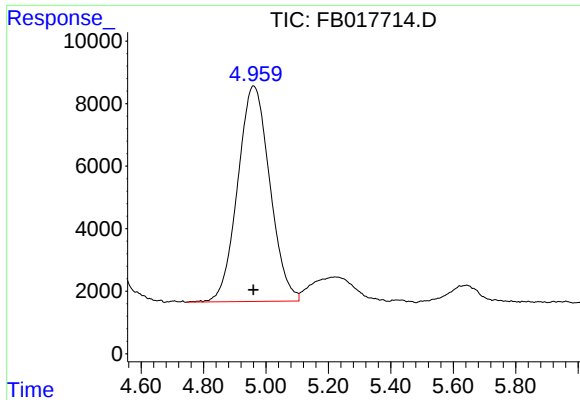


#1 2-Methylpentane

R.T.: 4.961 min
Delta R.T.: 0.000 min
Response: 492574
Conc: 30.93 ng/ml

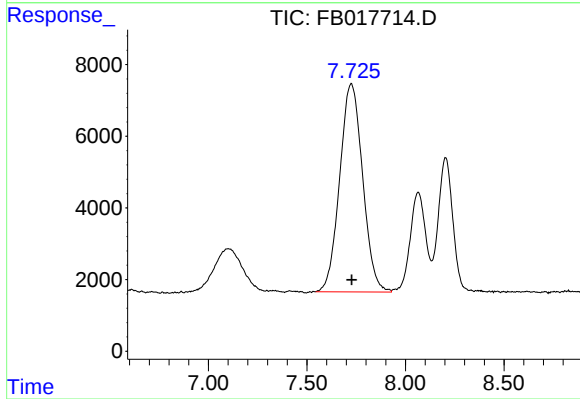


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: -0.001 min
Response: 470958
Conc: 29.59 ng/ml

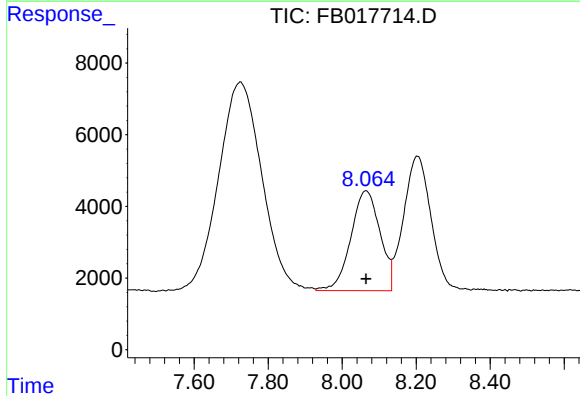


#3 n-Heptane

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 152692
Conc: 9.91 ng/ml

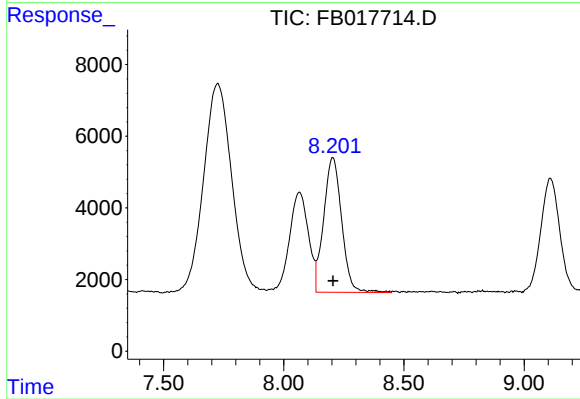


#4 Benzene

R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 196176
Conc: 10.31 ng/ml

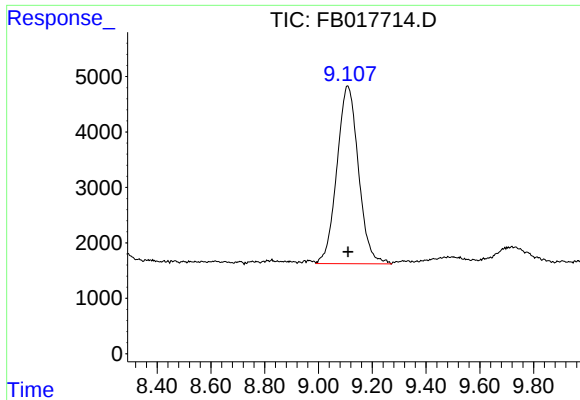


#5 AAA-TFT

R.T.: 9.109 min
Delta R.T.: 0.000 min
Response: 178088
Conc: 21.05 ng/ml

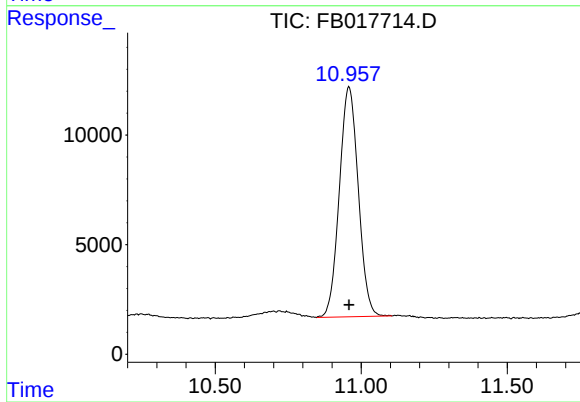


#6 Toluene

R.T.: 10.959 min
Delta R.T.: 0.000 min
Response: 473126
Conc: 29.90 ng/ml

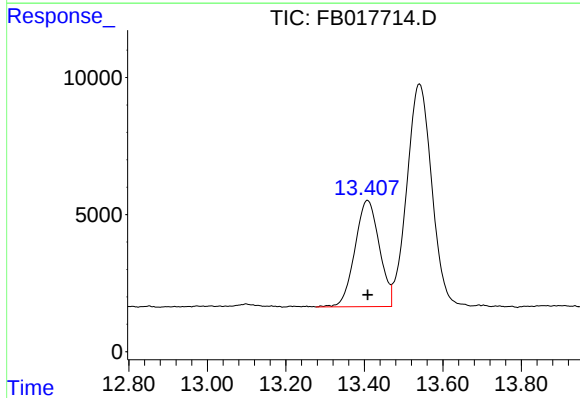


#7 Ethylbenzene

R.T.: 13.409 min
Delta R.T.: 0.000 min
Response: 167070
Conc: 10.22 ng/ml

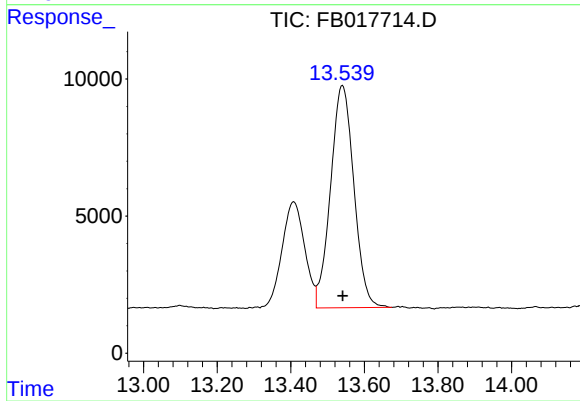


#8 m-Xylene

R.T.: 13.541 min
Delta R.T.: 0.000 min
Response: 356977
Conc: 20.63 ng/ml

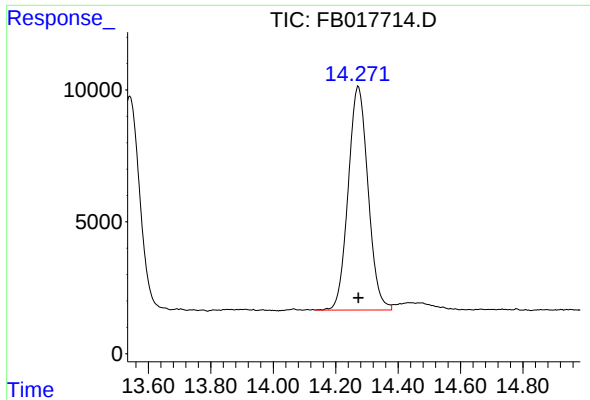

#9 O-Xylene

R.T.: 14.273 min
Delta R.T.: 0.000 min
Response: 374766
Conc: 20.62 ng/ml

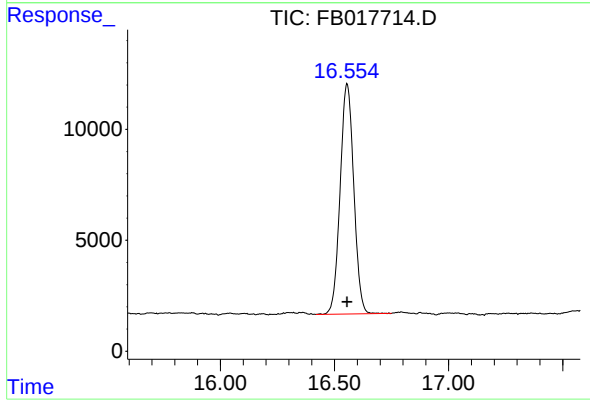

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: 0.000 min
Response: 431256
Conc: 20.27 ng/ml