

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091422\
 Data File : FB028260.D
 Signal(s) : FID2B.CH
 Acq On : 14 Sep 2022 12:53
 Operator : AJ/MA
 Sample : BSF0914S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0914S1

Integration File: Calibration.e
 Quant Time: Sep 15 10:56:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	200306	16.736 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	516014	25.486 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	583782	27.751 ng/ml
3) t n-Heptane	7.754	164627	7.658 ng/ml
4) t Benzene	7.891	205991	8.373 ng/ml
6) t Toluene	10.624	602459	25.877 ng/ml
7) t Ethylbenzene	13.061	193722	8.711 ng/ml
8) t m-Xylene	13.193	385572	17.668 ng/ml
9) t O-Xylene	13.920	386618	18.453 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	405837	20.184 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091422\
Data File : FB028260.D
Signal(s) : FID2B.CH
Acq On : 14 Sep 2022 12:53
Operator : AJ/MA
Sample : BSF0914S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0914S1

Integration File: Calibration.e
Quant Time: Sep 15 10:56:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

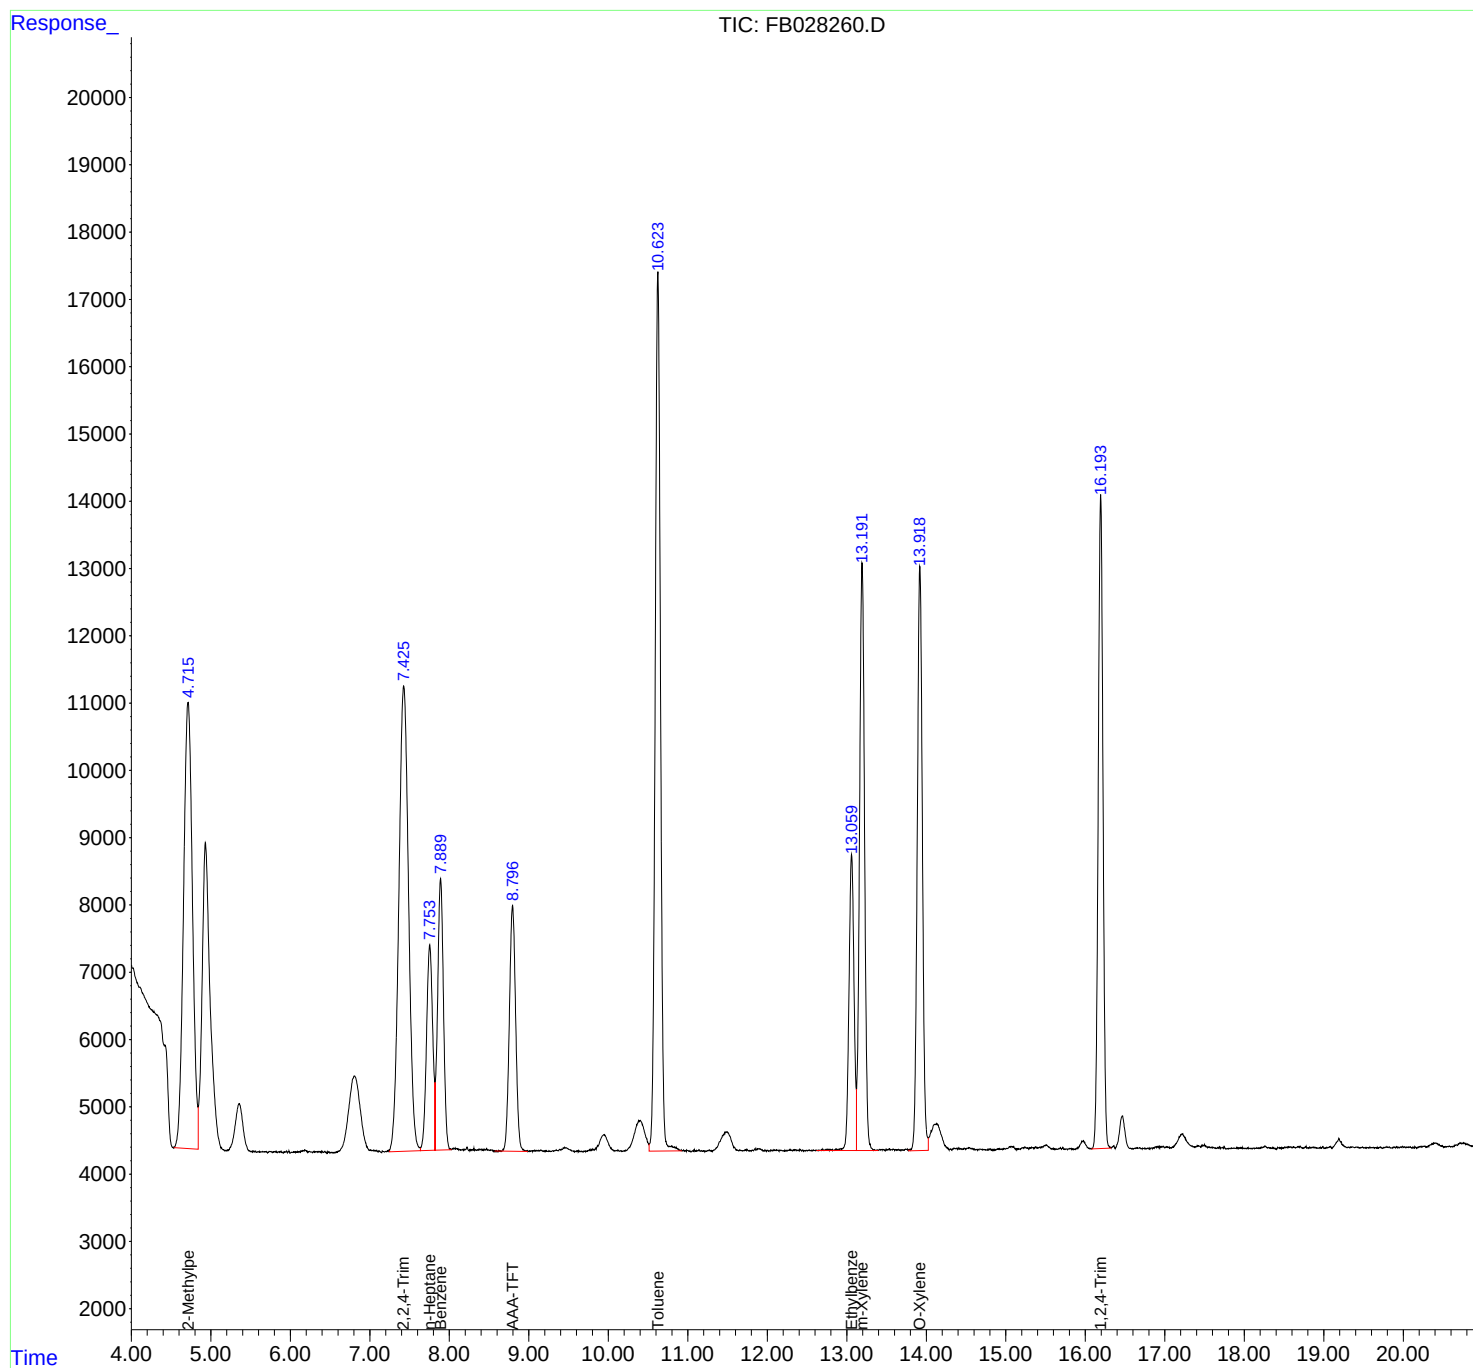


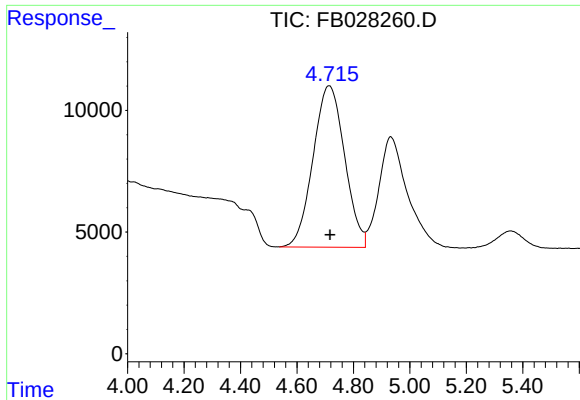

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: -0.003 min
Response: 516014
Conc: 25.49 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0914S1

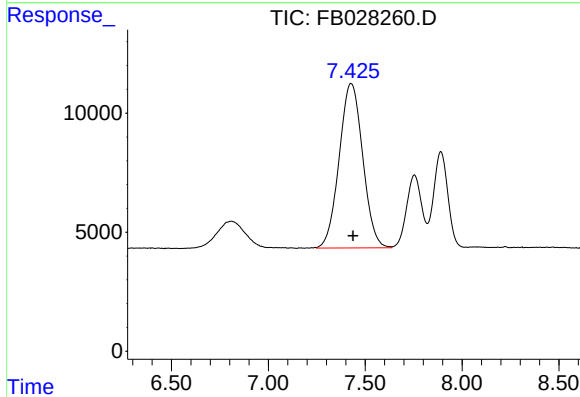


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: -0.011 min
Response: 583782
Conc: 27.75 ng/ml

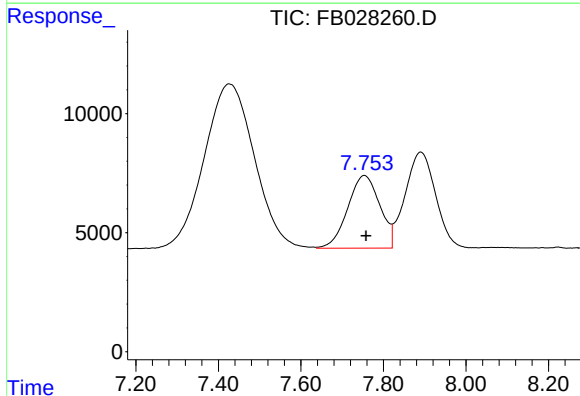


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 164627
Conc: 7.66 ng/ml

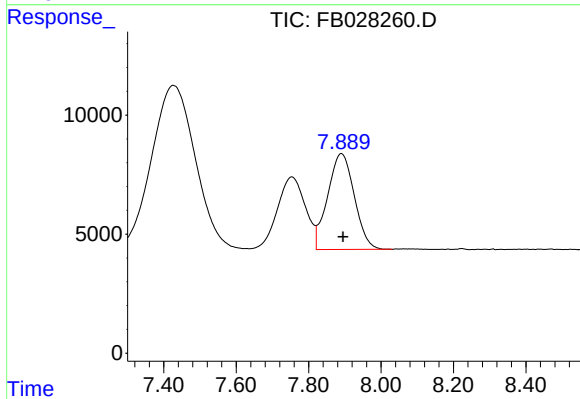

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.004 min
Response: 205991
Conc: 8.37 ng/ml

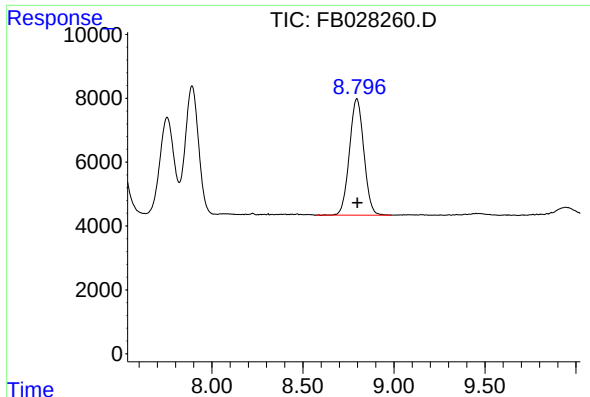

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 200306
Conc: 16.74 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0914S1

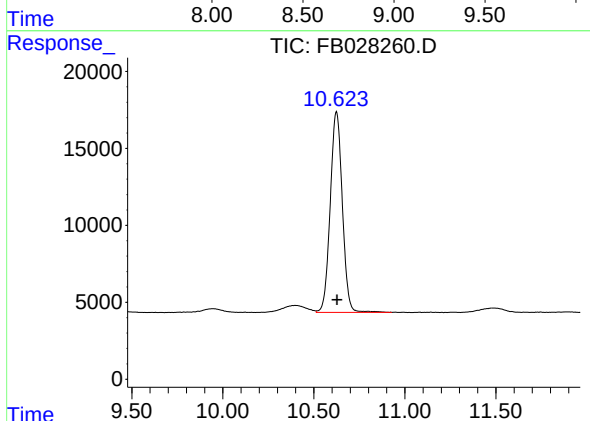


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.004 min
Response: 602459
Conc: 25.88 ng/ml

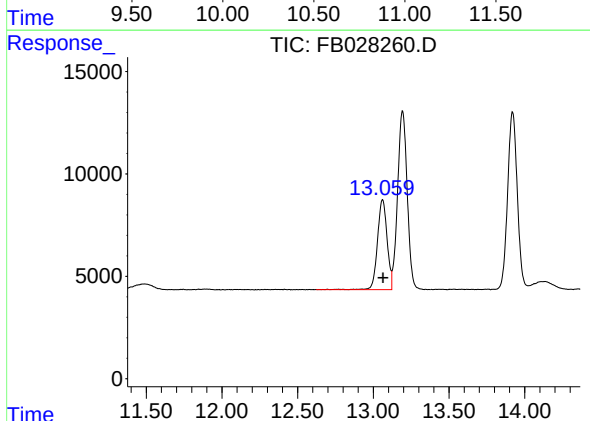


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: -0.004 min
Response: 193722
Conc: 8.71 ng/ml

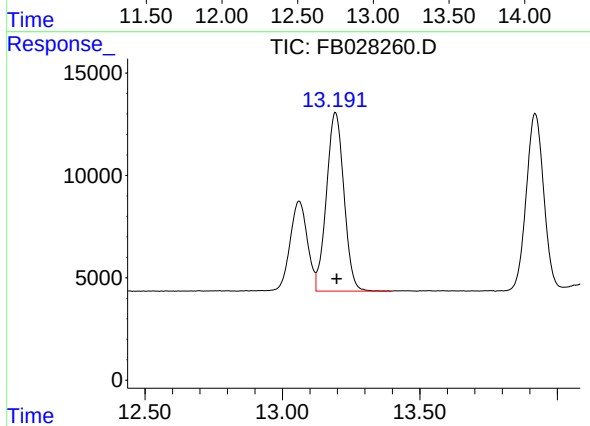

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: -0.004 min
Response: 385572
Conc: 17.67 ng/ml

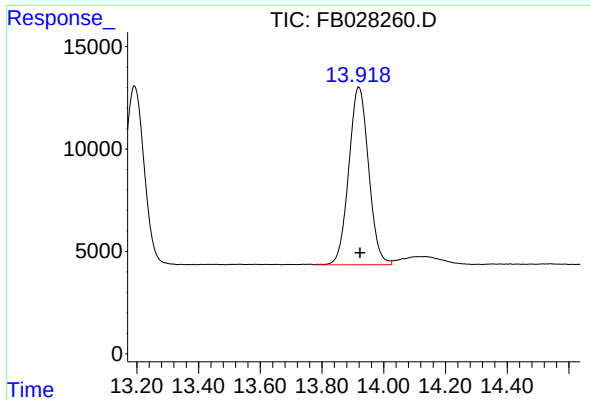

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: -0.004 min
Response: 386618
Conc: 18.45 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0914S1

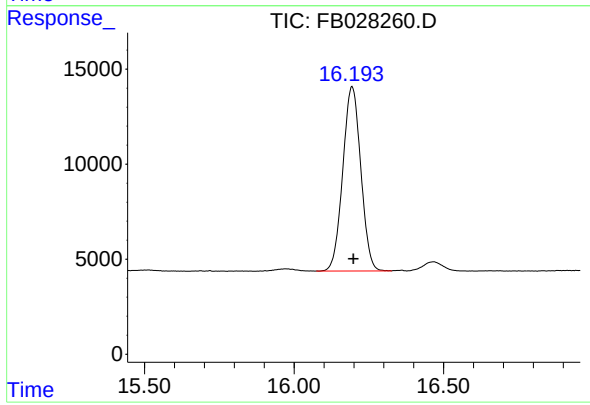

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: -0.005 min
Response: 405837
Conc: 20.18 ng/ml