

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091422\
 Data File : FB028268.D
 Signal(s) : FID2B.CH
 Acq On : 14 Sep 2022 21:14
 Operator : AJ/MA
 Sample : BSF0914S2
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0914S2

Integration File: Calibration.e
 Quant Time: Sep 15 10:57:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	225125	18.809 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	543712	26.854 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	593474	28.212 ng/ml
3) t n-Heptane	7.756	188908	8.788 ng/ml
4) t Benzene	7.893	230618	9.374 ng/ml
6) t Toluene	10.626	658009	28.263 ng/ml
7) t Ethylbenzene	13.062	210168	9.451 ng/ml
8) t m-Xylene	13.194	415477	19.039 ng/ml
9) t O-Xylene	13.922	403627	19.264 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	389593	19.376 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091422\
Data File : FB028268.D
Signal(s) : FID2B.CH
Acq On : 14 Sep 2022 21:14
Operator : AJ/MA
Sample : BSF0914S2
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0914S2

Integration File: Calibration.e
Quant Time: Sep 15 10:57:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

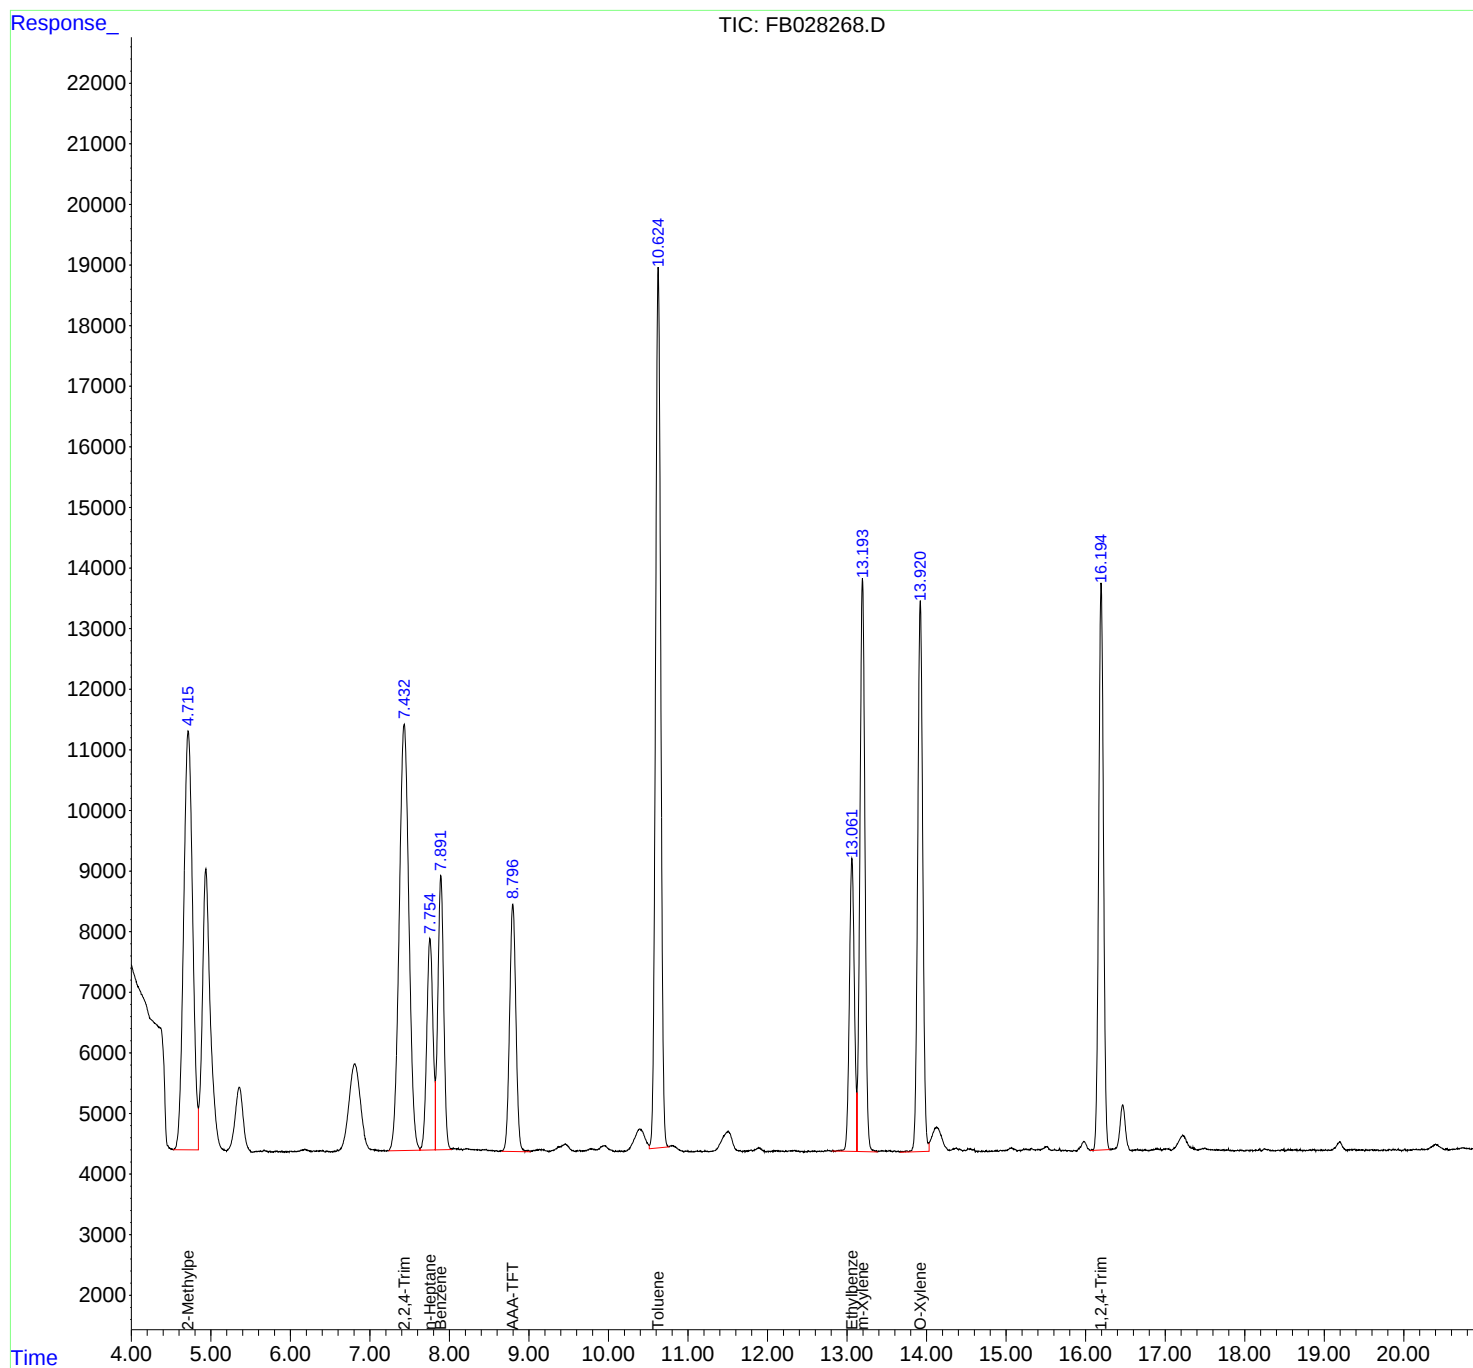


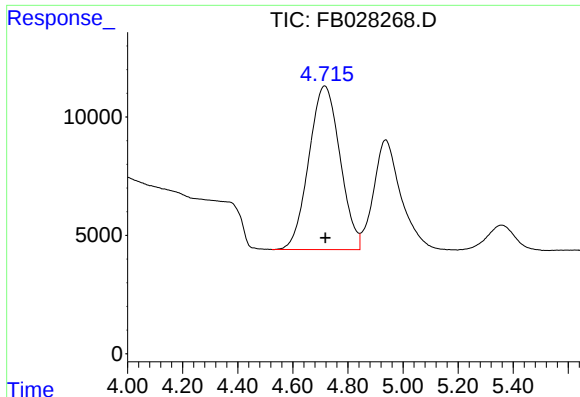

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: -0.002 min
Response: 543712
Conc: 26.85 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0914S2

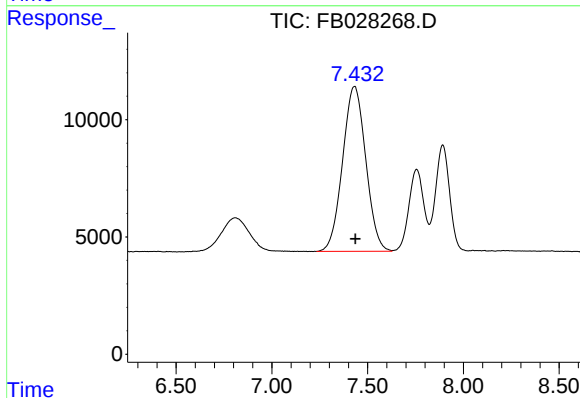


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: -0.004 min
Response: 593474
Conc: 28.21 ng/ml

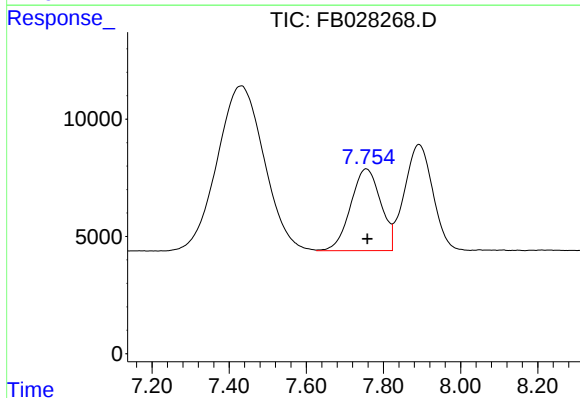


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.003 min
Response: 188908
Conc: 8.79 ng/ml

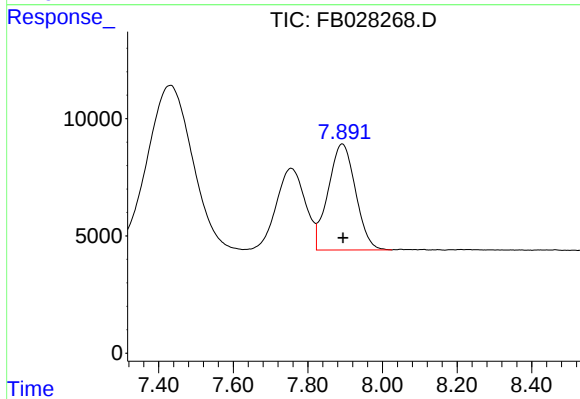

#4 Benzene


R.T.: 7.893 min
Delta R.T.: -0.002 min
Response: 230618
Conc: 9.37 ng/ml

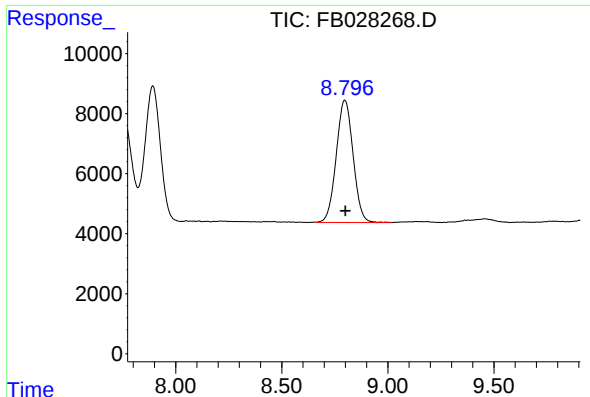

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.003 min
Response: 225125
Conc: 18.81 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0914S2

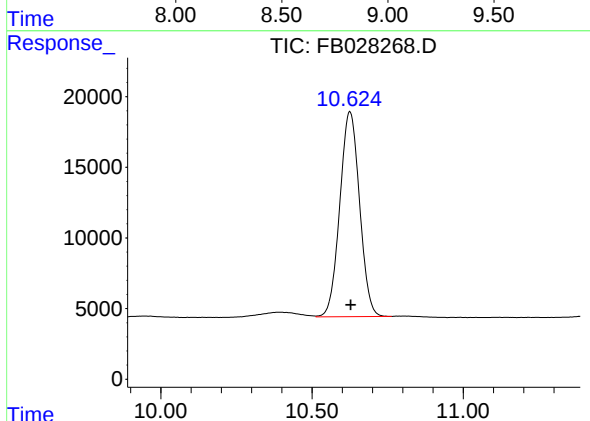


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.002 min
Response: 658009
Conc: 28.26 ng/ml

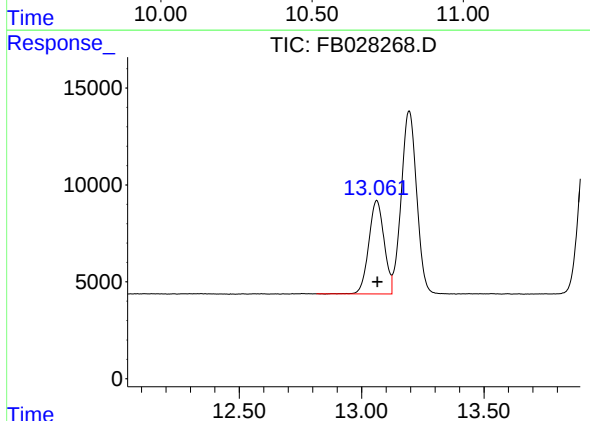


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.003 min
Response: 210168
Conc: 9.45 ng/ml

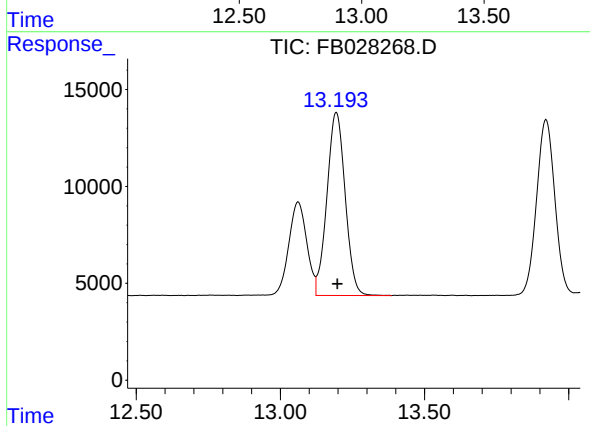

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: -0.003 min
Response: 415477
Conc: 19.04 ng/ml

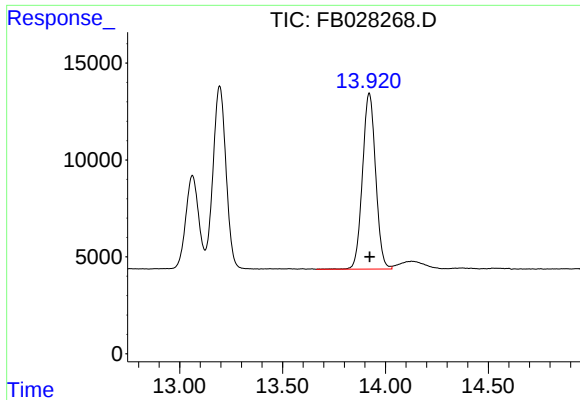

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.002 min
Response: 403627
Conc: 19.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0914S2

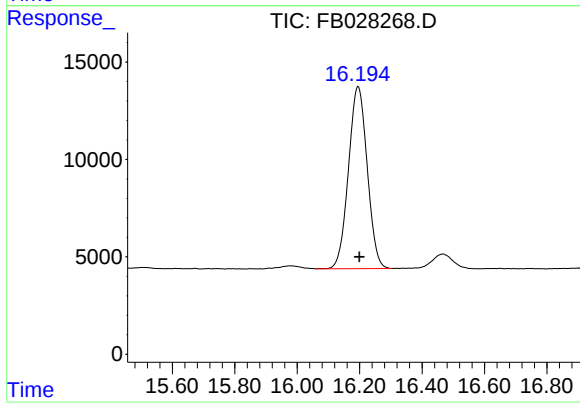

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: -0.003 min
Response: 389593
Conc: 19.38 ng/ml