

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091520\
 Data File : FB024877.D
 Signal(s) : FID2B.CH
 Acq On : 15 Sep 2020 20:22
 Operator : DD/AJ
 Sample : L4013-03MS
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 16 02:59:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
 Quant Title :
 QLast Update : Tue Sep 15 13:37:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.798	400222	17.986 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	776691	26.409 ng/ml
2) t	2,2,4-Trimethylpentane	7.416	626286	20.758 ng/ml
3) t	n-Heptane	7.757	214232	7.072 ng/ml
4) t	Benzene	7.891	359276	9.282 ng/ml
6) t	Toluene	10.628	981093	26.928 ng/ml
7) t	Ethylbenzene	13.068	299047	8.897 ng/ml
8) t	m-Xylene	13.201	584693	17.849 ng/ml
9) t	O-Xylene	13.929	567808	17.776 ng/ml
10) t	1,2,4-Trimethylbenzene	16.206	446196	17.110 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091520\
Data File : FB024877.D
Signal(s) : FID2B.CH
Acq On : 15 Sep 2020 20:22
Operator : DD/AJ
Sample : L4013-03MS
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 19 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 16 02:59:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
Quant Title :
QLast Update : Tue Sep 15 13:37:27 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

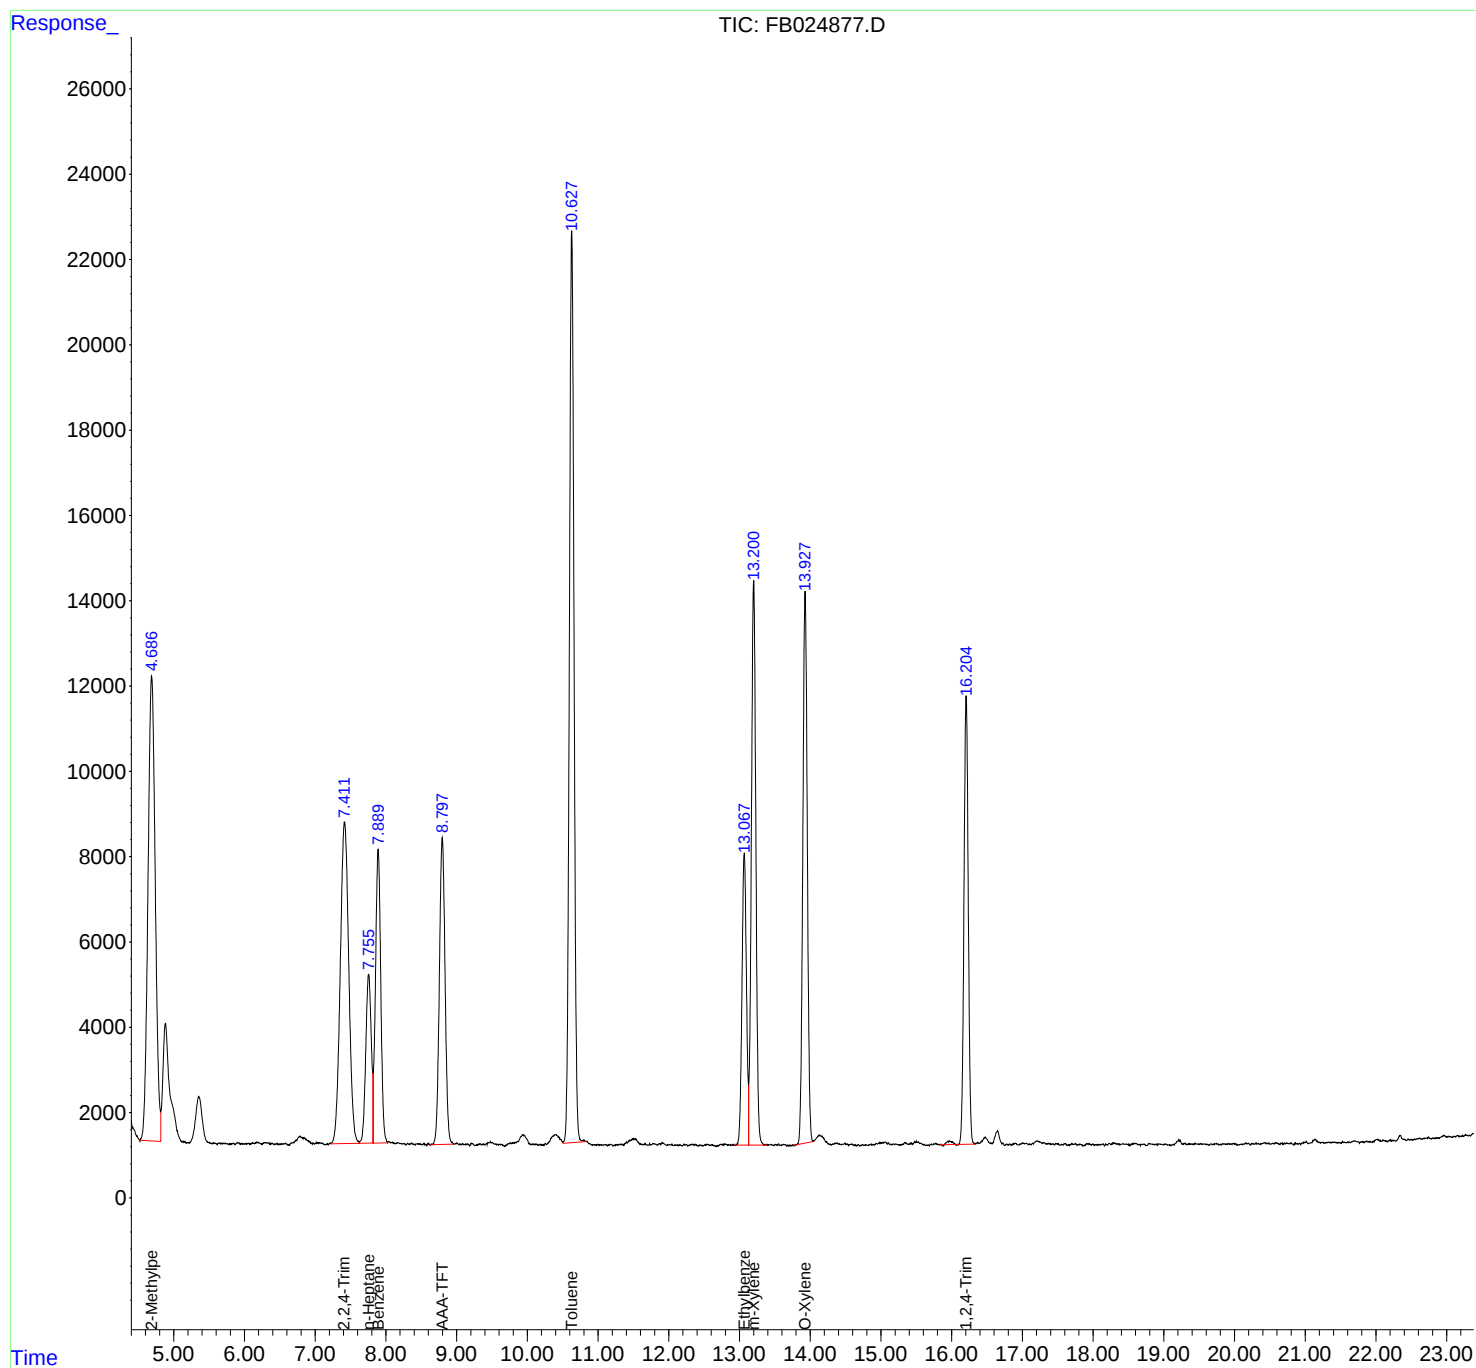

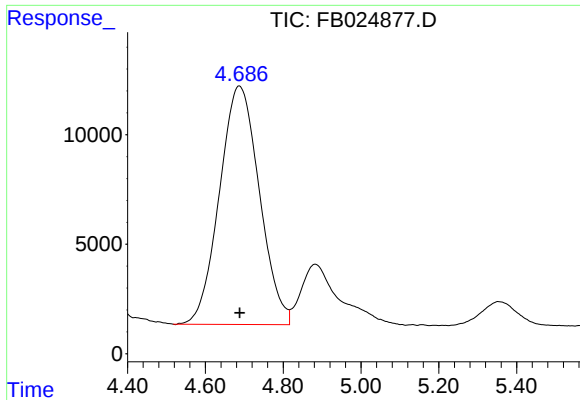


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 776691
Conc: 26.41 ng/ml

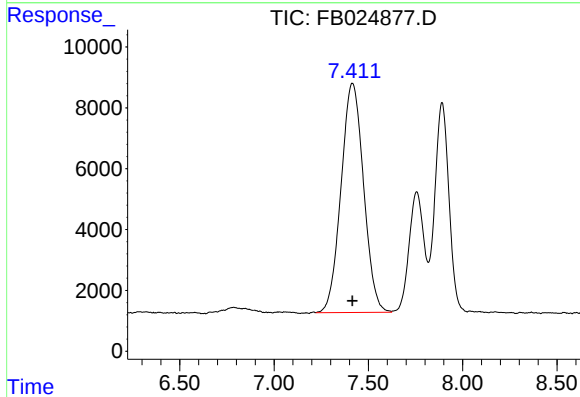


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 626286
Conc: 20.76 ng/ml

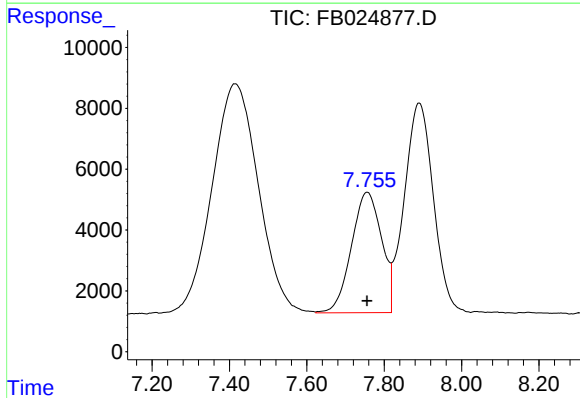


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.001 min
Response: 214232
Conc: 7.07 ng/ml

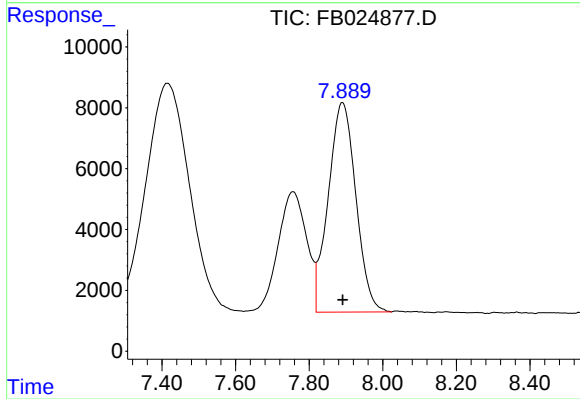


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 359276
Conc: 9.28 ng/ml

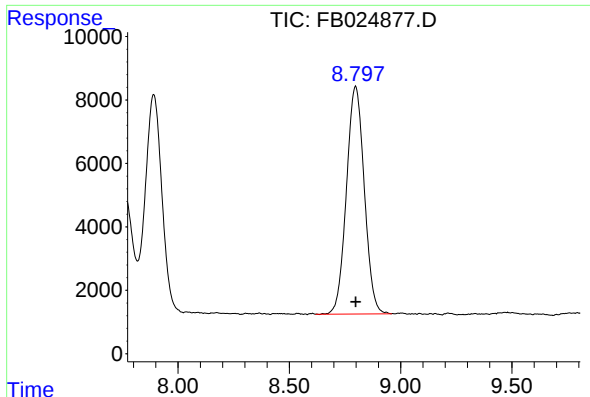


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 400222
Conc: 17.99 ng/ml

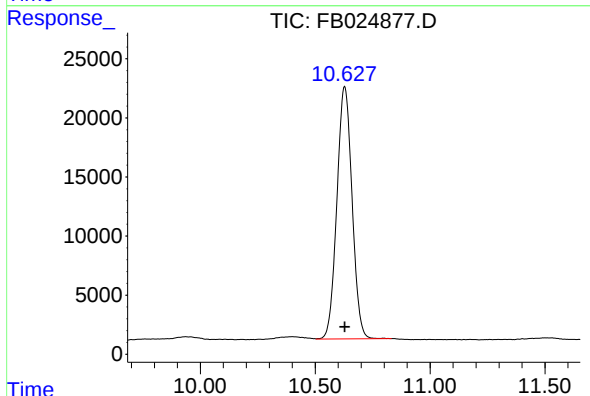


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 981093
Conc: 26.93 ng/ml

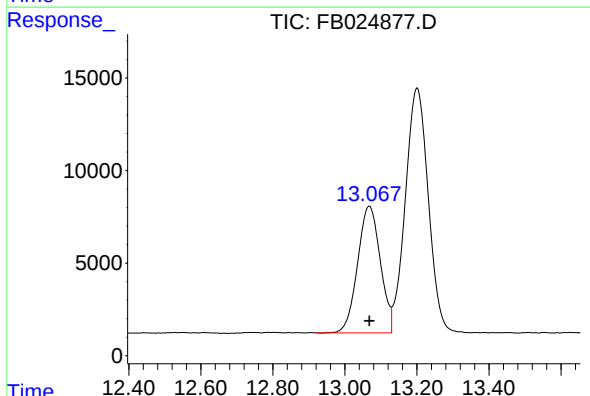


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: 0.000 min
Response: 299047
Conc: 8.90 ng/ml

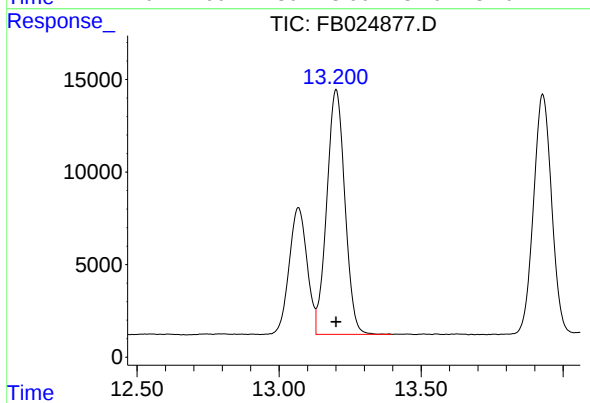


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 584693
Conc: 17.85 ng/ml

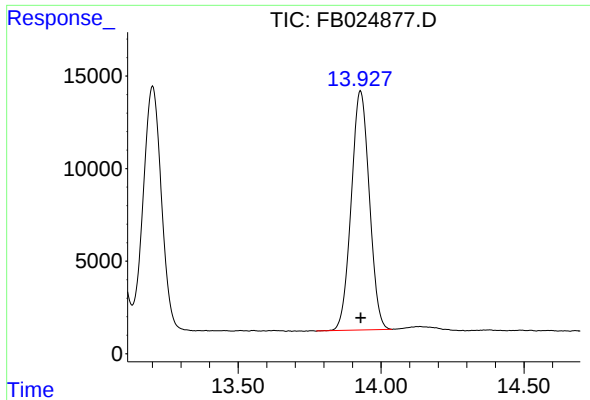

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.000 min
Response: 567808
Conc: 17.78 ng/ml

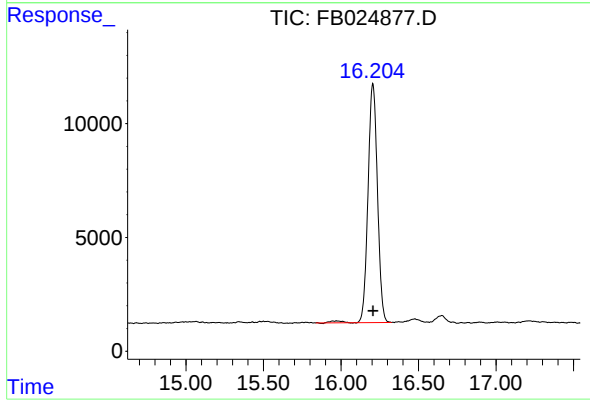

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.000 min
Response: 446196
Conc: 17.11 ng/ml