

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091520\
 Data File : FB024878.D
 Signal(s) : FID2B.CH
 Acq On : 15 Sep 2020 20:52
 Operator : DD/AJ
 Sample : L4013-03MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 16 03:00:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
 Quant Title :
 QLast Update : Tue Sep 15 13:37:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	343896	15.455 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	625762	21.277 ng/ml
2) t	2,2,4-Trimethylpentane	7.419	493618	16.361 ng/ml
3) t	n-Heptane	7.756	163768	5.406 ng/ml
4) t	Benzene	7.891	318188	8.221 ng/ml
6) t	Toluene	10.628	846518	23.234 ng/ml
7) t	Ethylbenzene	13.068	251857	7.493 ng/ml
8) t	m-Xylene	13.200	495648	15.131 ng/ml
9) t	O-Xylene	13.928	485823	15.210 ng/ml
10) t	1,2,4-Trimethylbenzene	16.206	377180	14.464 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091520\
Data File : FB024878.D
Signal(s) : FID2B.CH
Acq On : 15 Sep 2020 20:52
Operator : DD/AJ
Sample : L4013-03MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 16 03:00:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
Quant Title :
QLast Update : Tue Sep 15 13:37:27 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

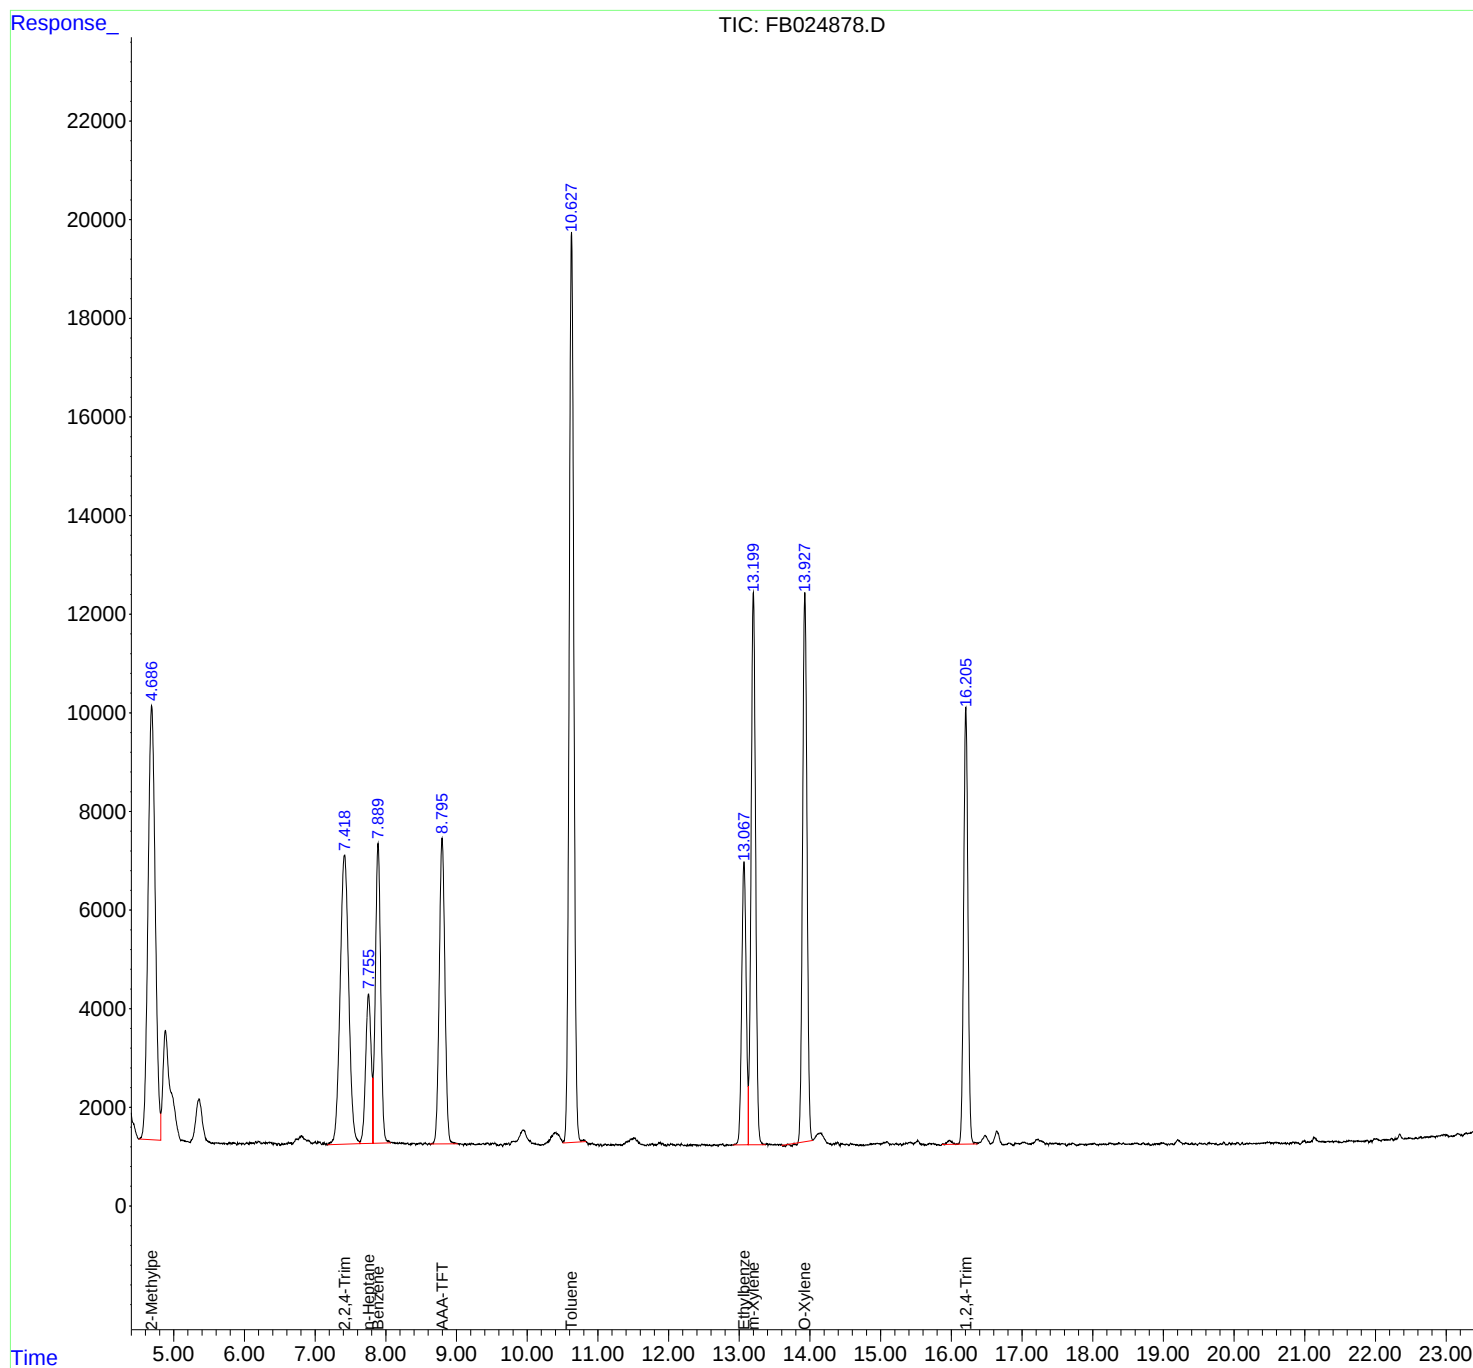

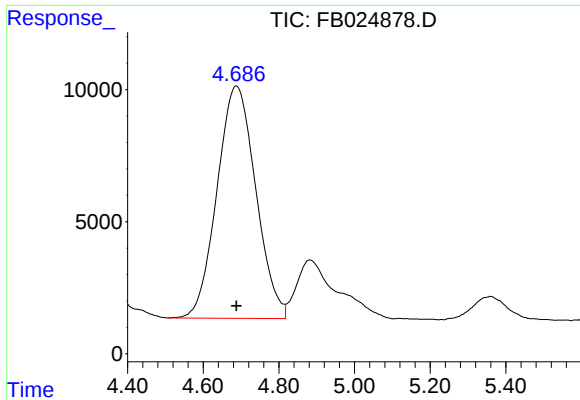


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 625762
Conc: 21.28 ng/ml

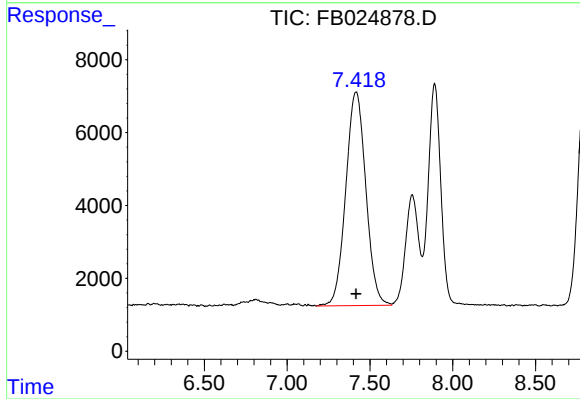


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.003 min
Response: 493618
Conc: 16.36 ng/ml

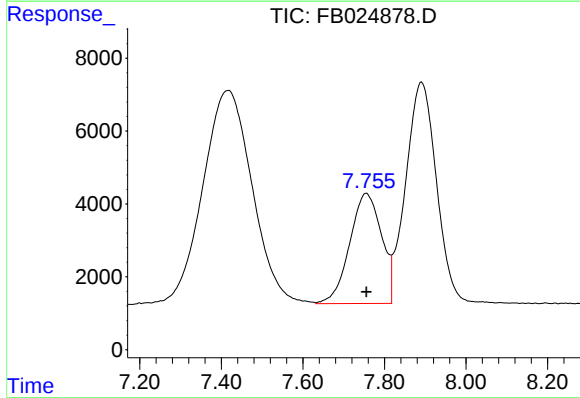


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 163768
Conc: 5.41 ng/ml

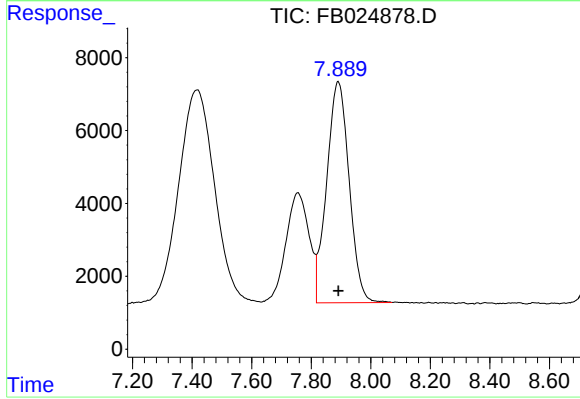


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 318188
Conc: 8.22 ng/ml

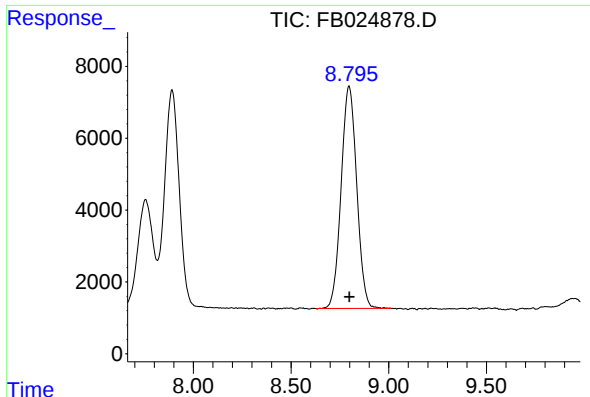


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 343896
Conc: 15.45 ng/ml

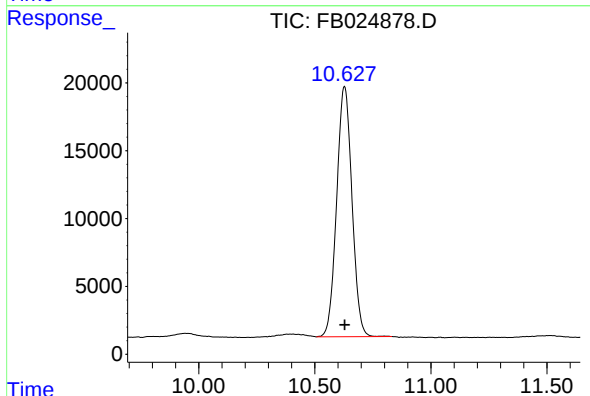


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 846518
Conc: 23.23 ng/ml

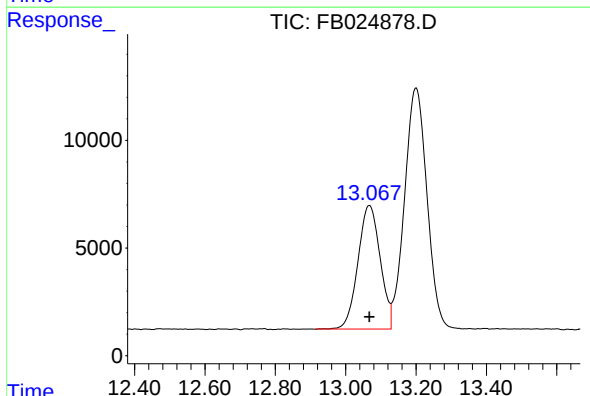


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: 0.000 min
Response: 251857
Conc: 7.49 ng/ml

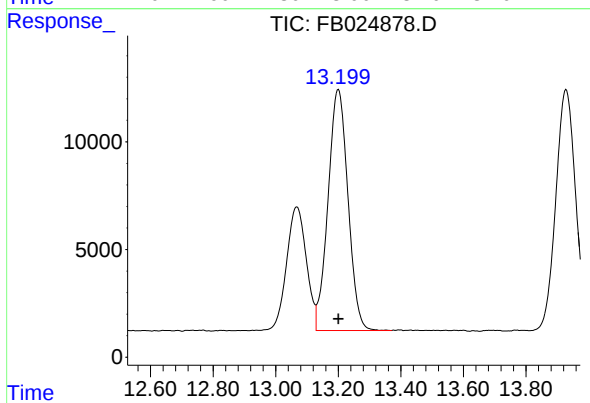


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: 0.000 min
Response: 495648
Conc: 15.13 ng/ml

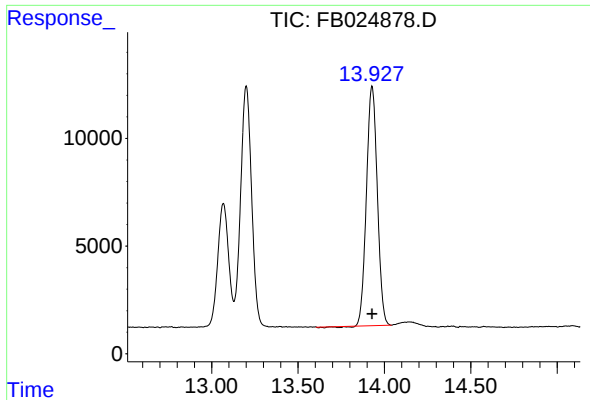

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.000 min
Response: 485823
Conc: 15.21 ng/ml

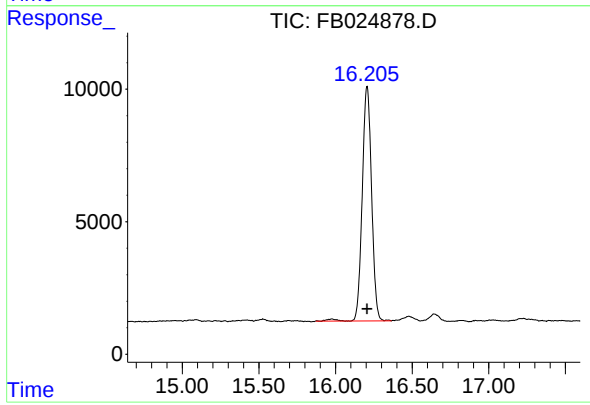

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.000 min
Response: 377180
Conc: 14.46 ng/ml