

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091522\
 Data File : FB028277.D
 Signal(s) : FID2B.CH
 Acq On : 15 Sep 2022 13:55
 Operator : AJ/MA
 Sample : N4630-09
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 16 05:53:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.851	553895	46.278 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	76390	3.773 ng/ml
2) t 2,2,4-Trimethylpentane	7.389	123090	5.851 ng/ml
3) t n-Heptane	7.764	220580	10.261 ng/ml
7) t Ethylbenzene	13.023	855838	38.485 ng/ml
9) t O-Xylene	13.924	286613	13.680 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	866059	43.072 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091522\
Data File : FB028277.D
Signal(s) : FID2B.CH
Acq On : 15 Sep 2022 13:55
Operator : AJ/MA
Sample : N4630-09
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 16 05:53:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

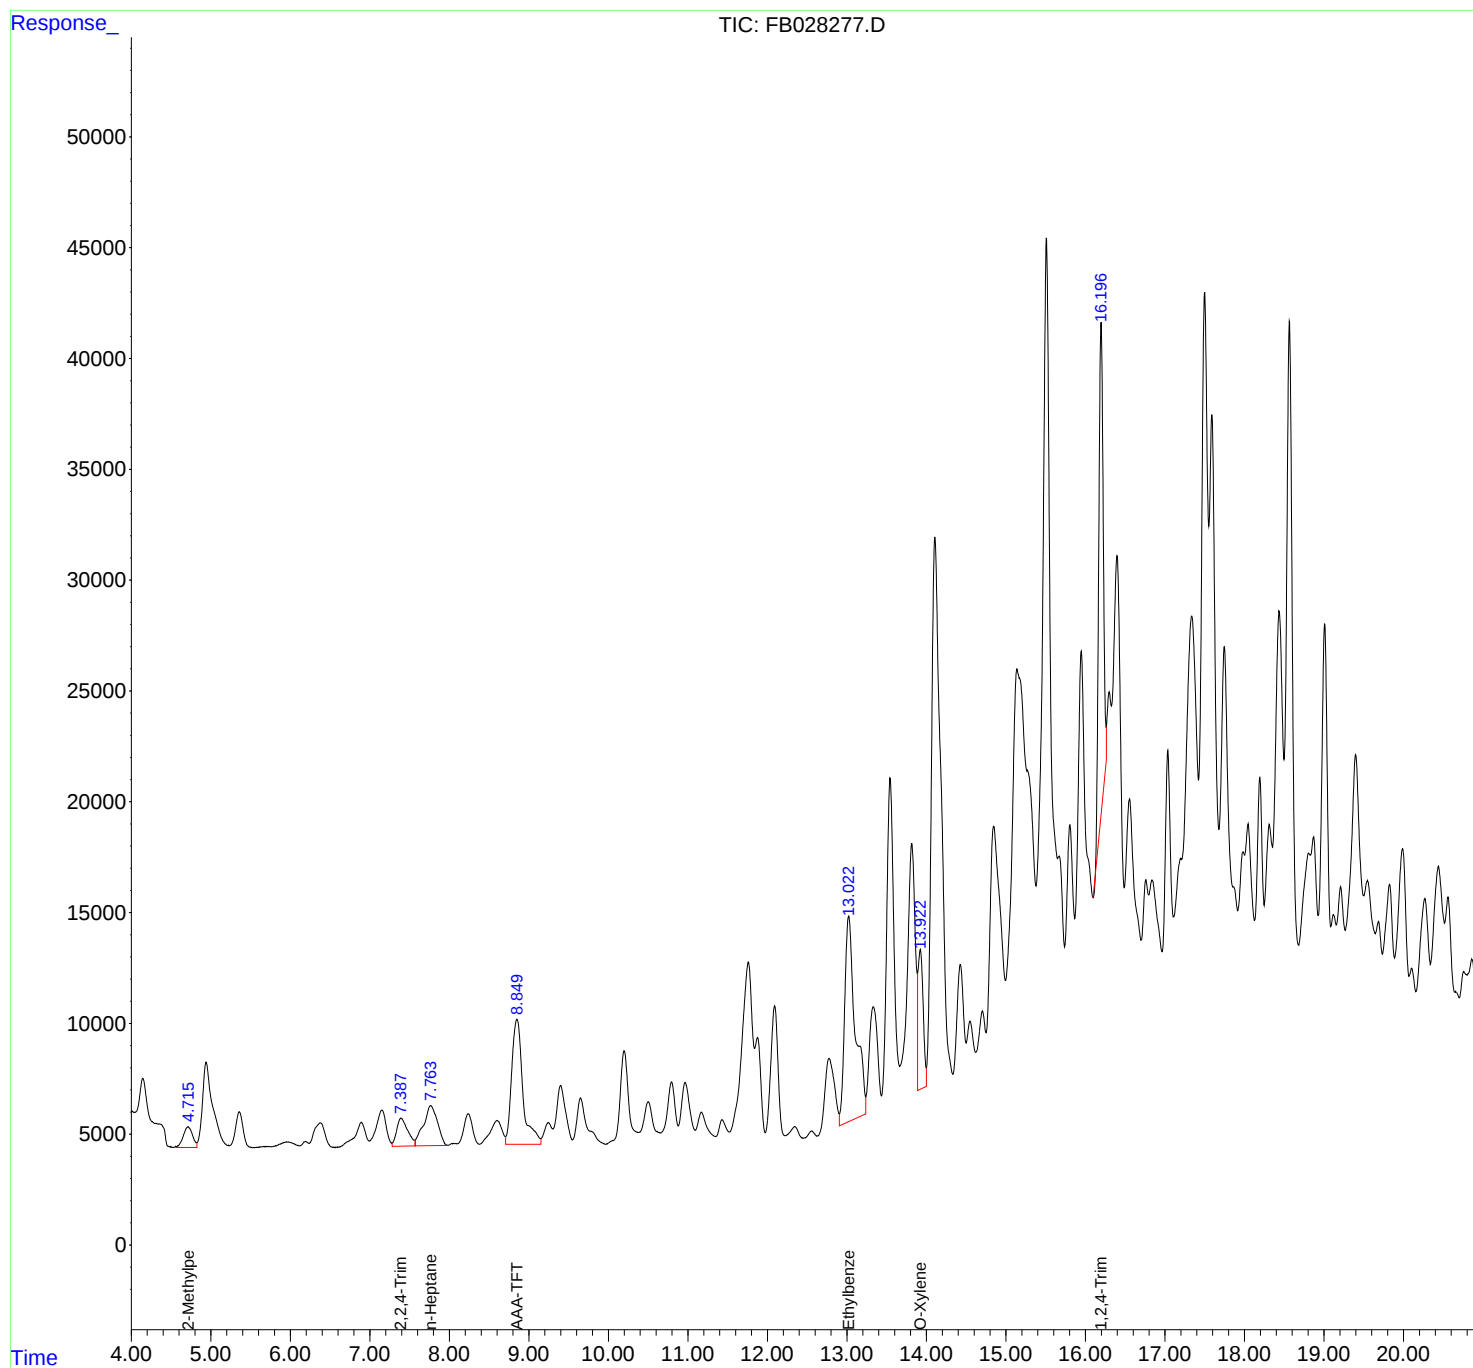


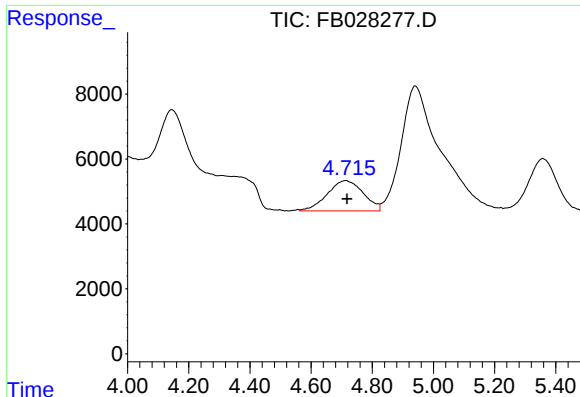

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: -0.001 min
Response: 76390
Conc: 3.77 ng/ml

Instrument :
FID_B
ClientSampleId :

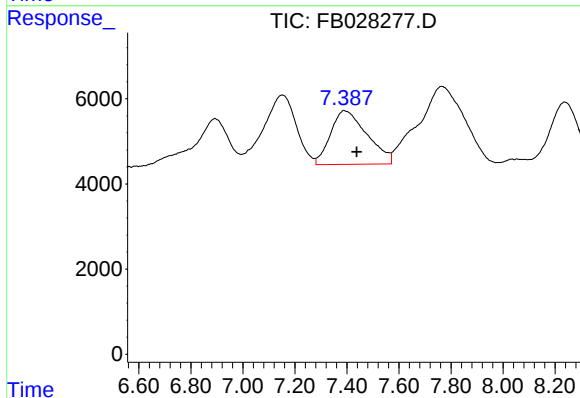


#2 2,2,4-Trimethylpentane

R.T.: 7.389 min
Delta R.T.: -0.049 min
Response: 123090
Conc: 5.85 ng/ml

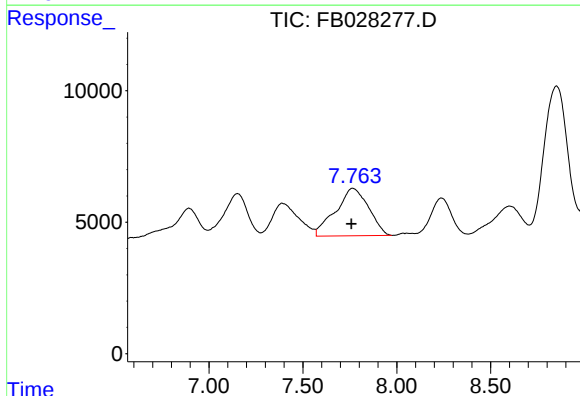


#3 n-Heptane

R.T.: 7.764 min
Delta R.T.: 0.006 min
Response: 220580
Conc: 10.26 ng/ml

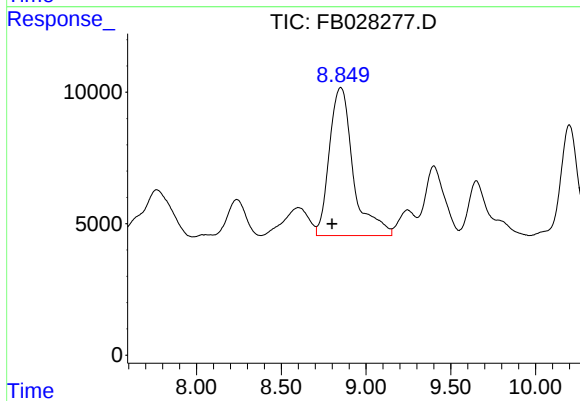

#5 AAA-TFT


R.T.: 8.851 min
Delta R.T.: 0.051 min
Response: 553895
Conc: 46.28 ng/ml

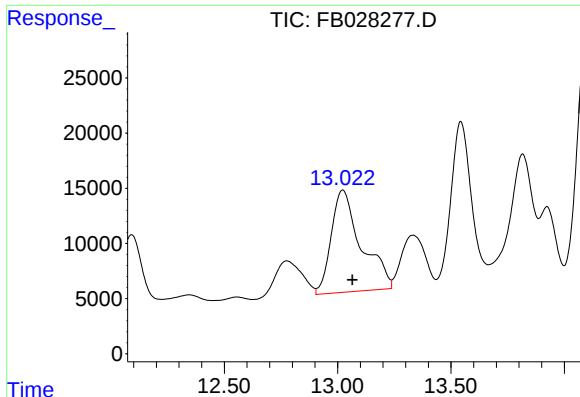

#7 Ethylbenzene


R.T.: 13.023 min
Delta R.T.: -0.042 min
Response: 855838
Conc: 38.48 ng/ml

Instrument :
FID_B
ClientSampleId :

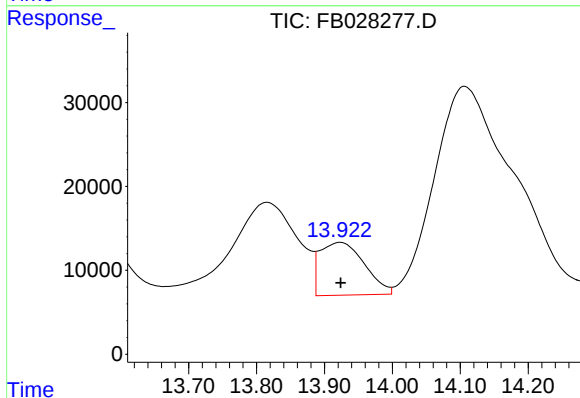

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.000 min
Response: 286613
Conc: 13.68 ng/ml

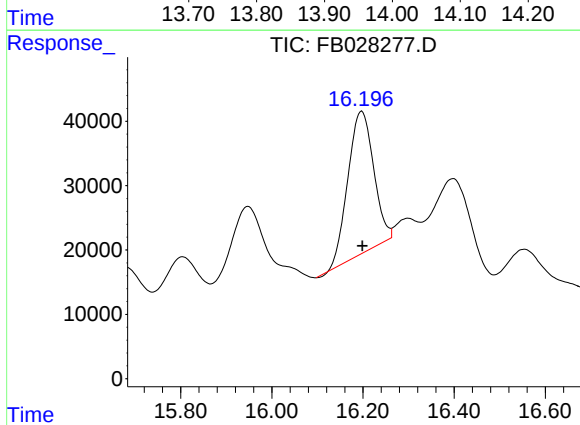

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: -0.002 min
Response: 866059
Conc: 43.07 ng/ml