

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091522\
 Data File : FB028287.D
 Signal(s) : FID2B.CH
 Acq On : 15 Sep 2022 21:23
 Operator : AJ/MA
 Sample : N4630-09RE
 Misc : 5.06G/5.00 ML DI WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 16 05:54:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.853	518343	43.308 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	109462	5.406 ng/ml
2) t 2,2,4-Trimethylpentane	7.392	136415	6.485 ng/ml
3) t n-Heptane	7.768	249511	11.607 ng/ml
7) t Ethylbenzene	13.023	414254	18.628 ng/ml
8) t m-Xylene	13.171	90744	4.158 ng/ml
9) t O-Xylene	13.922	168938	8.063 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	552494	27.478 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091522\
Data File : FB028287.D
Signal(s) : FID2B.CH
Acq On : 15 Sep 2022 21:23
Operator : AJ/MA
Sample : N4630-09RE
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 16 05:54:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

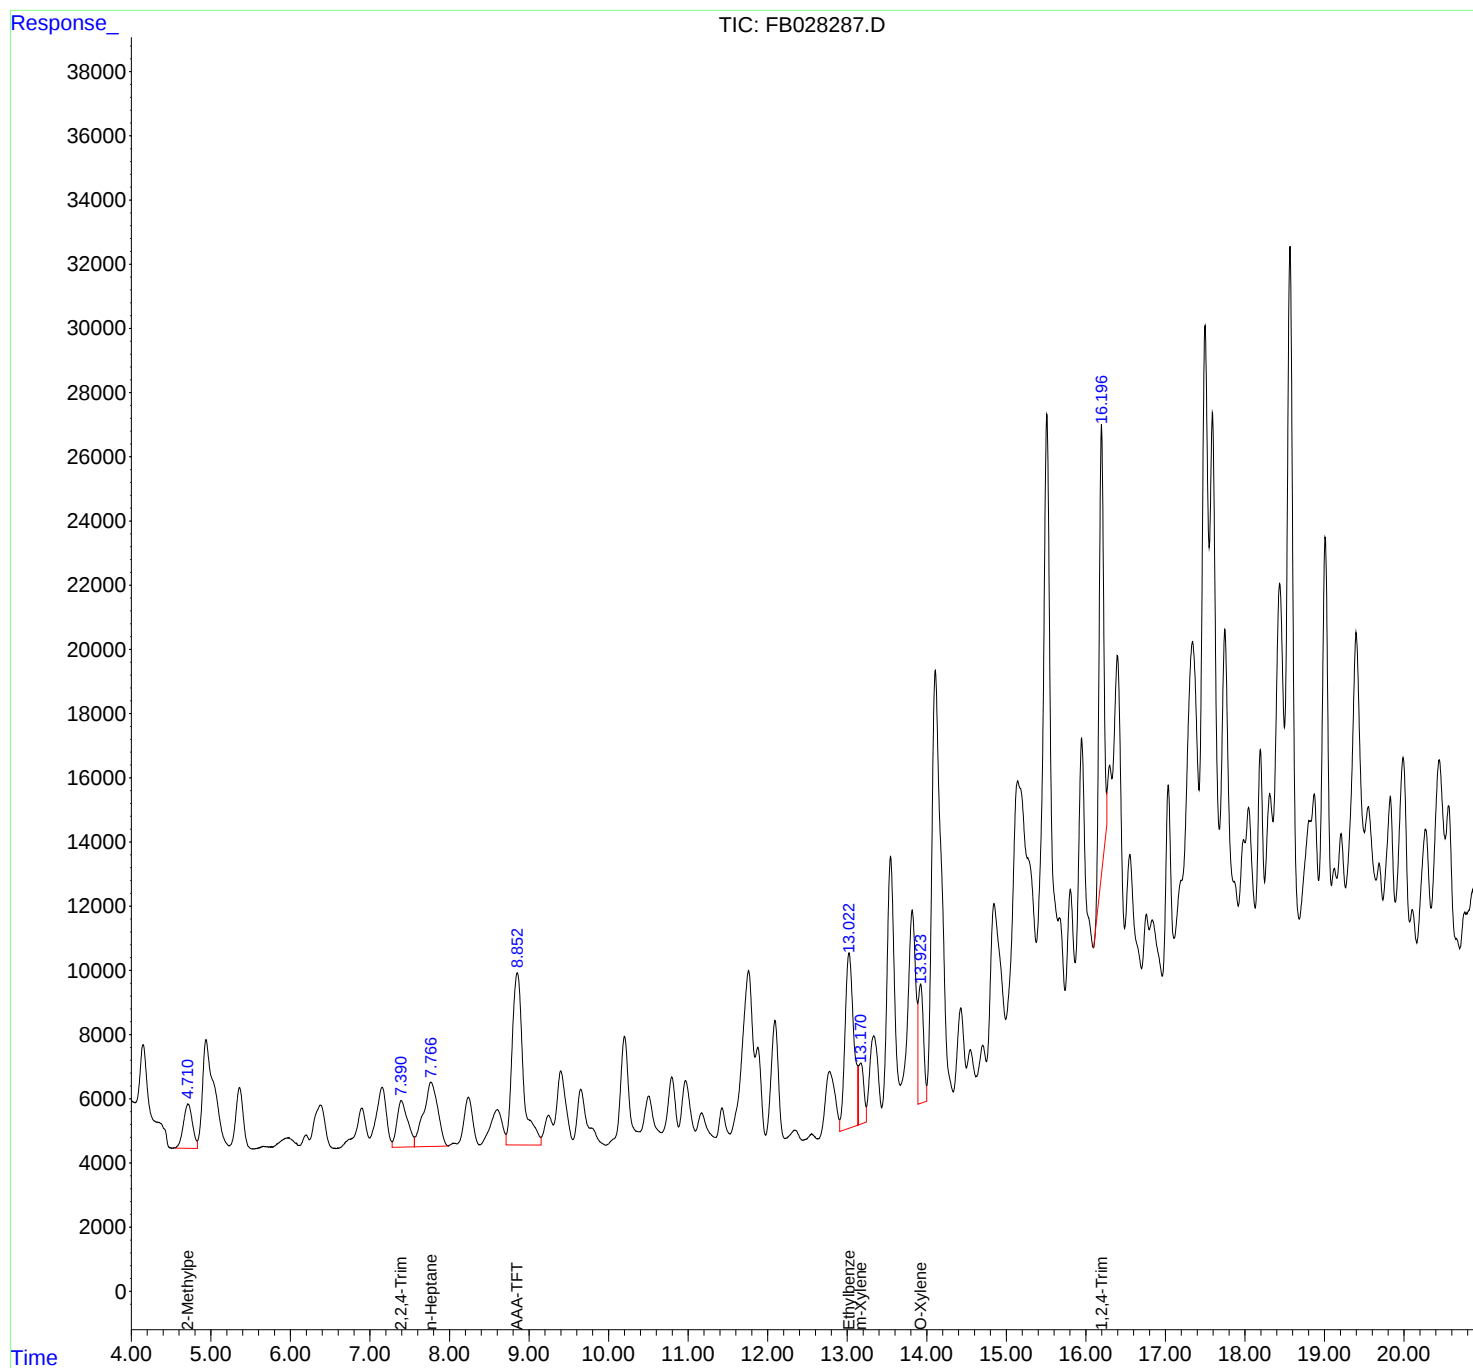


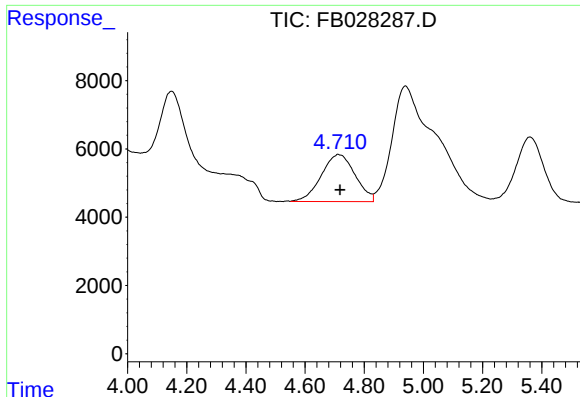

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: -0.006 min
Response: 109462
Conc: 5.41 ng/ml

Instrument :
FID_B
ClientSampleId :

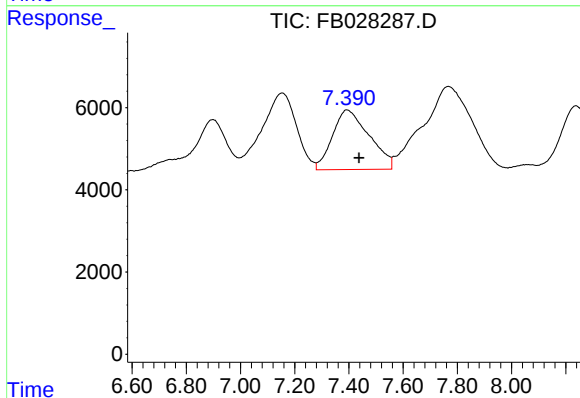


#2 2,2,4-Trimethylpentane

R.T.: 7.392 min
Delta R.T.: -0.045 min
Response: 136415
Conc: 6.48 ng/ml

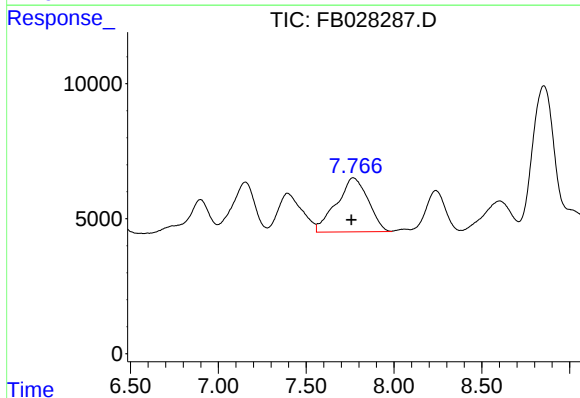


#3 n-Heptane

R.T.: 7.768 min
Delta R.T.: 0.009 min
Response: 249511
Conc: 11.61 ng/ml

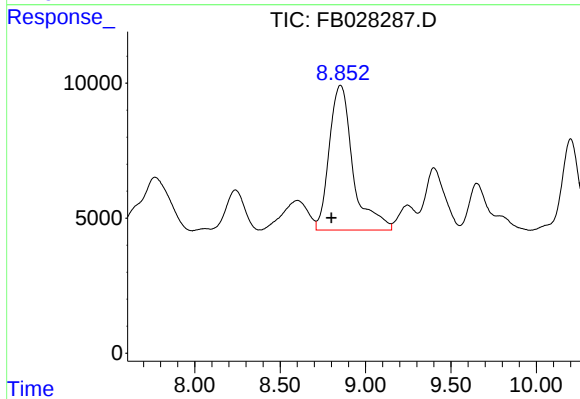

#5 AAA-TFT


R.T.: 8.853 min
Delta R.T.: 0.053 min
Response: 518343
Conc: 43.31 ng/ml

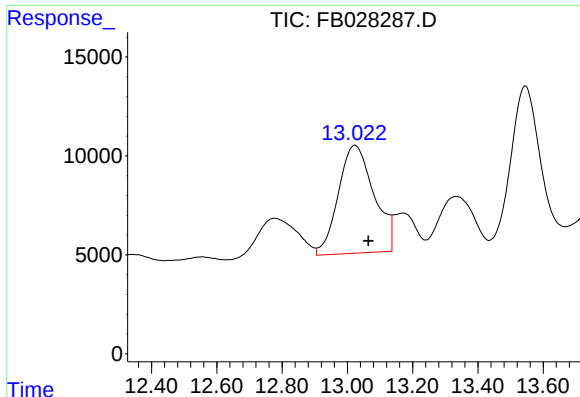

#7 Ethylbenzene


R.T.: 13.023 min
Delta R.T.: -0.041 min
Response: 414254
Conc: 18.63 ng/ml

Instrument :
FID_B
ClientSampleId :

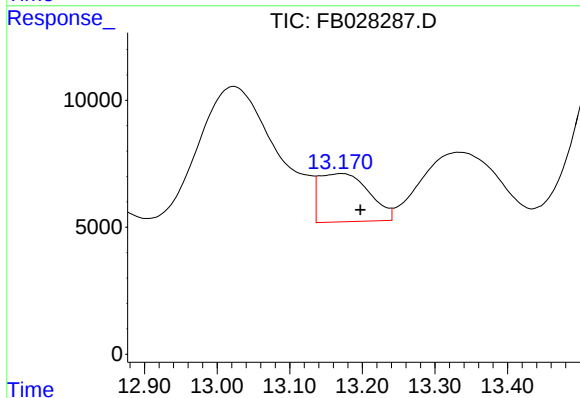


#8 m-Xylene

R.T.: 13.171 min
Delta R.T.: -0.026 min
Response: 90744
Conc: 4.16 ng/ml

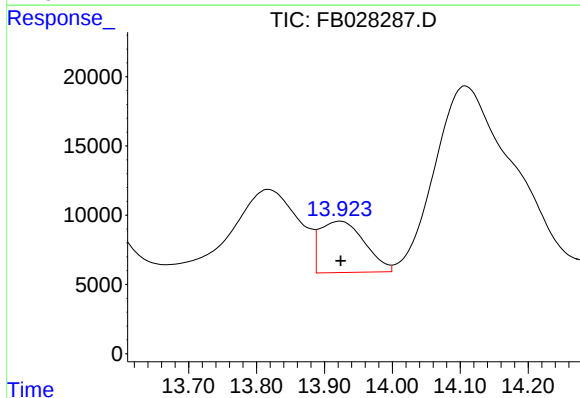

#9 o-Xylene

R.T.: 13.922 min
Delta R.T.: -0.002 min
Response: 168938
Conc: 8.06 ng/ml

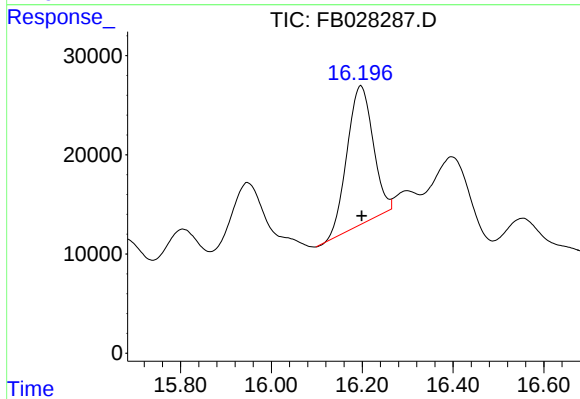

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: -0.001 min
Response: 552494
Conc: 27.48 ng/ml