

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091522\
 Data File : FB028273.D
 Signal(s) : FID2B.CH
 Acq On : 15 Sep 2022 11:24
 Operator : AJ/MA
 Sample : BSF0915S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0915S1

Integration File: SAMPLE.e
 Quant Time: Sep 16 05:53:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	204908	17.120 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	561872	27.751 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	639149	30.383 ng/ml
3) t n-Heptane	7.753	179253	8.339 ng/ml
4) t Benzene	7.889	223595	9.089 ng/ml
6) t Toluene	10.622	640528	27.512 ng/ml
7) t Ethylbenzene	13.059	207465	9.329 ng/ml
8) t m-Xylene	13.191	413797	18.962 ng/ml
9) t O-Xylene	13.918	411402	19.636 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	439752	21.870 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091522\
Data File : FB028273.D
Signal(s) : FID2B.CH
Acq On : 15 Sep 2022 11:24
Operator : AJ/MA
Sample : BSF0915S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0915S1

Integration File: SAMPLE.e
Quant Time: Sep 16 05:53:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

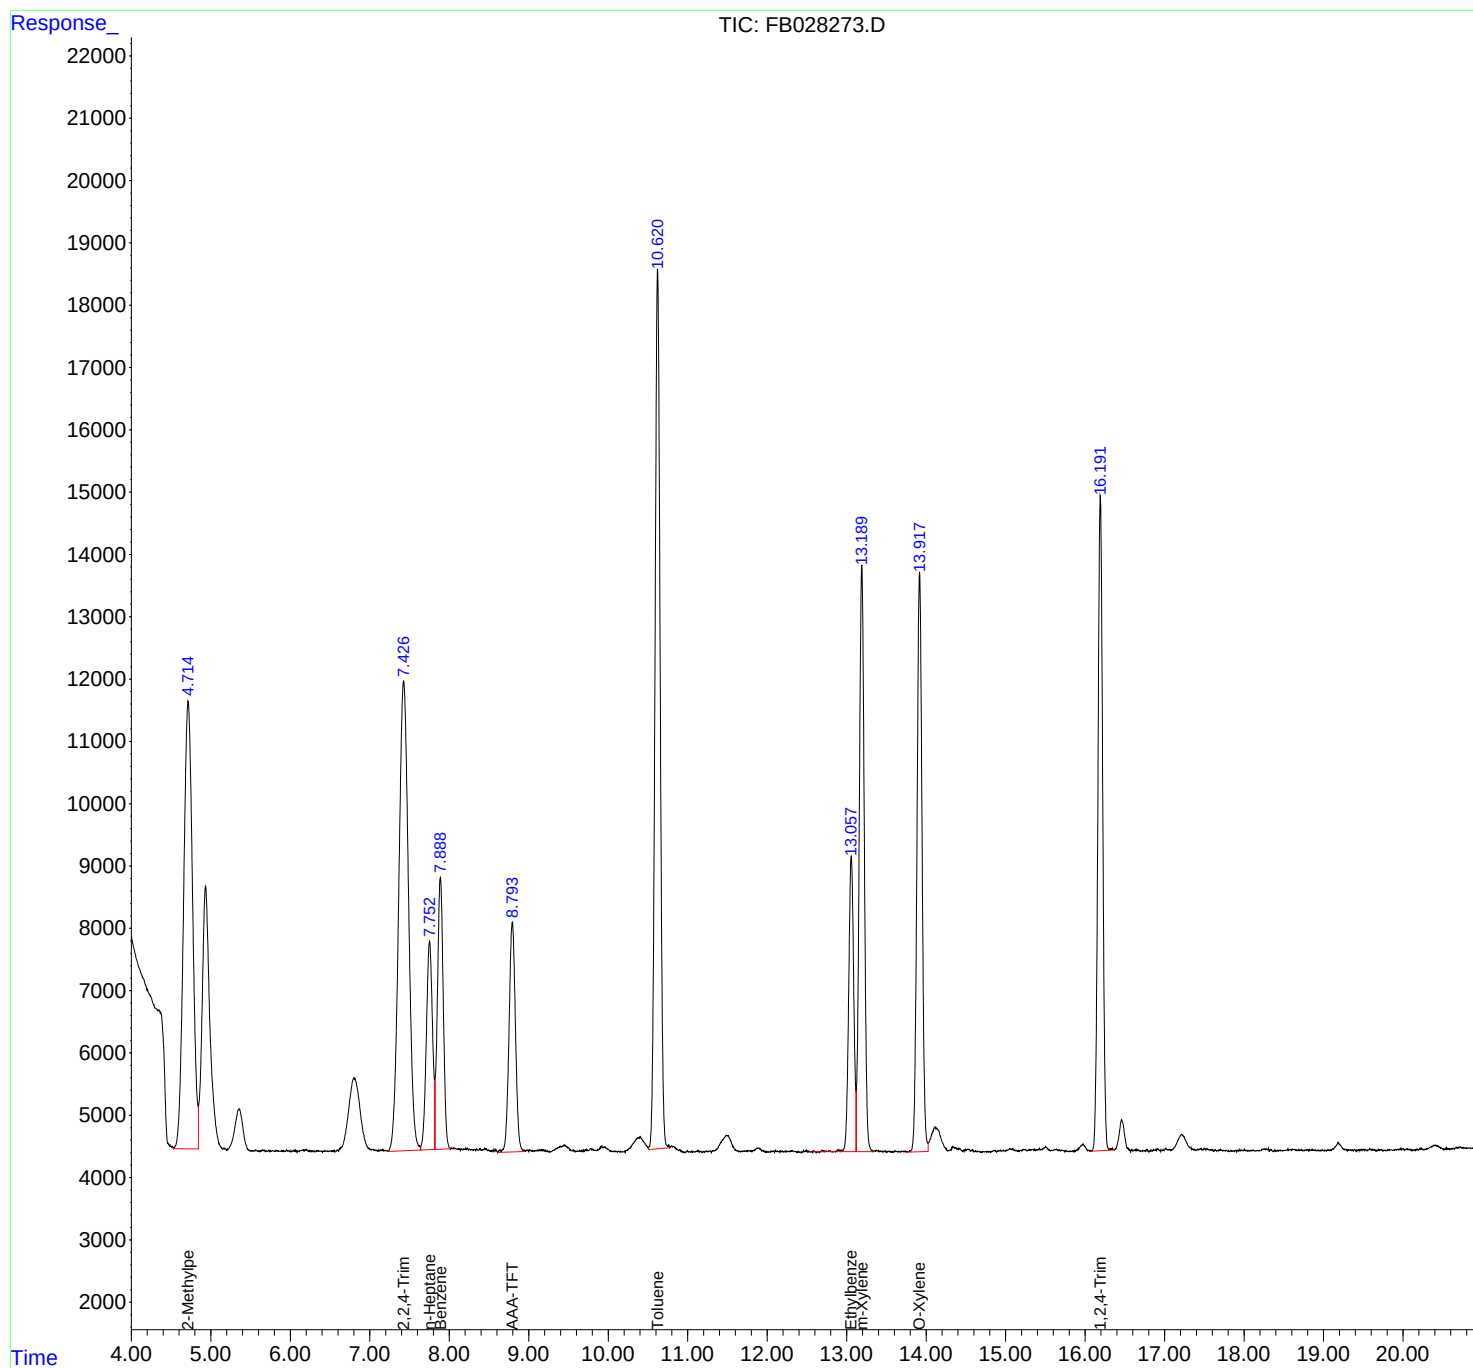


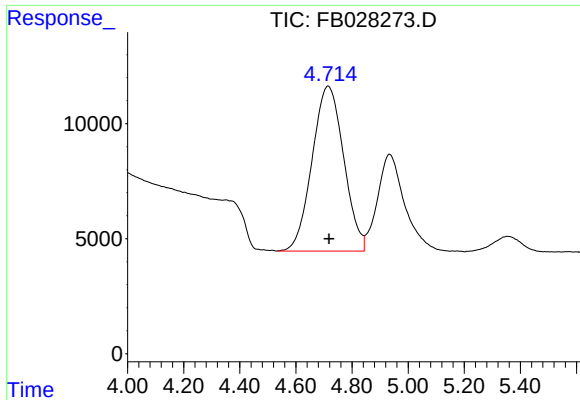

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: -0.003 min
Response: 561872
Conc: 27.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0915S1

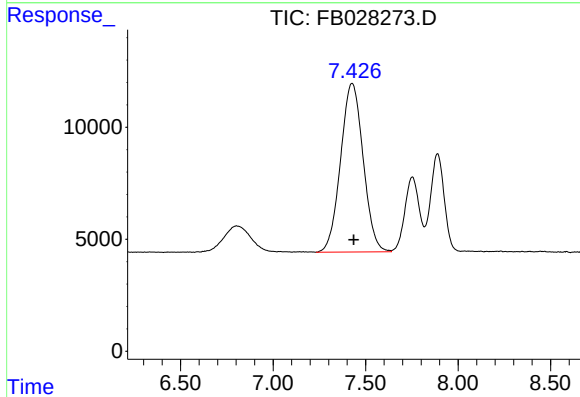


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: -0.010 min
Response: 639149
Conc: 30.38 ng/ml

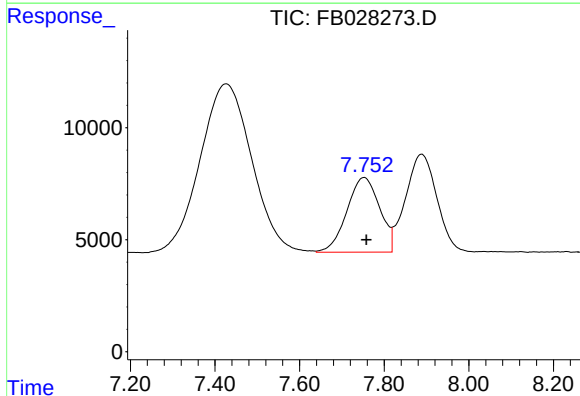


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.005 min
Response: 179253
Conc: 8.34 ng/ml

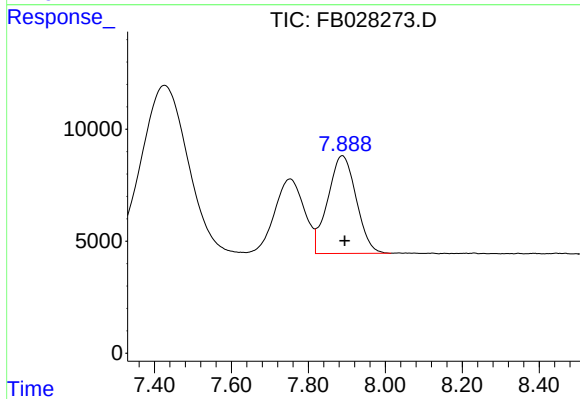

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.006 min
Response: 223595
Conc: 9.09 ng/ml

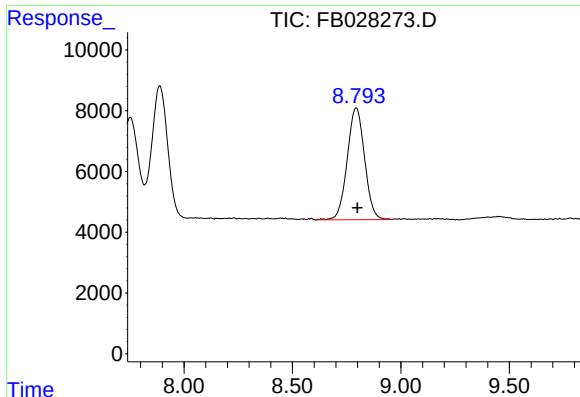

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.006 min
Response: 204908
Conc: 17.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0915S1

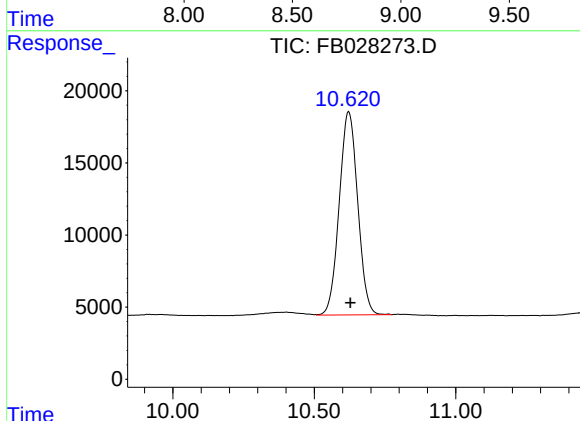


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.006 min
Response: 640528
Conc: 27.51 ng/ml

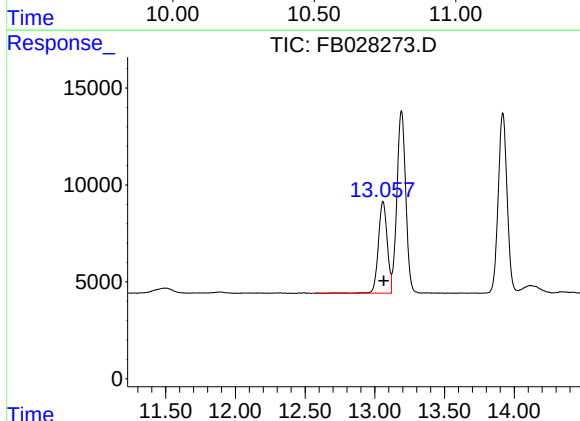


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: -0.006 min
Response: 207465
Conc: 9.33 ng/ml

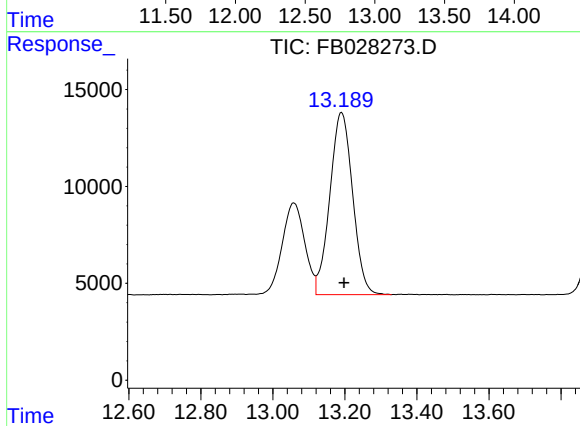

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: -0.006 min
Response: 413797
Conc: 18.96 ng/ml

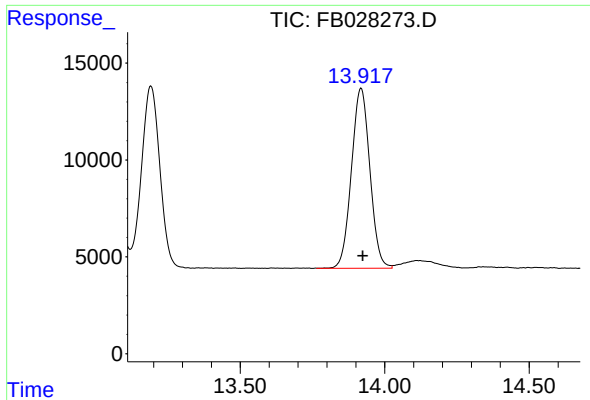

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: -0.006 min
Response: 411402
Conc: 19.64 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0915S1

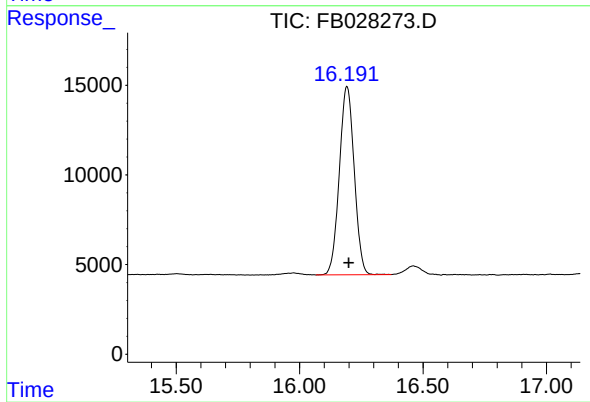

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.007 min
Response: 439752
Conc: 21.87 ng/ml