

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091522\
 Data File : FB028313.D
 Signal(s) : FID2B.CH
 Acq On : 16 Sep 2022 19:11
 Operator : AJ/MA
 Sample : BSF0915S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0915S2

Integration File: SAMPLE.e
 Quant Time: Sep 17 11:42:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	232547	19.429 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	547567	27.044 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	612361	29.110 ng/ml
3) t n-Heptane	7.754	187918	8.742 ng/ml
4) t Benzene	7.892	233935	9.509 ng/ml
6) t Toluene	10.625	684321	29.393 ng/ml
7) t Ethylbenzene	13.061	219285	9.861 ng/ml
8) t m-Xylene	13.193	430891	19.745 ng/ml
9) t O-Xylene	13.920	414154	19.767 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	407560	20.269 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091522\
Data File : FB028313.D
Signal(s) : FID2B.CH
Acq On : 16 Sep 2022 19:11
Operator : AJ/MA
Sample : BSF0915S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0915S2

Integration File: SAMPLE.e
Quant Time: Sep 17 11:42:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

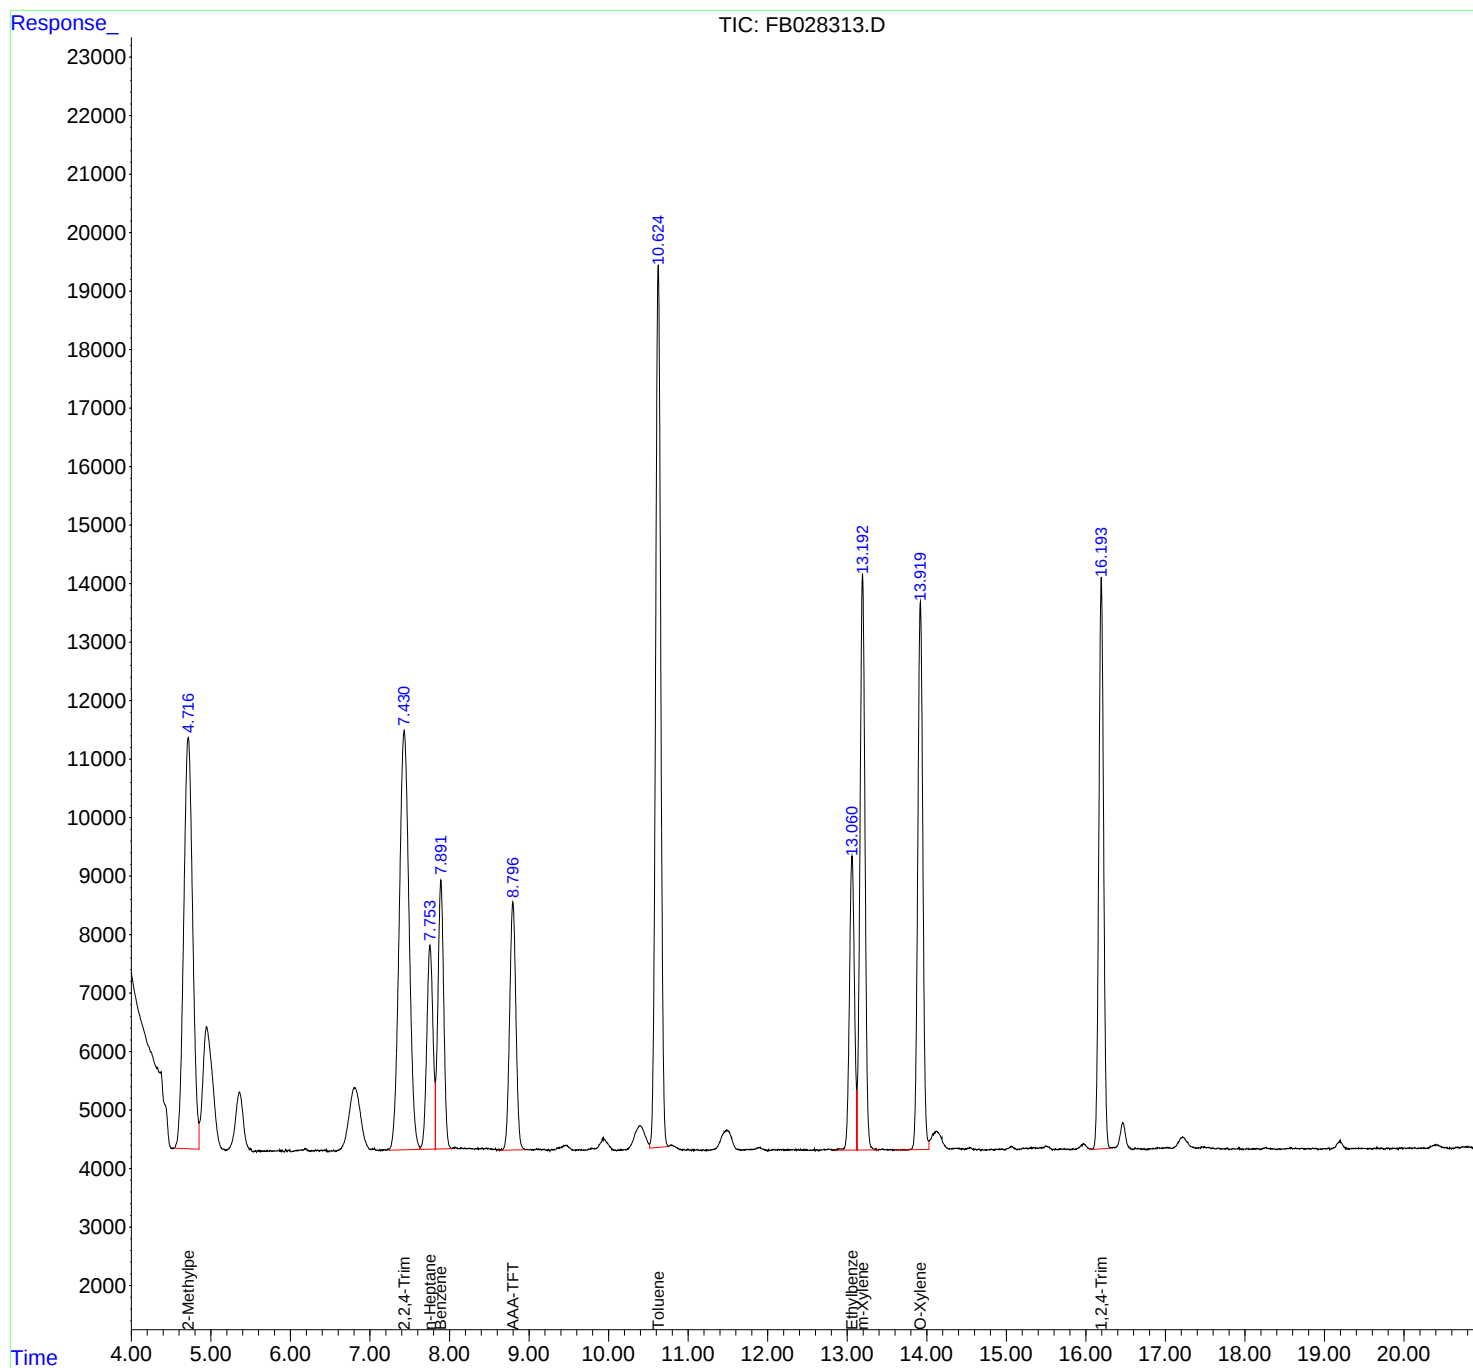


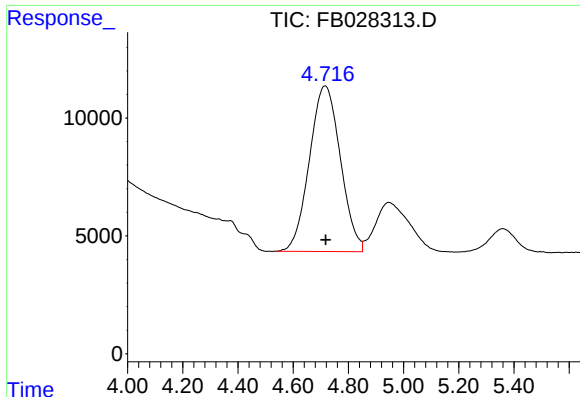

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: -0.001 min
Response: 547567
Conc: 27.04 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0915S2

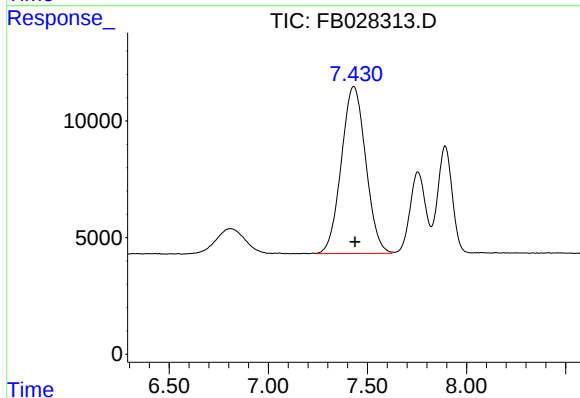


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: -0.006 min
Response: 612361
Conc: 29.11 ng/ml

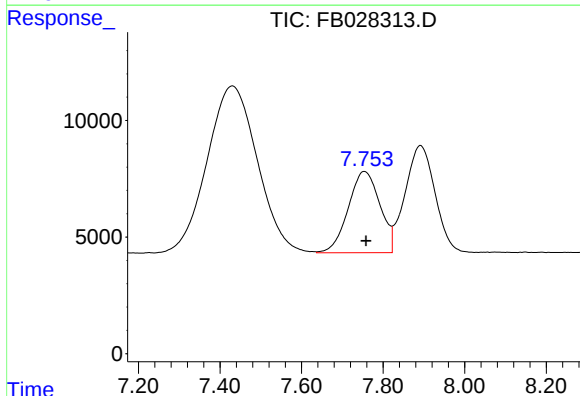


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 187918
Conc: 8.74 ng/ml

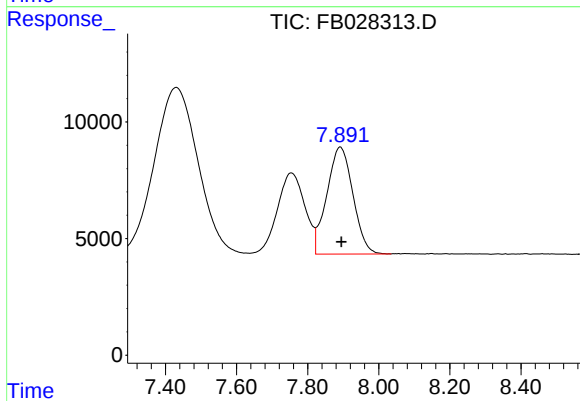

#4 Benzene


R.T.: 7.892 min
Delta R.T.: -0.003 min
Response: 233935
Conc: 9.51 ng/ml

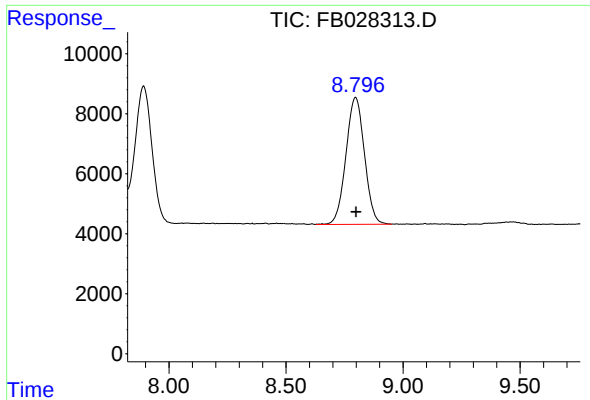

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.002 min
Response: 232547
Conc: 19.43 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0915S2

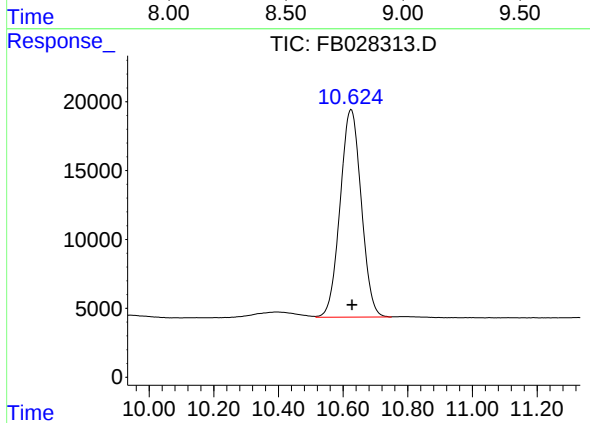


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.003 min
Response: 684321
Conc: 29.39 ng/ml

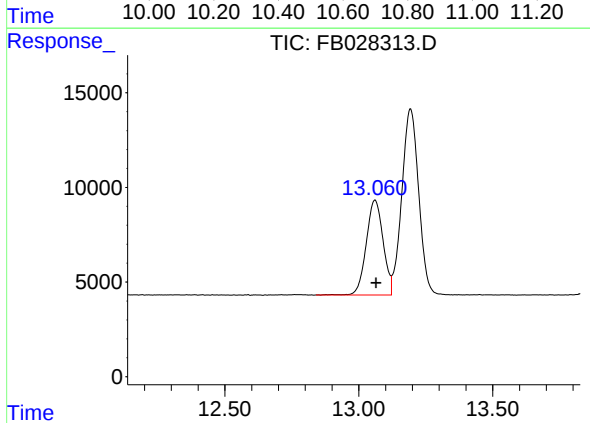


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: -0.004 min
Response: 219285
Conc: 9.86 ng/ml

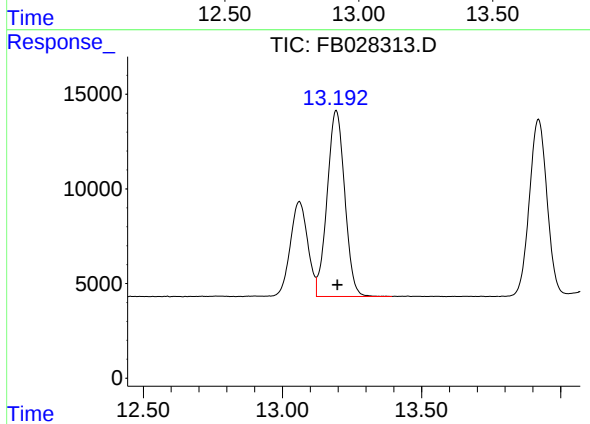

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: -0.004 min
Response: 430891
Conc: 19.75 ng/ml

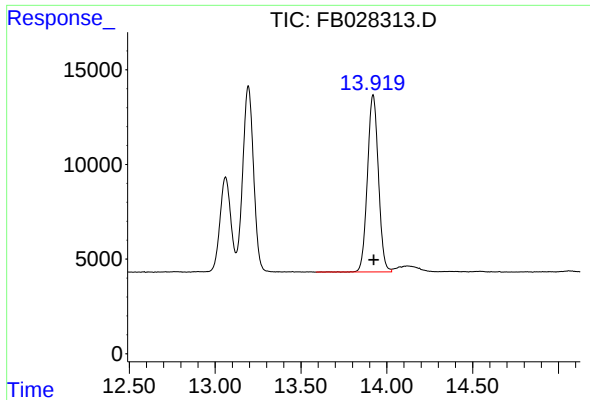

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: -0.004 min
Response: 414154
Conc: 19.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0915S2

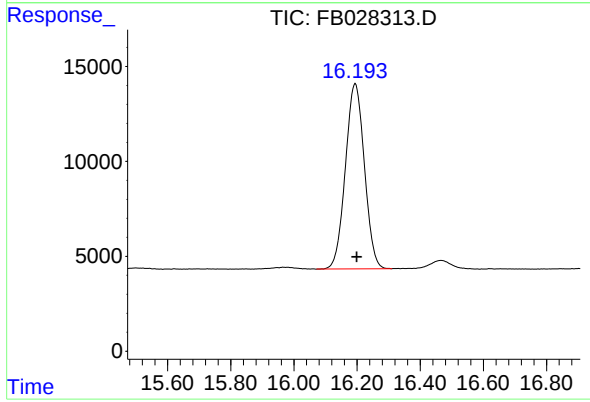

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: -0.005 min
Response: 407560
Conc: 20.27 ng/ml