

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091619\
 Data File : FB022515.D
 Signal(s) : FID2B.CH
 Acq On : 16 Sep 2019 10:20
 Operator : DD/AJ
 Sample : BSF0916S1
 Misc : 5.01g/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0916S1

Integration File: Calibration.e
 Quant Time: Sep 17 02:17:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.967	550397	18.922 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.833	1060125	21.577 ng/ml
2) t 2,2,4-Trimethylpentane	7.585	1241900	24.050 ng/ml
3) t n-Heptane	7.925	406493	8.076 ng/ml
4) t Benzene	8.059	486074	8.190 ng/ml
6) t Toluene	10.807	1462110	30.734 ng/ml
7) t Ethylbenzene	13.254	466937	15.575 ng/ml
8) t m-Xylene	13.386	928219	34.940 ng/ml
9) t O-Xylene	14.116	873714	36.015 ng/ml
10) t 1,2,4-Trimethylbenzene	16.397	595563	22.844 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091619\
Data File : FB022515.D
Signal(s) : FID2B.CH
Acq On : 16 Sep 2019 10:20
Operator : DD/AJ
Sample : BSF0916S1
Misc : 5.01g/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0916S1

Integration File: Calibration.e
Quant Time: Sep 17 02:17:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

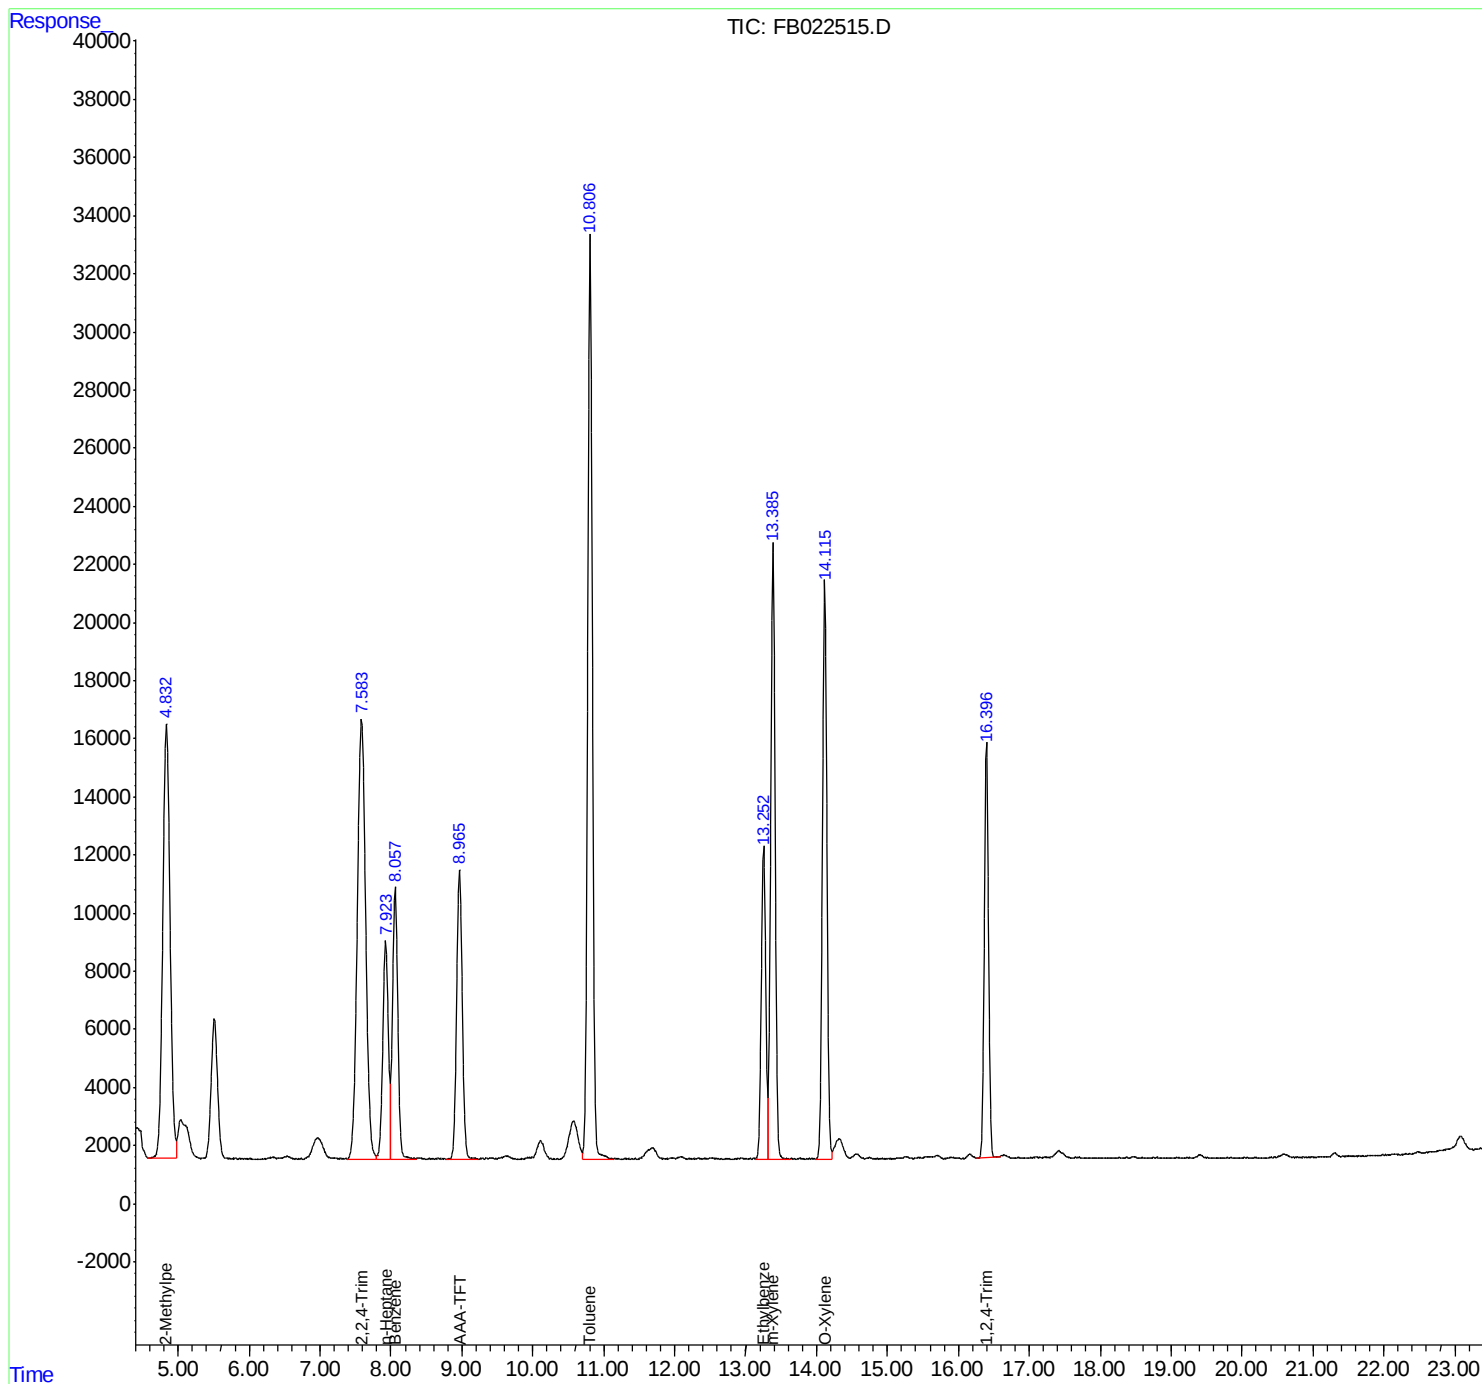


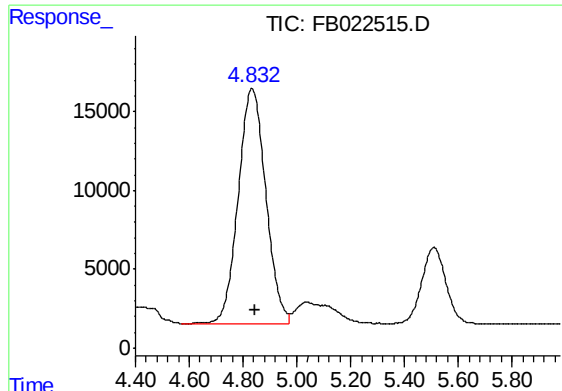

#1 2-Methylpentane


R.T.: 4.833 min
Delta R.T.: -0.014 min
Response: 1060125
Conc: 21.58 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0916S1

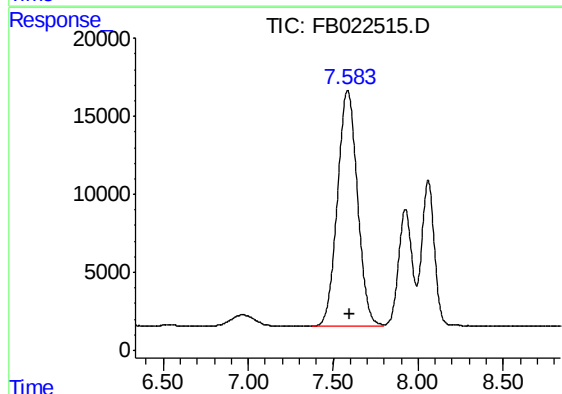


#2 2,2,4-Trimethylpentane

R.T.: 7.585 min
Delta R.T.: -0.013 min
Response: 1241900
Conc: 24.05 ng/ml

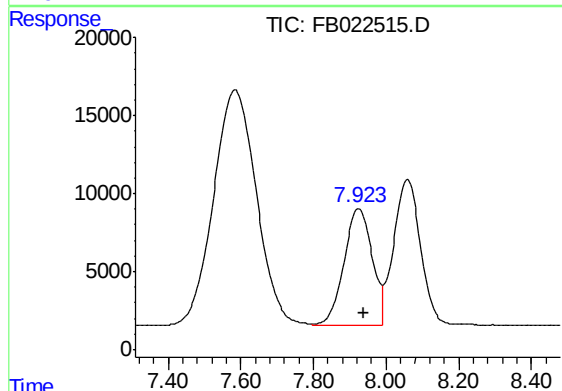


#3 n-Heptane

R.T.: 7.925 min
Delta R.T.: -0.013 min
Response: 406493
Conc: 8.08 ng/ml

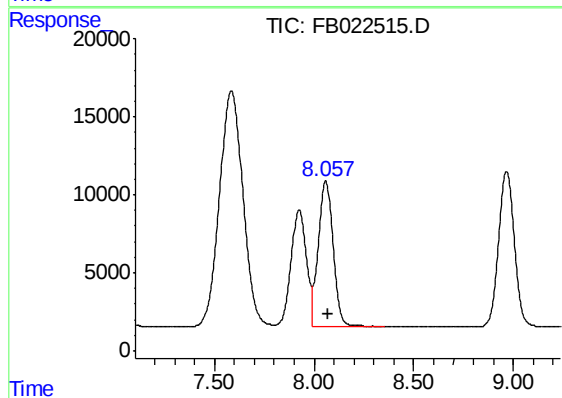

#4 Benzene


R.T.: 8.059 min
Delta R.T.: -0.013 min
Response: 486074
Conc: 8.19 ng/ml

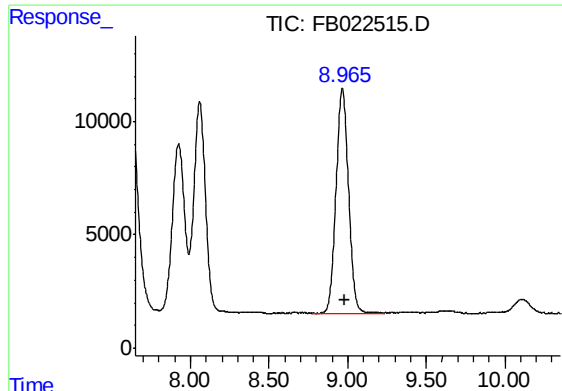

#5 AAA-TFT


R.T.: 8.967 min
Delta R.T.: -0.013 min
Response: 550397
Conc: 18.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0916S1

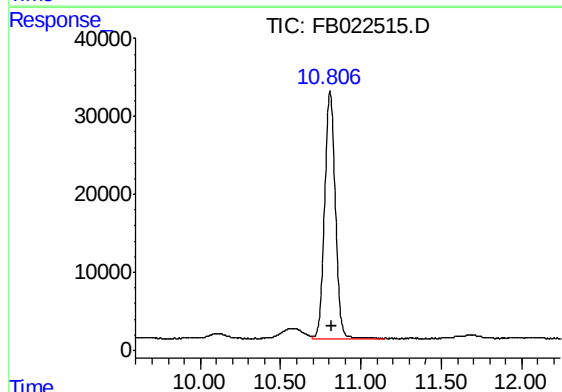


#6 Toluene

R.T.: 10.807 min
Delta R.T.: -0.012 min
Response: 1462110
Conc: 30.73 ng/ml

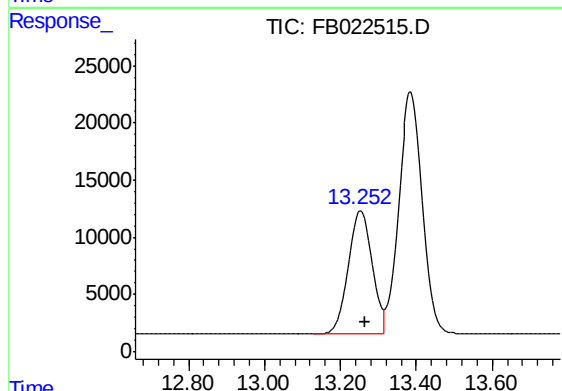


#7 Ethylbenzene

R.T.: 13.254 min
Delta R.T.: -0.012 min
Response: 466937
Conc: 15.58 ng/ml

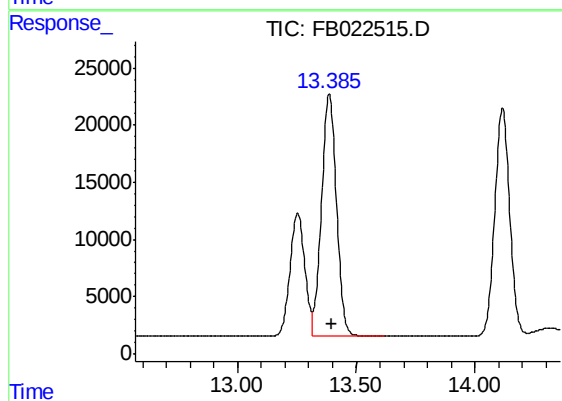

#8 m-Xylene


R.T.: 13.386 min
Delta R.T.: -0.012 min
Response: 928219
Conc: 34.94 ng/ml

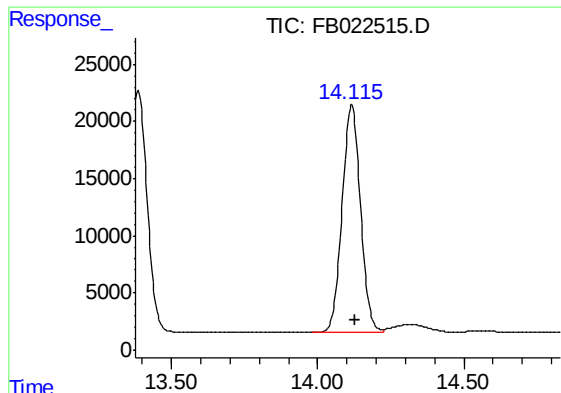

#9 O-Xylene

R.T.: 14.116 min
Delta R.T.: -0.012 min
Response: 873714
Conc: 36.01 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0916S1

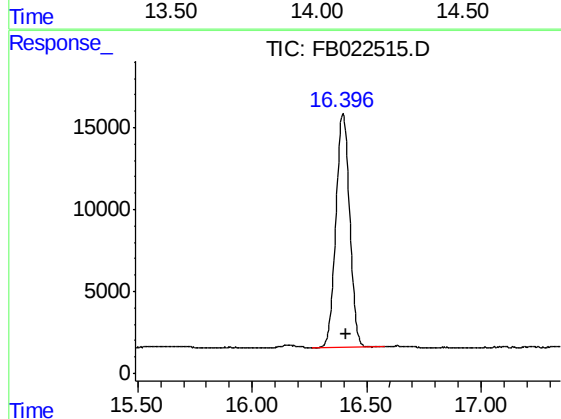

#10 1,2,4-Trimethylbenzene

R.T.: 16.397 min
Delta R.T.: -0.010 min
Response: 595563
Conc: 22.84 ng/ml