

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091619\
 Data File : FB022520.D
 Signal(s) : FID2B.CH
 Acq On : 16 Sep 2019 16:34
 Operator : DD/AJ
 Sample : K4897-05MSD
 Misc : 5.02g/5.00ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 RBR-200052MSD

Integration File: Calibration.e
 Quant Time: Sep 17 02:18:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.967	574155	19.739 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.833	656065	13.353 ng/ml
2) t 2,2,4-Trimethylpentane	7.585	545744	10.569 ng/ml
3) t n-Heptane	7.926	187115	3.718 ng/ml
4) t Benzene	8.060	426450	7.185 ng/ml
6) t Toluene	10.809	1217062	25.583 ng/ml
7) t Ethylbenzene	13.255	363358	12.120 ng/ml
8) t m-Xylene	13.388	712717	26.828 ng/ml
9) t O-Xylene	14.118	687162	28.325 ng/ml
10) t 1,2,4-Trimethylbenzene	16.399	400236	15.352 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091619\
Data File : FB022520.D
Signal(s) : FID2B.CH
Acq On : 16 Sep 2019 16:34
Operator : DD/AJ
Sample : K4897-05MSD
Misc : 5.02g/5.00ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RBR-200052MSD

Integration File: Calibration.e
Quant Time: Sep 17 02:18:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

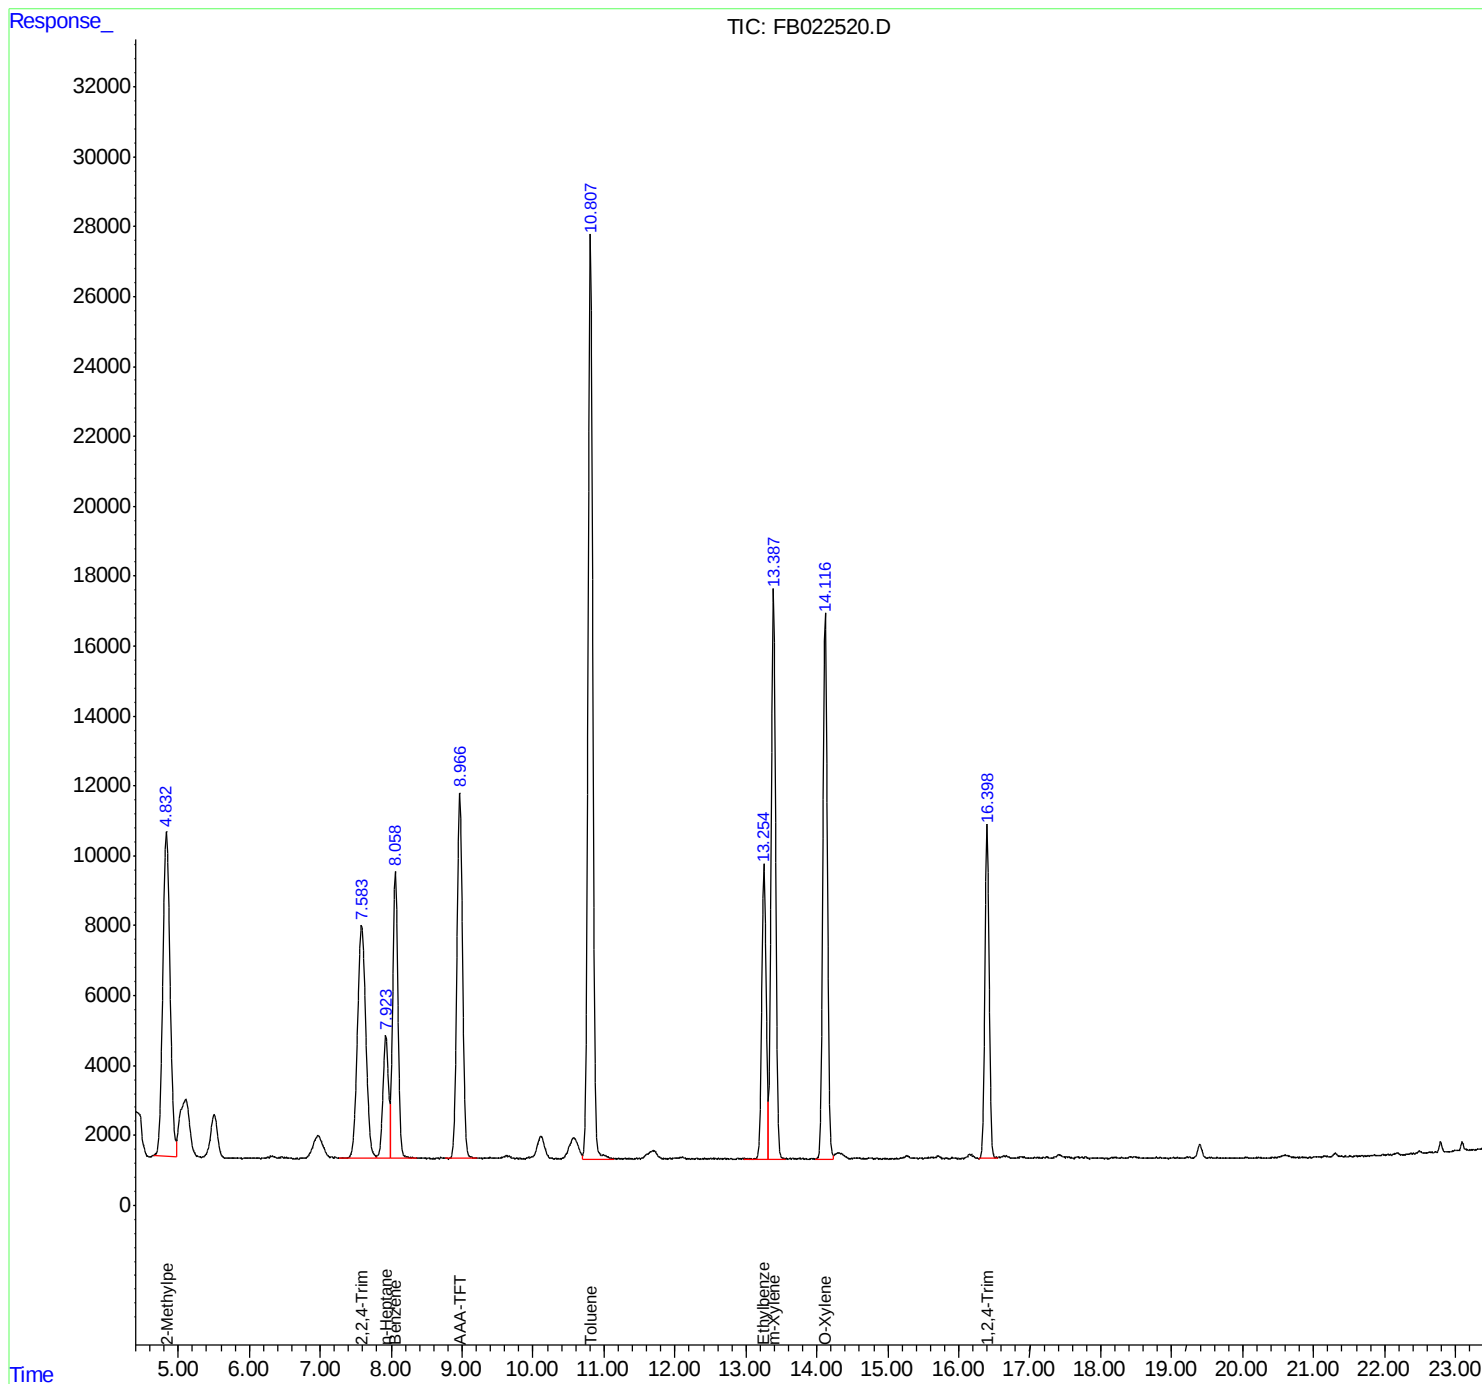


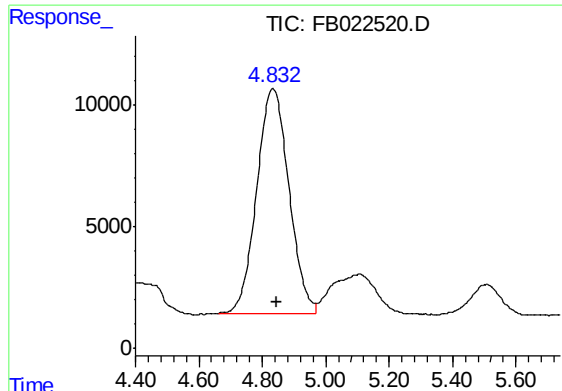

#1 2-Methylpentane


R.T.: 4.833 min
Delta R.T.: -0.014 min
Response: 656065
Conc: 13.35 ng/ml

Instrument :
FID_B
ClientSampleId :
RBR-200052MSD

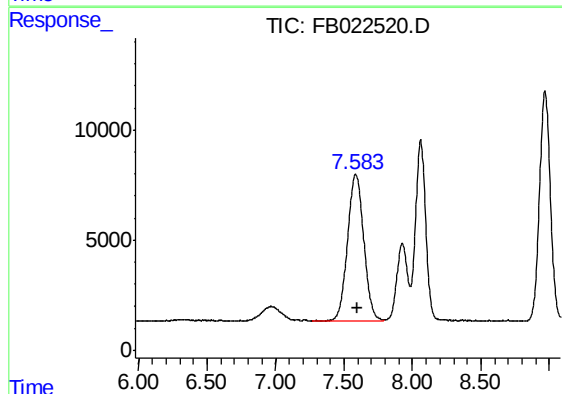


#2 2,2,4-Trimethylpentane

R.T.: 7.585 min
Delta R.T.: -0.013 min
Response: 545744
Conc: 10.57 ng/ml

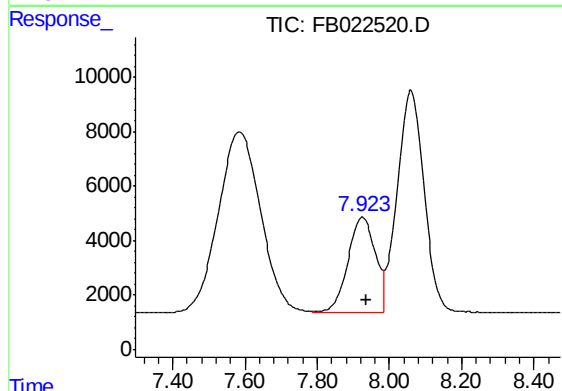


#3 n-Heptane

R.T.: 7.926 min
Delta R.T.: -0.012 min
Response: 187115
Conc: 3.72 ng/ml

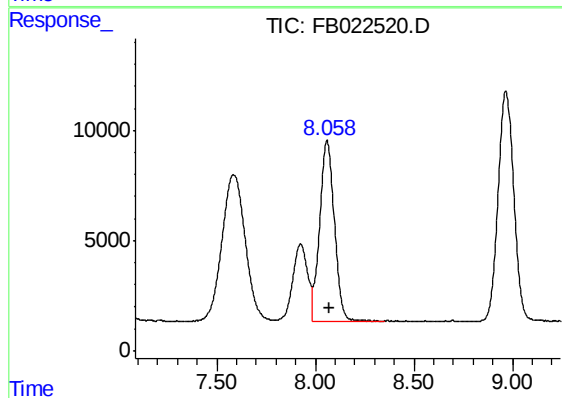

#4 Benzene


R.T.: 8.060 min
Delta R.T.: -0.013 min
Response: 426450
Conc: 7.19 ng/ml

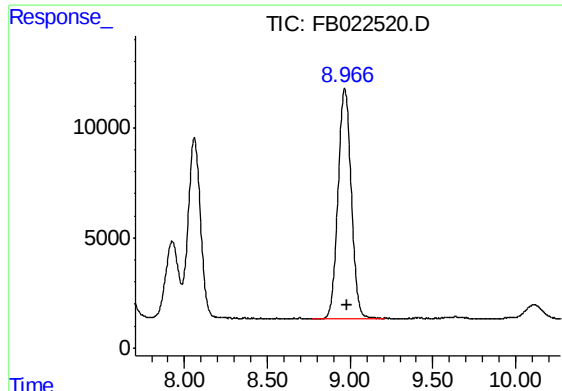

#5 AAA-TFT


R.T.: 8.967 min
Delta R.T.: -0.012 min
Response: 574155
Conc: 19.74 ng/ml

Instrument :
FID_B
ClientSampleId :
RBR-200052MSD

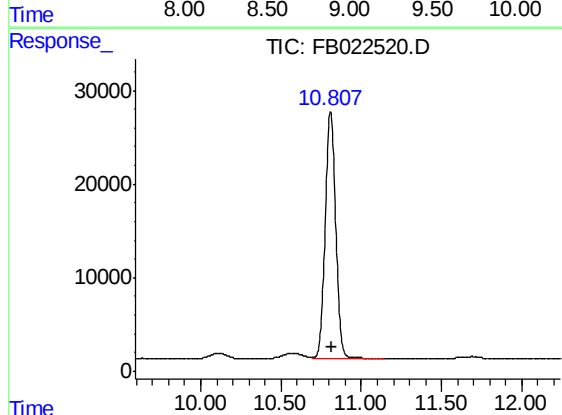


#6 Toluene

R.T.: 10.809 min
Delta R.T.: -0.011 min
Response: 1217062
Conc: 25.58 ng/ml

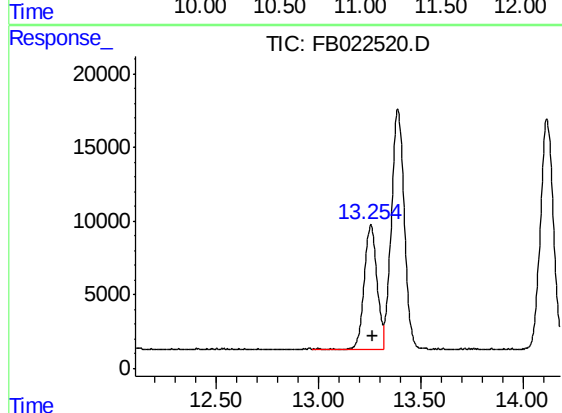


#7 Ethylbenzene

R.T.: 13.255 min
Delta R.T.: -0.010 min
Response: 363358
Conc: 12.12 ng/ml

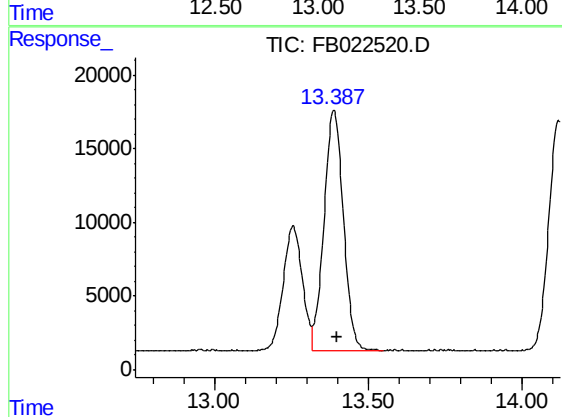

#8 m-Xylene


R.T.: 13.388 min
Delta R.T.: -0.010 min
Response: 712717
Conc: 26.83 ng/ml

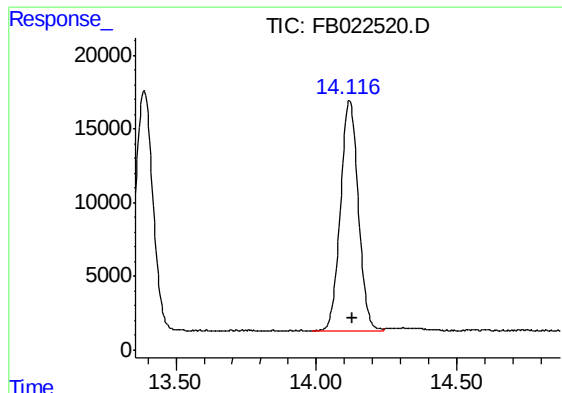

#9 O-Xylene

R.T.: 14.118 min
Delta R.T.: -0.010 min
Response: 687162
Conc: 28.32 ng/ml

Instrument :
FID_B
ClientSampleId :
RBR-200052MSD

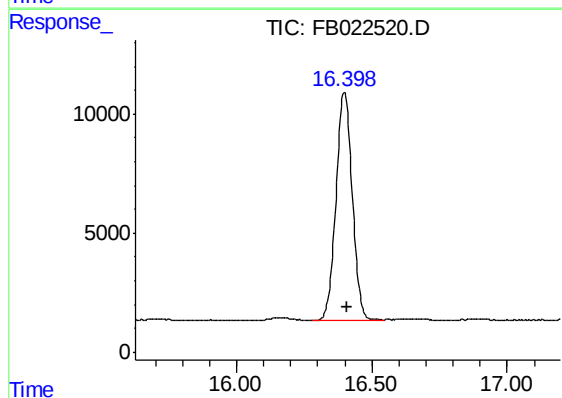

#10 1,2,4-Trimethylbenzene

R.T.: 16.399 min
Delta R.T.: -0.008 min
Response: 400236
Conc: 15.35 ng/ml