

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091620\
 Data File : FB024882.D
 Signal(s) : FID2B.CH
 Acq On : 16 Sep 2020 11:29
 Operator : DD/AJ
 Sample : BSF0916S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0916S1

Integration File: Calibration.e
 Quant Time: Sep 17 01:08:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
 Quant Title :
 QLast Update : Tue Sep 15 13:37:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	411252	18.482 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	933244	31.732 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	960348	31.831 ng/ml
3) t n-Heptane	7.757	316332	10.443 ng/ml
4) t Benzene	7.892	378148	9.770 ng/ml
6) t Toluene	10.629	1051878	28.870 ng/ml
7) t Ethylbenzene	13.068	316936	9.429 ng/ml
8) t m-Xylene	13.201	631603	19.281 ng/ml
9) t O-Xylene	13.929	617739	19.339 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	515940	19.785 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091620\
Data File : FB024882.D
Signal(s) : FID2B.CH
Acq On : 16 Sep 2020 11:29
Operator : DD/AJ
Sample : BSF0916S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0916S1

Integration File: Calibration.e
Quant Time: Sep 17 01:08:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
Quant Title :
QLast Update : Tue Sep 15 13:37:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

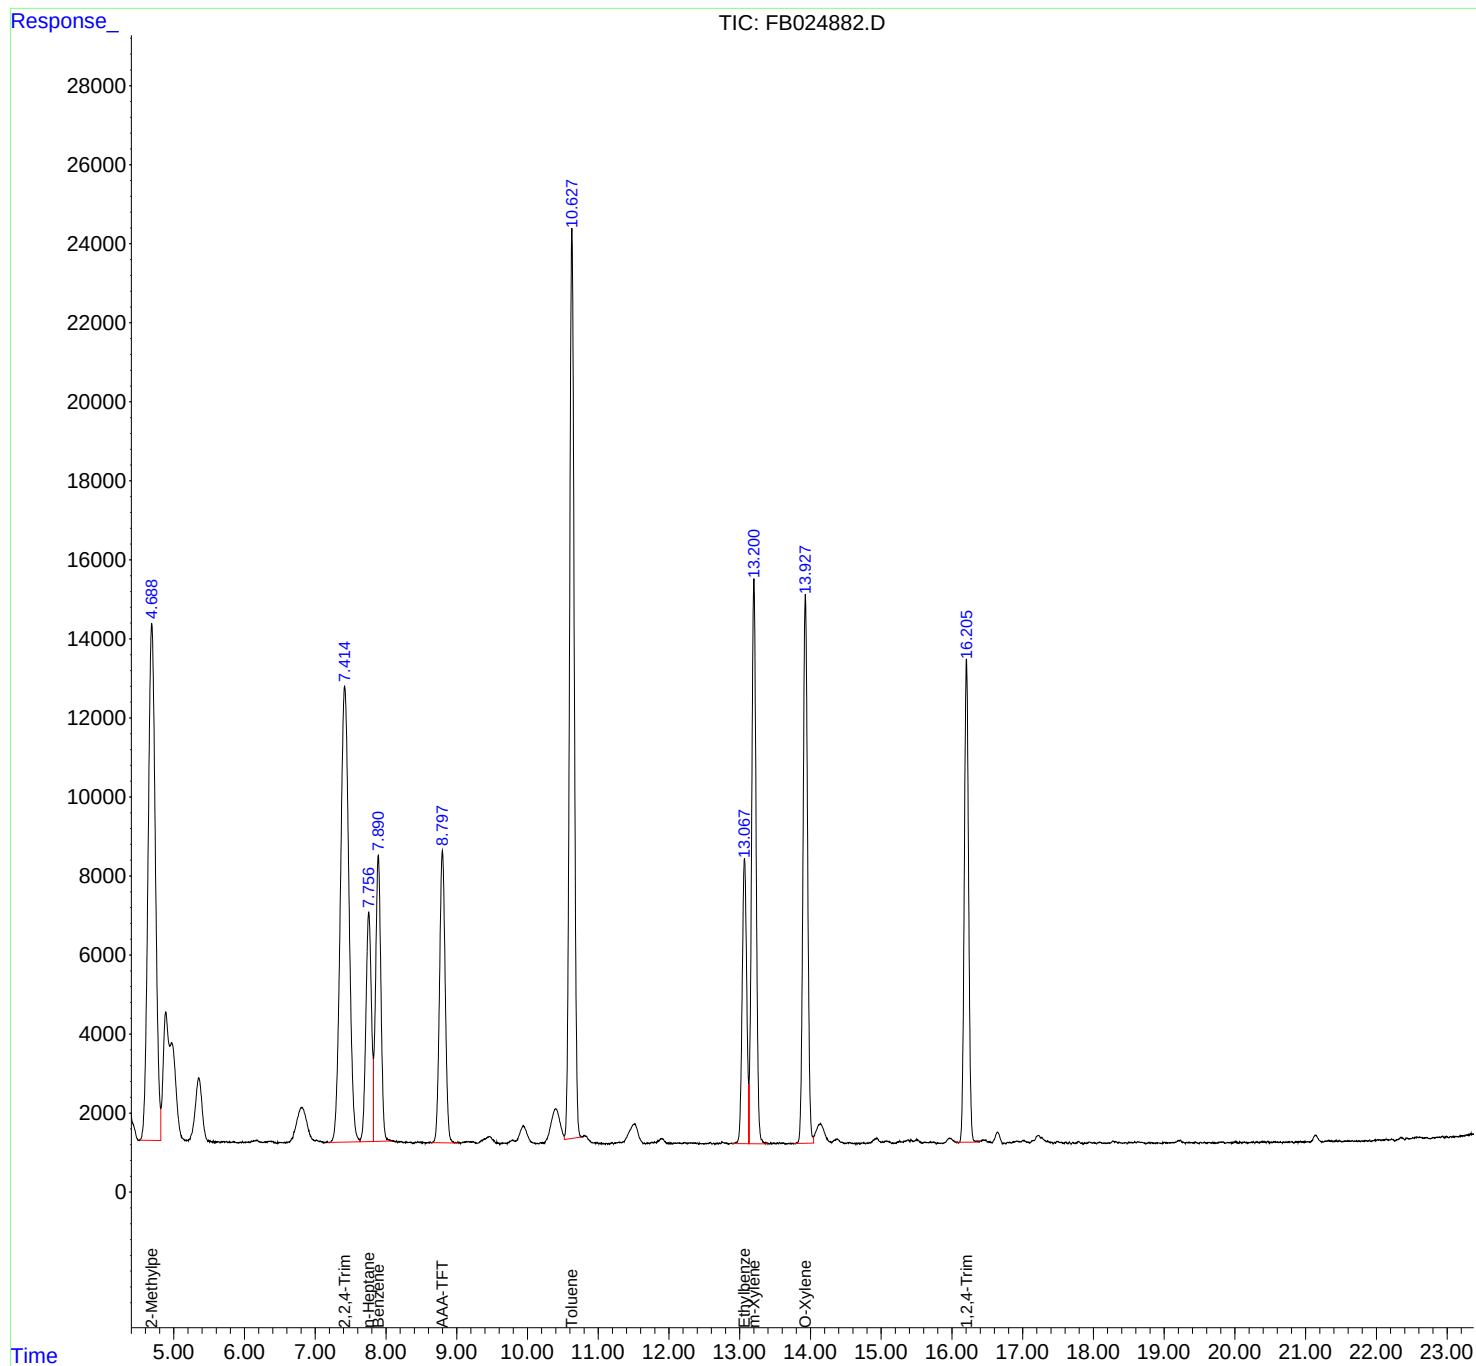


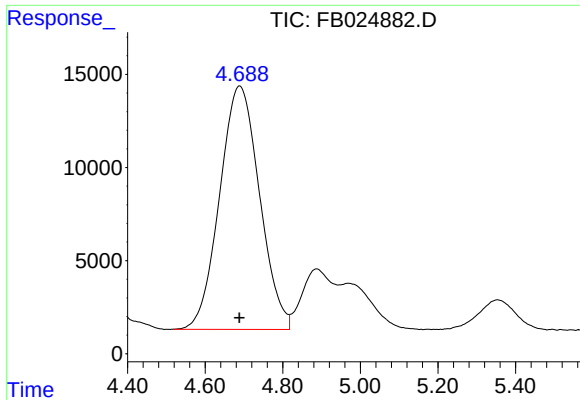

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.002 min
Response: 933244
Conc: 31.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0916S1

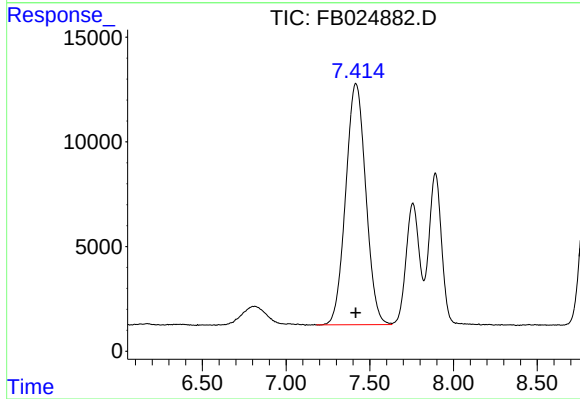


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 960348
Conc: 31.83 ng/ml

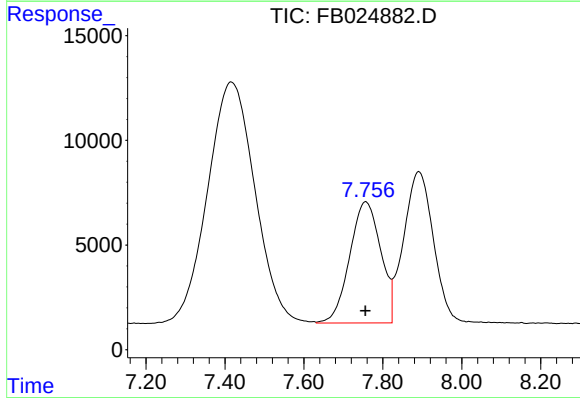


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.001 min
Response: 316332
Conc: 10.44 ng/ml

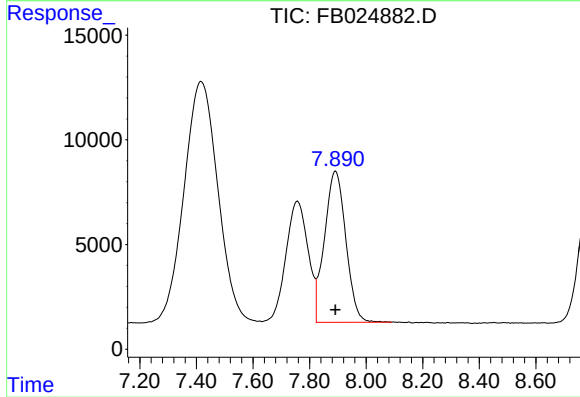

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 378148
Conc: 9.77 ng/ml

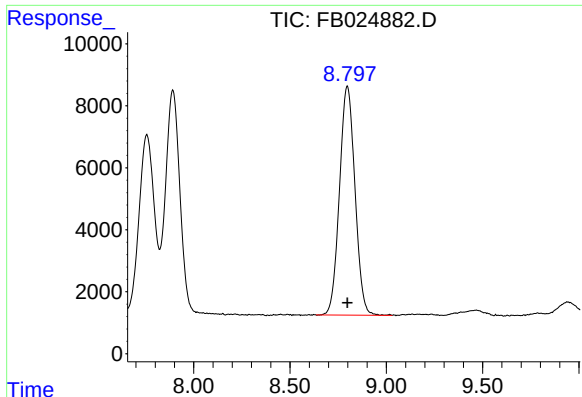

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 411252
Conc: 18.48 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0916S1

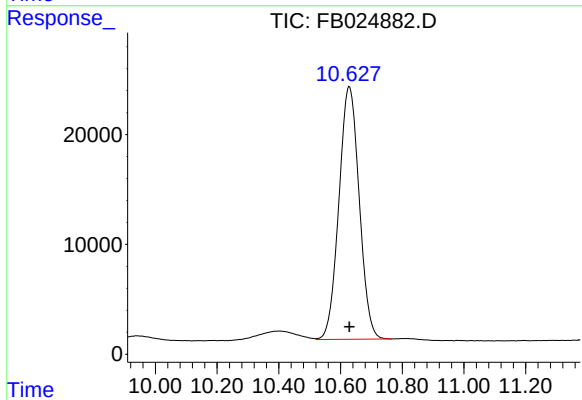


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 1051878
Conc: 28.87 ng/ml

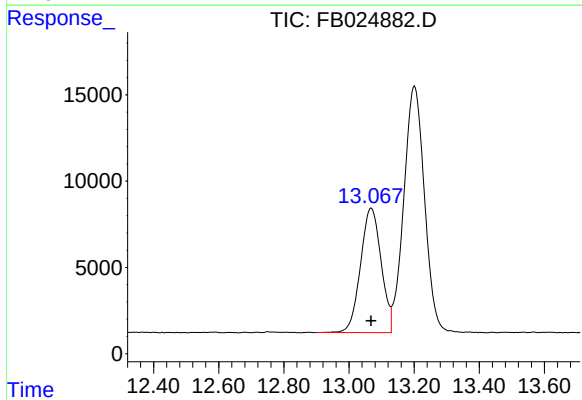


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: 0.000 min
Response: 316936
Conc: 9.43 ng/ml

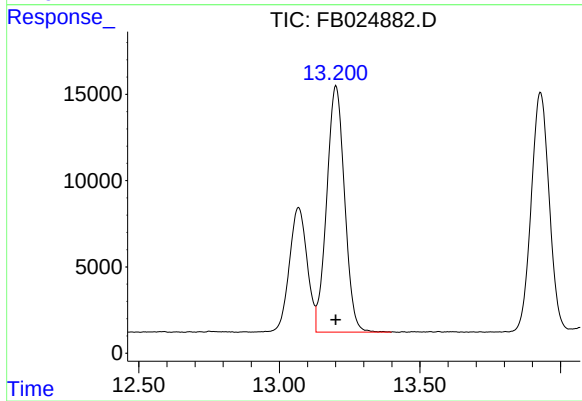

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 631603
Conc: 19.28 ng/ml

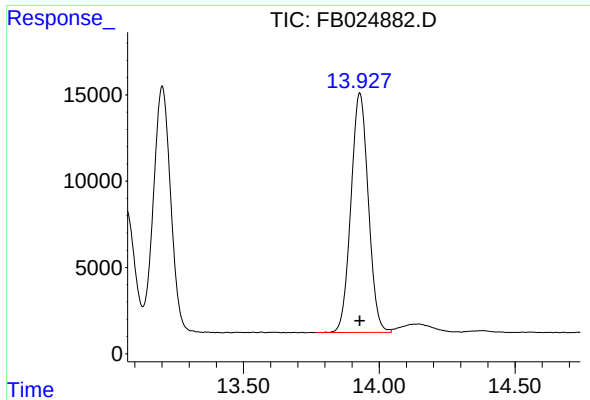

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.000 min
Response: 617739
Conc: 19.34 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0916S1

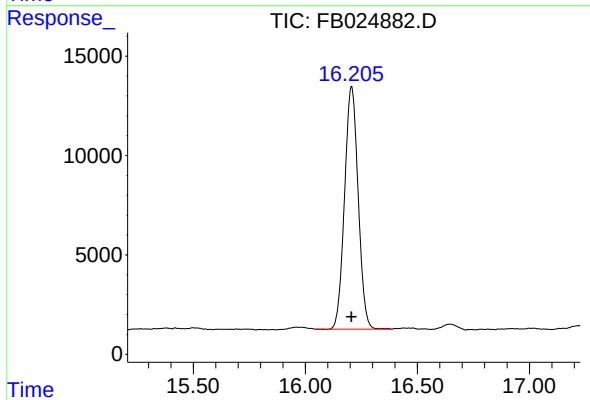

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.000 min
Response: 515940
Conc: 19.78 ng/ml