

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091620\
Data File : FB024885.D
Signal(s) : FID2B.CH
Acq On : 16 Sep 2020 13:11
Operator : DD/AJ
Sample : L4020-03
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
ETGI-370

Integration File: Calibration.e
Quant Time: Sep 17 01:08:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
Quant Title :
QLast Update : Tue Sep 15 13:37:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	361277	16.236 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091620\
Data File : FB024885.D
Signal(s) : FID2B.CH
Acq On : 16 Sep 2020 13:11
Operator : DD/AJ
Sample : L4020-03
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
ETGI-370

Integration File: Calibration.e
Quant Time: Sep 17 01:08:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
Quant Title :
QLast Update : Tue Sep 15 13:37:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

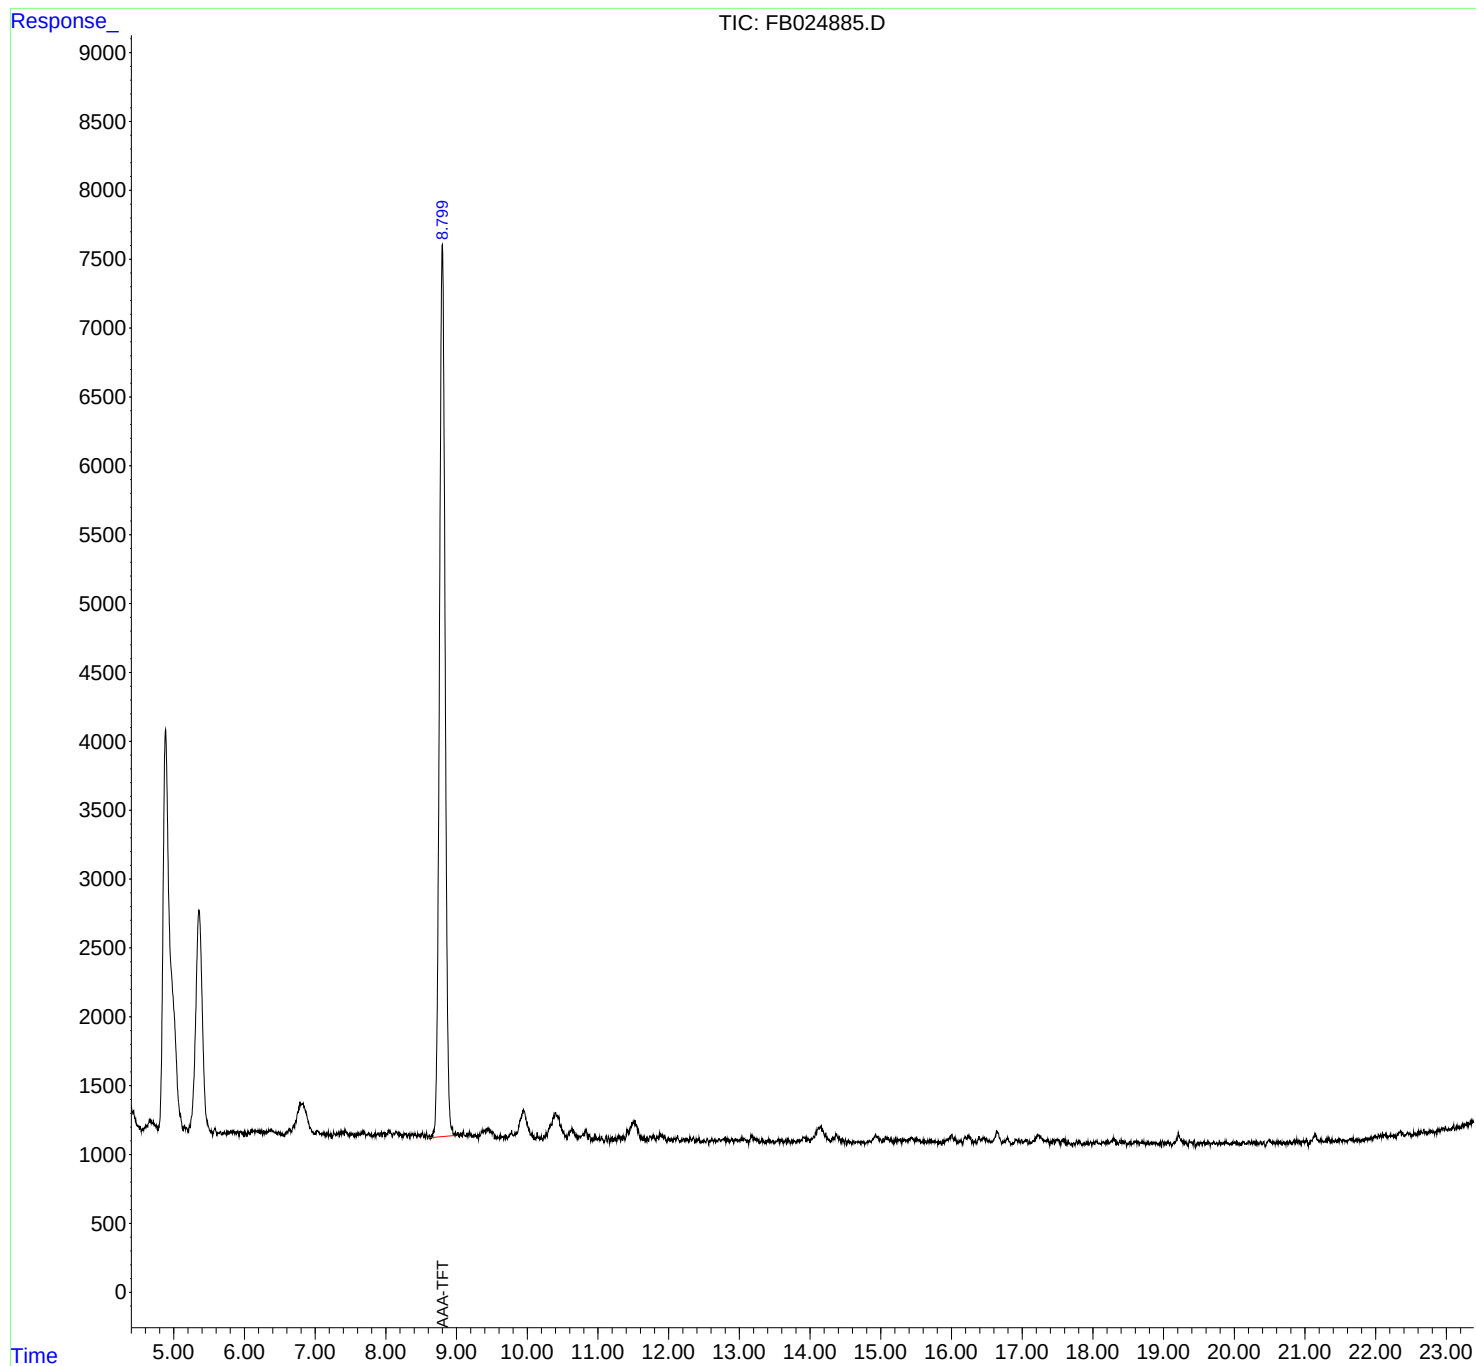

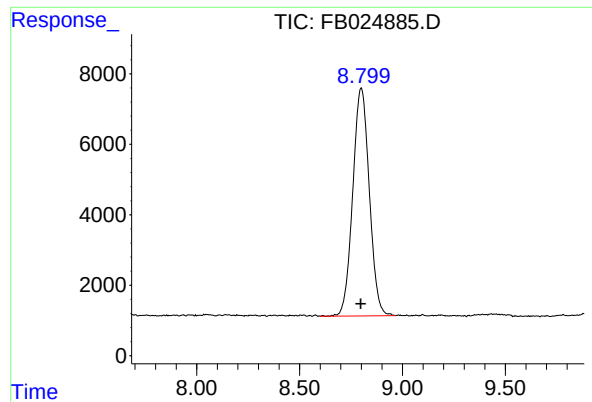

#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.002 min
Response: 361277
Conc: 16.24 ng/ml

Instrument :
FID_B
ClientSampleId :
ETGI-370