

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091620\
 Data File : FB024886.D
 Signal(s) : FID2B.CH
 Acq On : 16 Sep 2020 13:42
 Operator : DD/AJ
 Sample : L4020-01MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 ETGI-362MS

Integration File: Calibration.e
 Quant Time: Sep 17 01:08:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
 Quant Title :
 QLast Update : Tue Sep 15 13:37:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	371605	16.700 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	774841	26.346 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	744111	24.664 ng/ml
3) t n-Heptane	7.758	244966	8.087 ng/ml
4) t Benzene	7.893	323545	8.359 ng/ml
6) t Toluene	10.630	902002	24.757 ng/ml
7) t Ethylbenzene	13.070	270208	8.039 ng/ml
8) t m-Xylene	13.203	530363	16.190 ng/ml
9) t O-Xylene	13.930	510213	15.973 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	405978	15.568 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091620\
Data File : FB024886.D
Signal(s) : FID2B.CH
Acq On : 16 Sep 2020 13:42
Operator : DD/AJ
Sample : L4020-01MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
ETGI-362MS

Integration File: Calibration.e
Quant Time: Sep 17 01:08:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
Quant Title :
QLast Update : Tue Sep 15 13:37:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

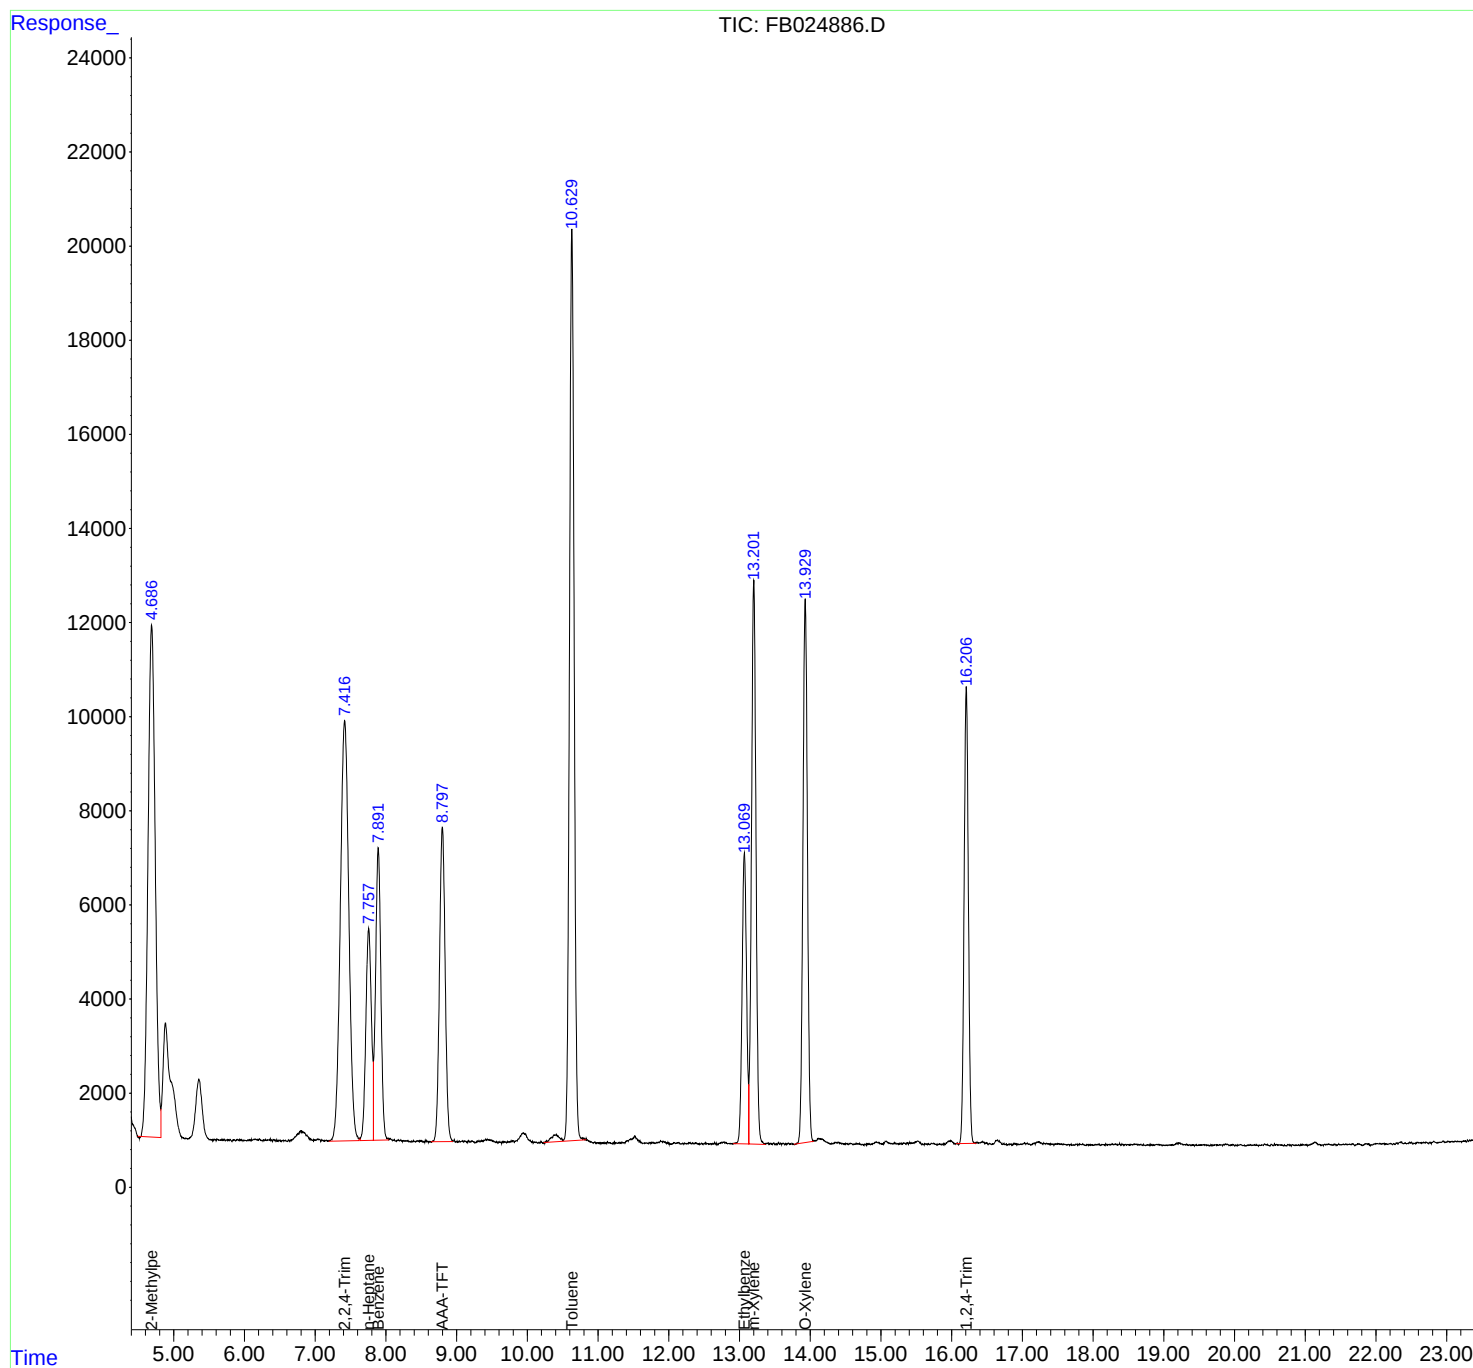


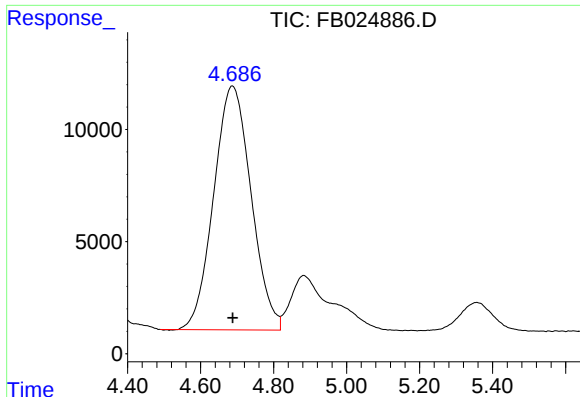

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 774841
Conc: 26.35 ng/ml

Instrument :
FID_B
ClientSampleId :
ETGI-362MS

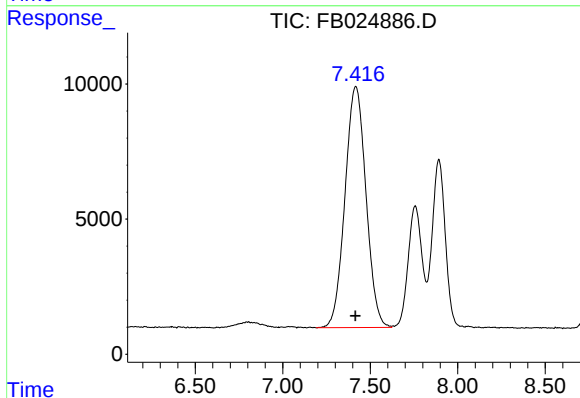


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.002 min
Response: 744111
Conc: 24.66 ng/ml

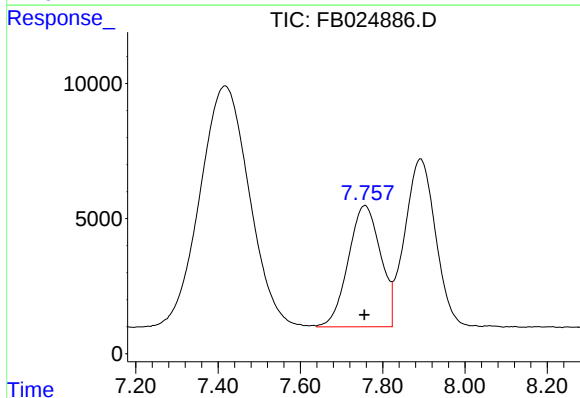


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.002 min
Response: 244966
Conc: 8.09 ng/ml

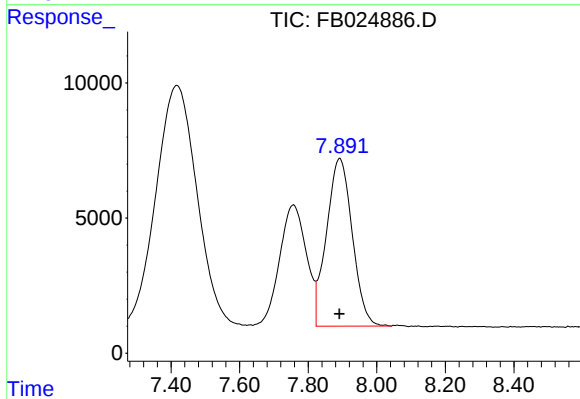

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.001 min
Response: 323545
Conc: 8.36 ng/ml

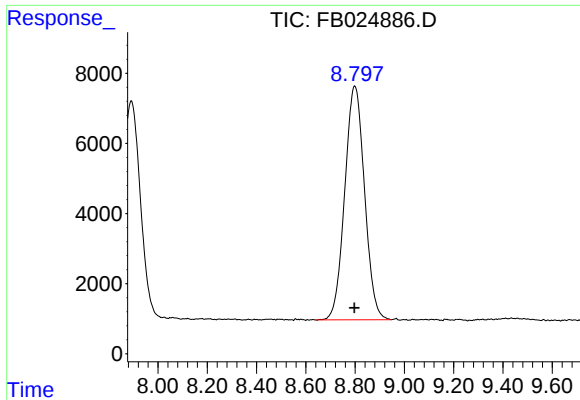

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.001 min
Response: 371605
Conc: 16.70 ng/ml

Instrument :
FID_B
ClientSampleId :
ETGI-362MS

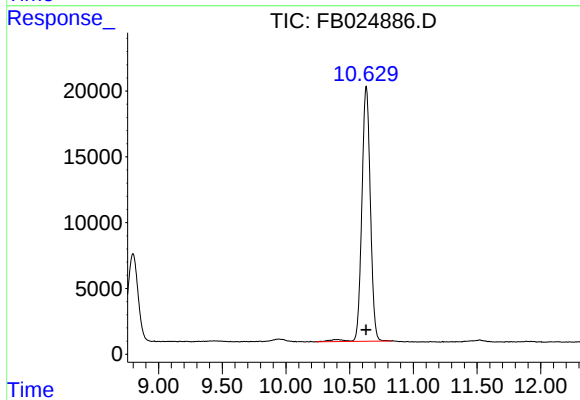


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.002 min
Response: 902002
Conc: 24.76 ng/ml

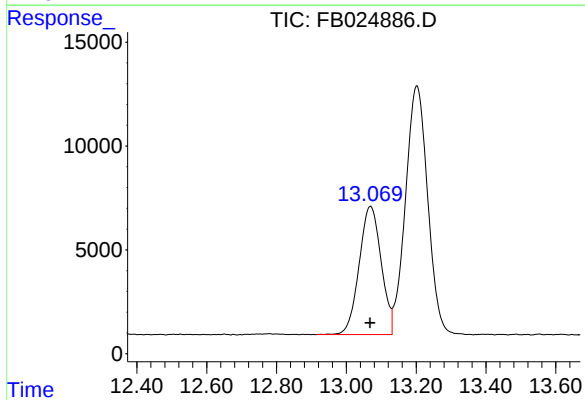


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.002 min
Response: 270208
Conc: 8.04 ng/ml

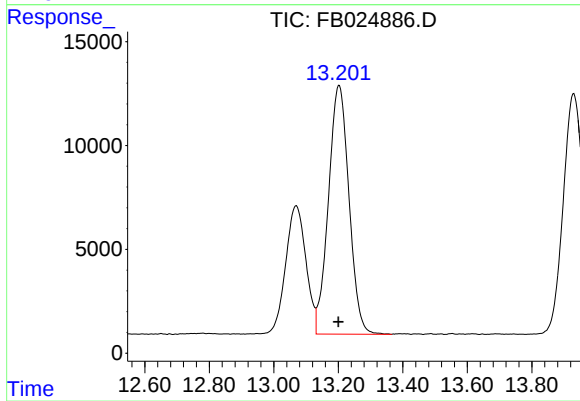

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.002 min
Response: 530363
Conc: 16.19 ng/ml

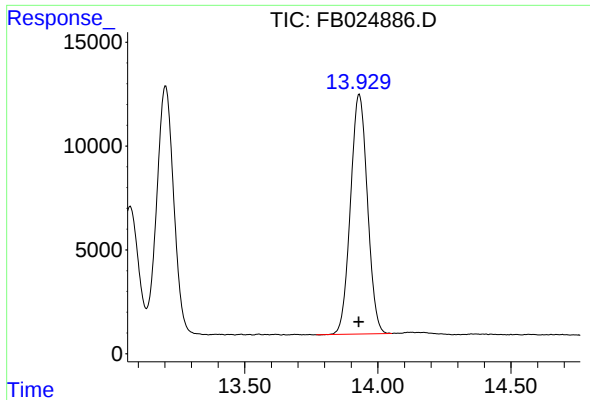

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.002 min
Response: 510213
Conc: 15.97 ng/ml

Instrument :
FID_B
ClientSampleId :
ETGI-362MS

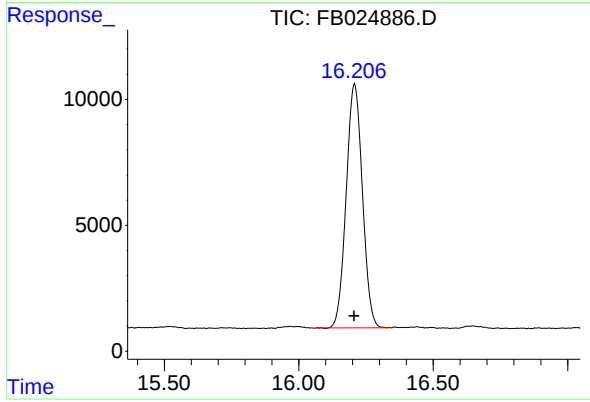

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.002 min
Response: 405978
Conc: 15.57 ng/ml