

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091620\
 Data File : FB024887.D
 Signal(s) : FID2B.CH
 Acq On : 16 Sep 2020 14:13
 Operator : DD/AJ
 Sample : L4020-01MSD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 ETGI-362MSD

Integration File: Calibration.e
 Quant Time: Sep 17 01:08:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
 Quant Title :
 QLast Update : Tue Sep 15 13:37:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	267106	12.004 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	557274	18.948 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	500787	16.599 ng/ml
3) t n-Heptane	7.758	163399	5.394 ng/ml
4) t Benzene	7.894	244234	6.310 ng/ml
6) t Toluene	10.631	633471	17.387 ng/ml
7) t Ethylbenzene	13.071	186339	5.544 ng/ml
8) t m-Xylene	13.203	366761	11.196 ng/ml
9) t O-Xylene	13.931	356079	11.148 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	272161	10.436 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091620\
Data File : FB024887.D
Signal(s) : FID2B.CH
Acq On : 16 Sep 2020 14:13
Operator : DD/AJ
Sample : L4020-01MSD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
ETGI-362MSD

Integration File: Calibration.e
Quant Time: Sep 17 01:08:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
Quant Title :
QLast Update : Tue Sep 15 13:37:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

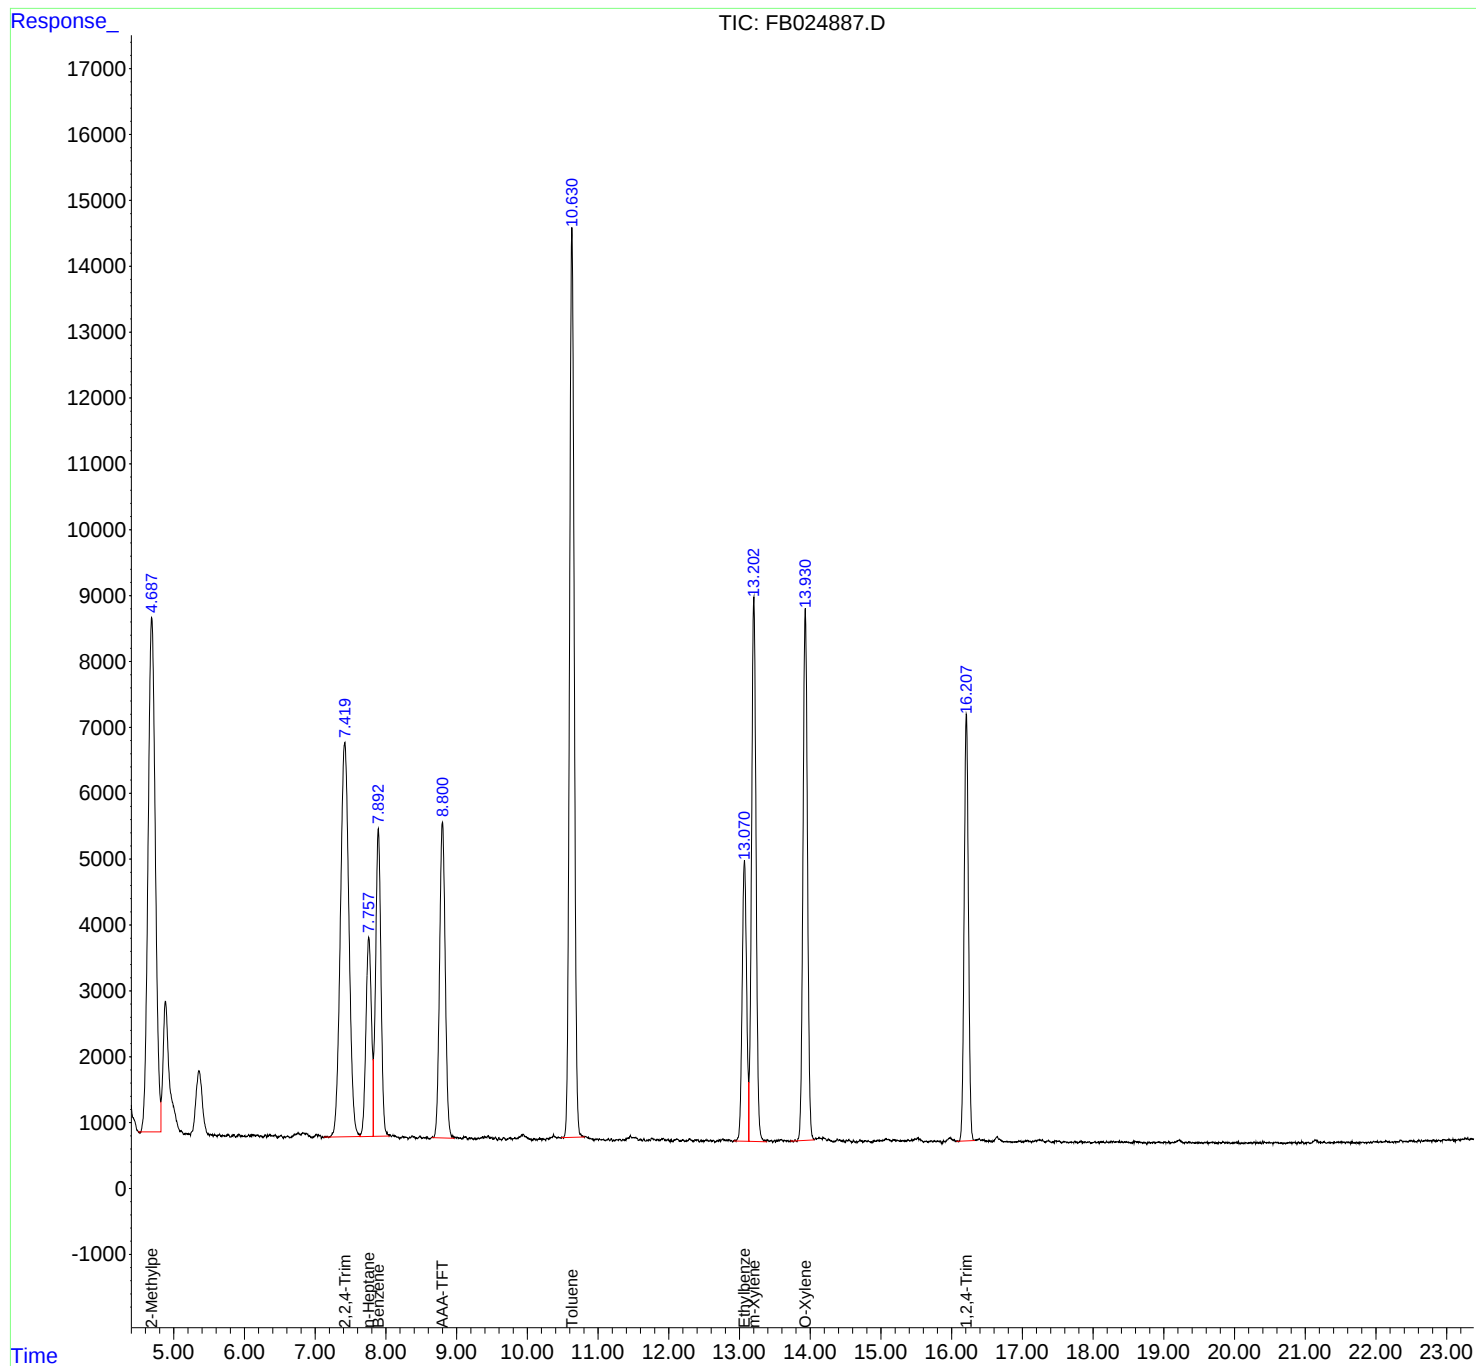


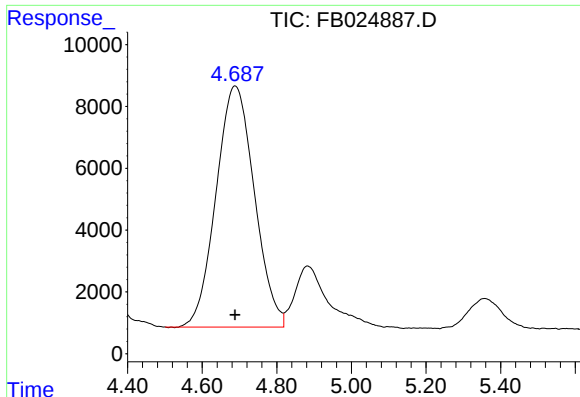

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 557274
Conc: 18.95 ng/ml

Instrument :
FID_B
ClientSampleId :
ETGI-362MSD

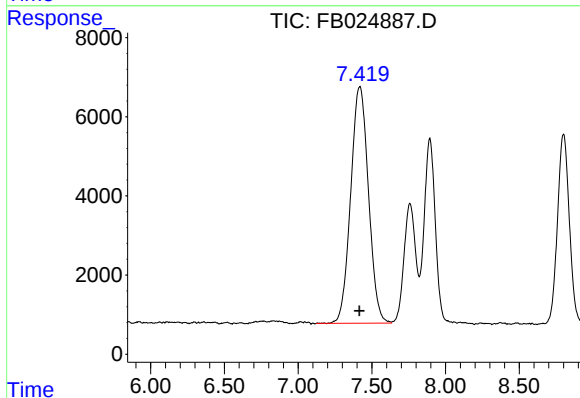


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.005 min
Response: 500787
Conc: 16.60 ng/ml

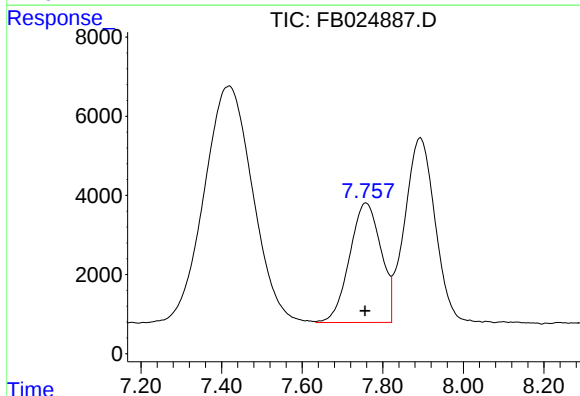


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.003 min
Response: 163399
Conc: 5.39 ng/ml

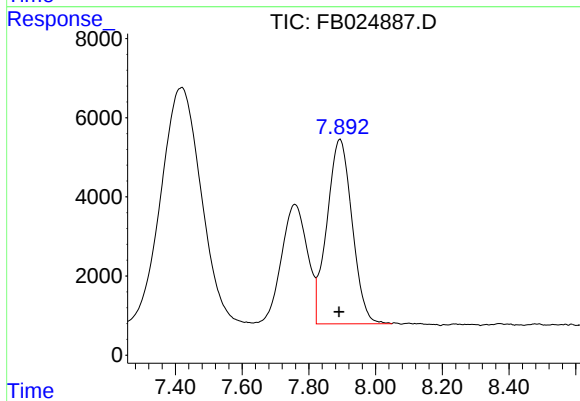

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.003 min
Response: 244234
Conc: 6.31 ng/ml

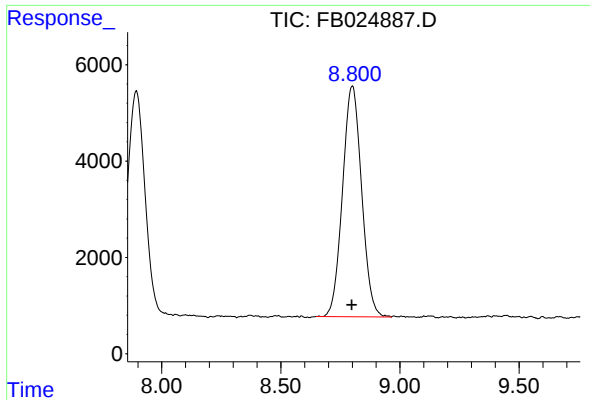

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.003 min
Response: 267106
Conc: 12.00 ng/ml

Instrument :
FID_B
ClientSampleId :
ETGI-362MSD

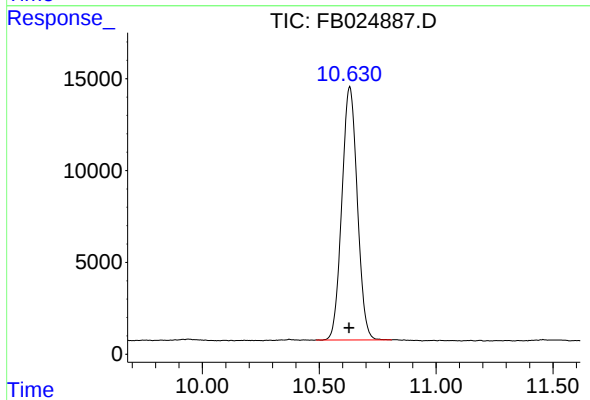


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.002 min
Response: 633471
Conc: 17.39 ng/ml

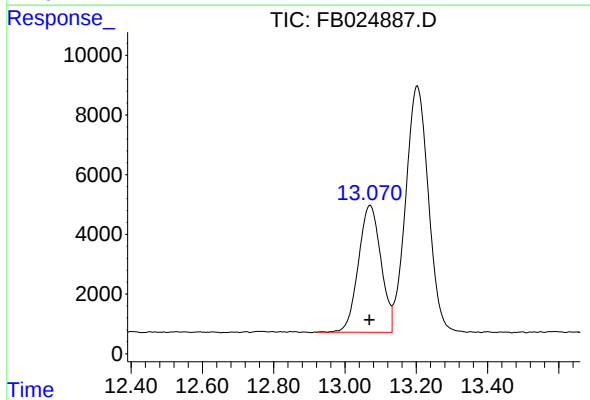


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.003 min
Response: 186339
Conc: 5.54 ng/ml

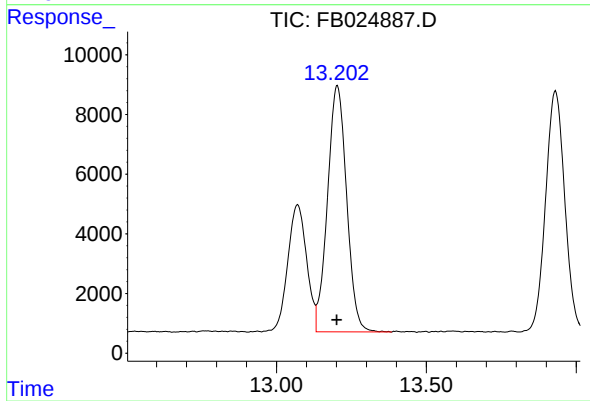

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.002 min
Response: 366761
Conc: 11.20 ng/ml

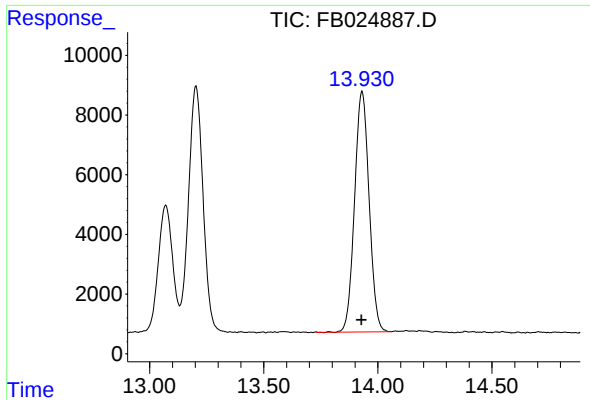

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.002 min
Response: 356079
Conc: 11.15 ng/ml

Instrument :
FID_B
ClientSampleId :
ETGI-362MSD

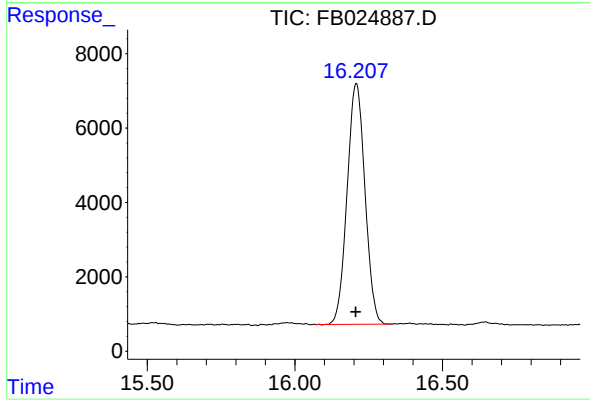

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.003 min
Response: 272161
Conc: 10.44 ng/ml