

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091621\
 Data File : FB026225.D
 Signal(s) : FID2B.CH
 Acq On : 16 Sep 2021 13:34
 Operator : AJ/MA
 Sample : FB091621GROICV
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 16 16:25:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
 Quant Title :
 QLast Update : Thu Sep 16 16:24:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.838	339520	19.935 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.832	680867	30.645 ng/ml
2) t 2,2,4-Trimethylpentane	7.496	689567	31.024 ng/ml
3) t n-Heptane	7.813	268277	10.388 ng/ml
4) t Benzene	7.950	282000	10.354 ng/ml
6) t Toluene	10.649	802180	30.606 ng/ml
7) t Ethylbenzene	13.069	234821	10.298 ng/ml
8) t m-Xylene	13.201	454106	20.256 ng/ml
9) t O-Xylene	13.925	424118	19.973 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	443494	19.667 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091621\
Data File : FB026225.D
Signal(s) : FID2B.CH
Acq On : 16 Sep 2021 13:34
Operator : AJ/MA
Sample : FB091621GR0ICV
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 16 16:25:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
Quant Title :
QLast Update : Thu Sep 16 16:24:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

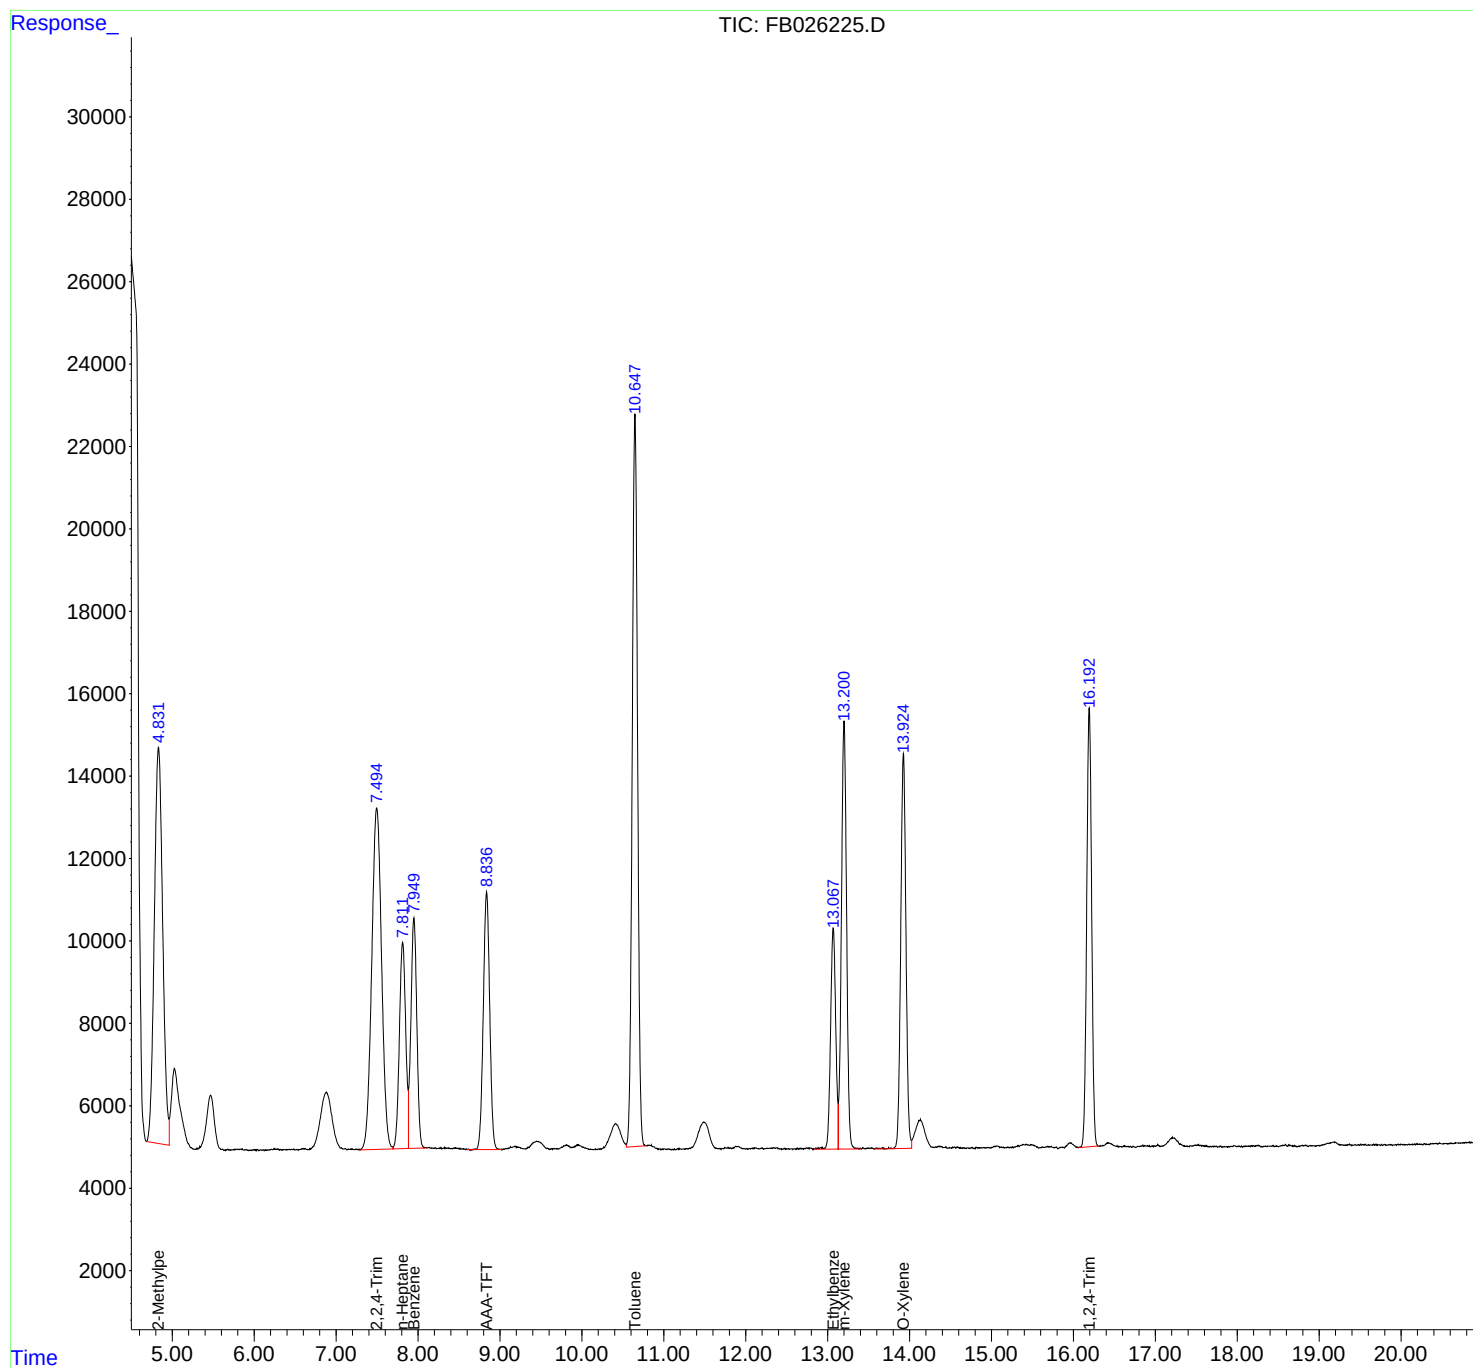


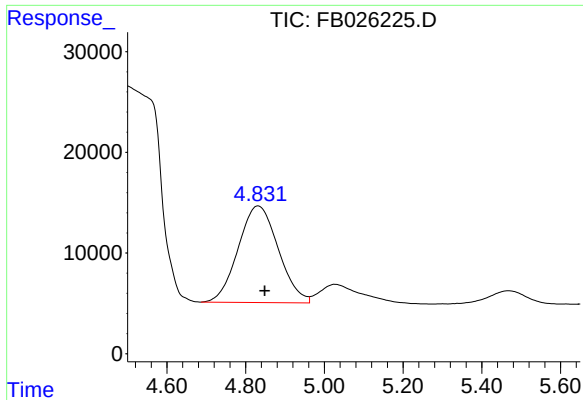

#1 2-Methylpentane


R.T.: 4.832 min
Delta R.T.: -0.016 min
Response: 680867
Conc: 30.64 ng/ml

Instrument :
FID_B
ClientSampleId :

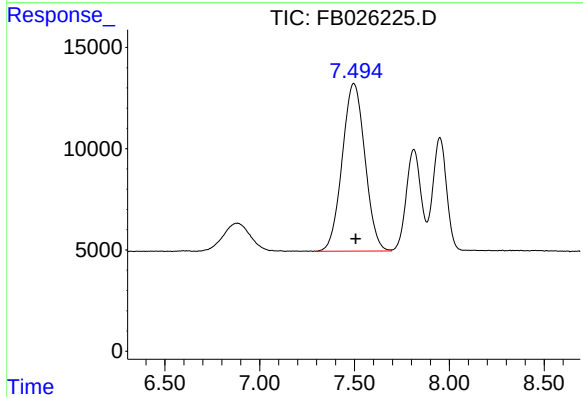


#2 2,2,4-Trimethylpentane

R.T.: 7.496 min
Delta R.T.: -0.011 min
Response: 689567
Conc: 31.02 ng/ml

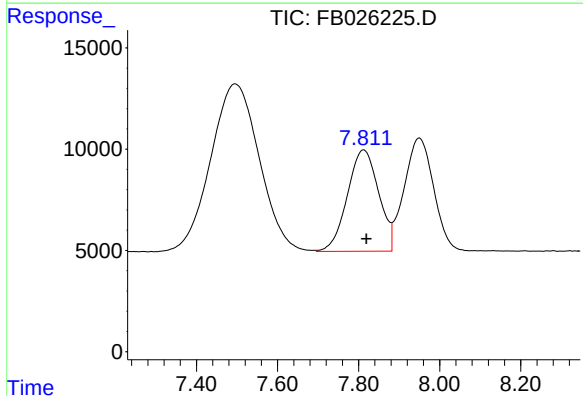


#3 n-Heptane

R.T.: 7.813 min
Delta R.T.: -0.006 min
Response: 268277
Conc: 10.39 ng/ml

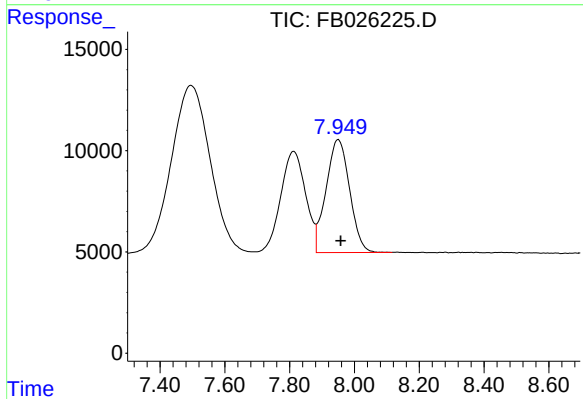

#4 Benzene


R.T.: 7.950 min
Delta R.T.: -0.007 min
Response: 282000
Conc: 10.35 ng/ml

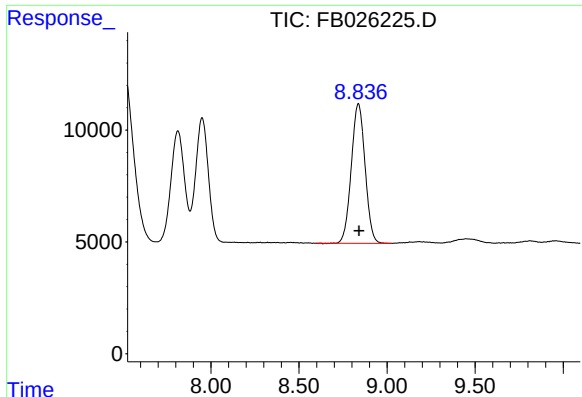

#5 AAA-TFT


R.T.: 8.838 min
Delta R.T.: -0.004 min
Response: 339520
Conc: 19.94 ng/ml

Instrument :
FID_B
ClientSampleId :

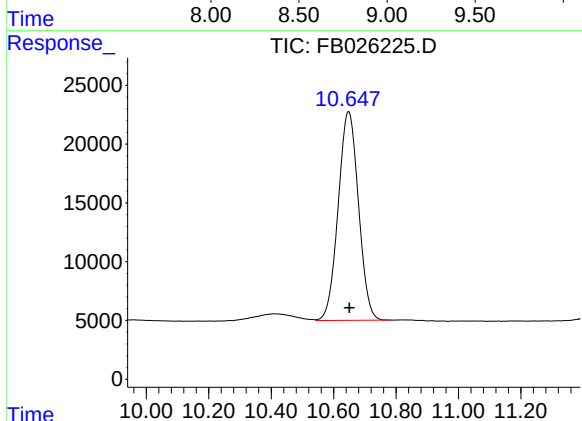


#6 Toluene

R.T.: 10.649 min
Delta R.T.: -0.003 min
Response: 802180
Conc: 30.61 ng/ml

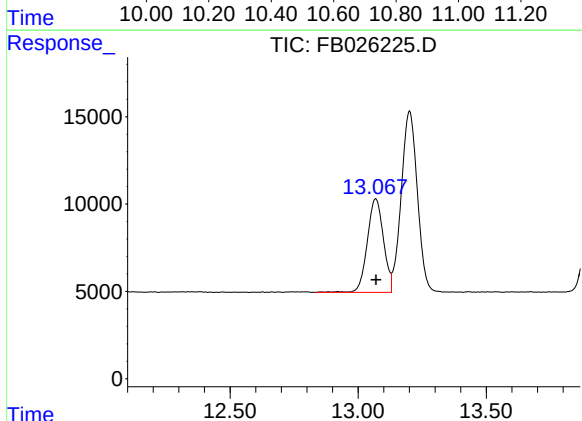


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 234821
Conc: 10.30 ng/ml

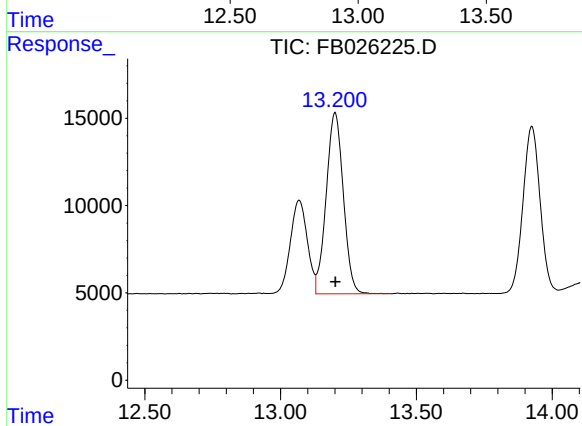

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 454106
Conc: 20.26 ng/ml

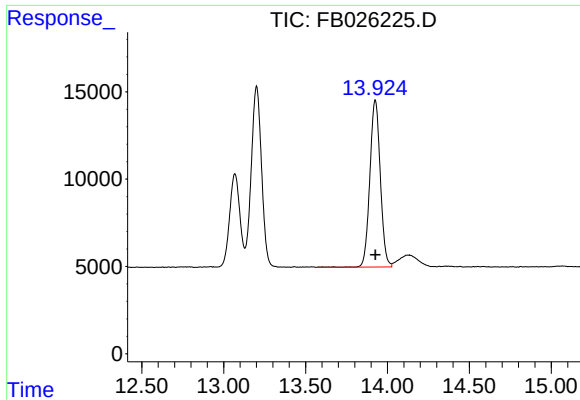

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.000 min
Response: 424118
Conc: 19.97 ng/ml

Instrument :
FID_B
ClientSampleId :

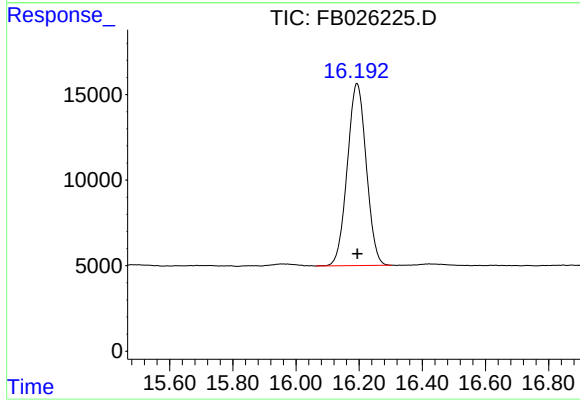

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 443494
Conc: 19.67 ng/ml