

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091621\
 Data File : FB026220.D
 Signal(s) : FID2B.CH
 Acq On : 16 Sep 2021 10:17
 Operator : AJ/MA
 Sample : 5 GRO STD
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 5 GRO STD

Integration File: Calibration.e
 Quant Time: Sep 16 16:21:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
 Quant Title :
 QLast Update : Thu Sep 16 16:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.833	83722	4.894 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.827	167508	7.458 ng/ml
2) t 2,2,4-Trimethylpentane	7.492	163978	7.362 ng/ml
3) t n-Heptane	7.809	63289	2.483 ng/ml
4) t Benzene	7.947	62245	2.277 ng/ml
6) t Toluene	10.646	190461	7.257 ng/ml
7) t Ethylbenzene	13.065	55961	2.460 ng/ml
8) t m-Xylene	13.198	111421	4.968 ng/ml
9) t O-Xylene	13.923	107275	5.024 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	114325	5.087 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091621\
Data File : FB026220.D
Signal(s) : FID2B.CH
Acq On : 16 Sep 2021 10:17
Operator : AJ/MA
Sample : 5 GRO STD
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
5 GRO STD

Integration File: Calibration.e
Quant Time: Sep 16 16:21:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
Quant Title :
QLast Update : Thu Sep 16 16:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

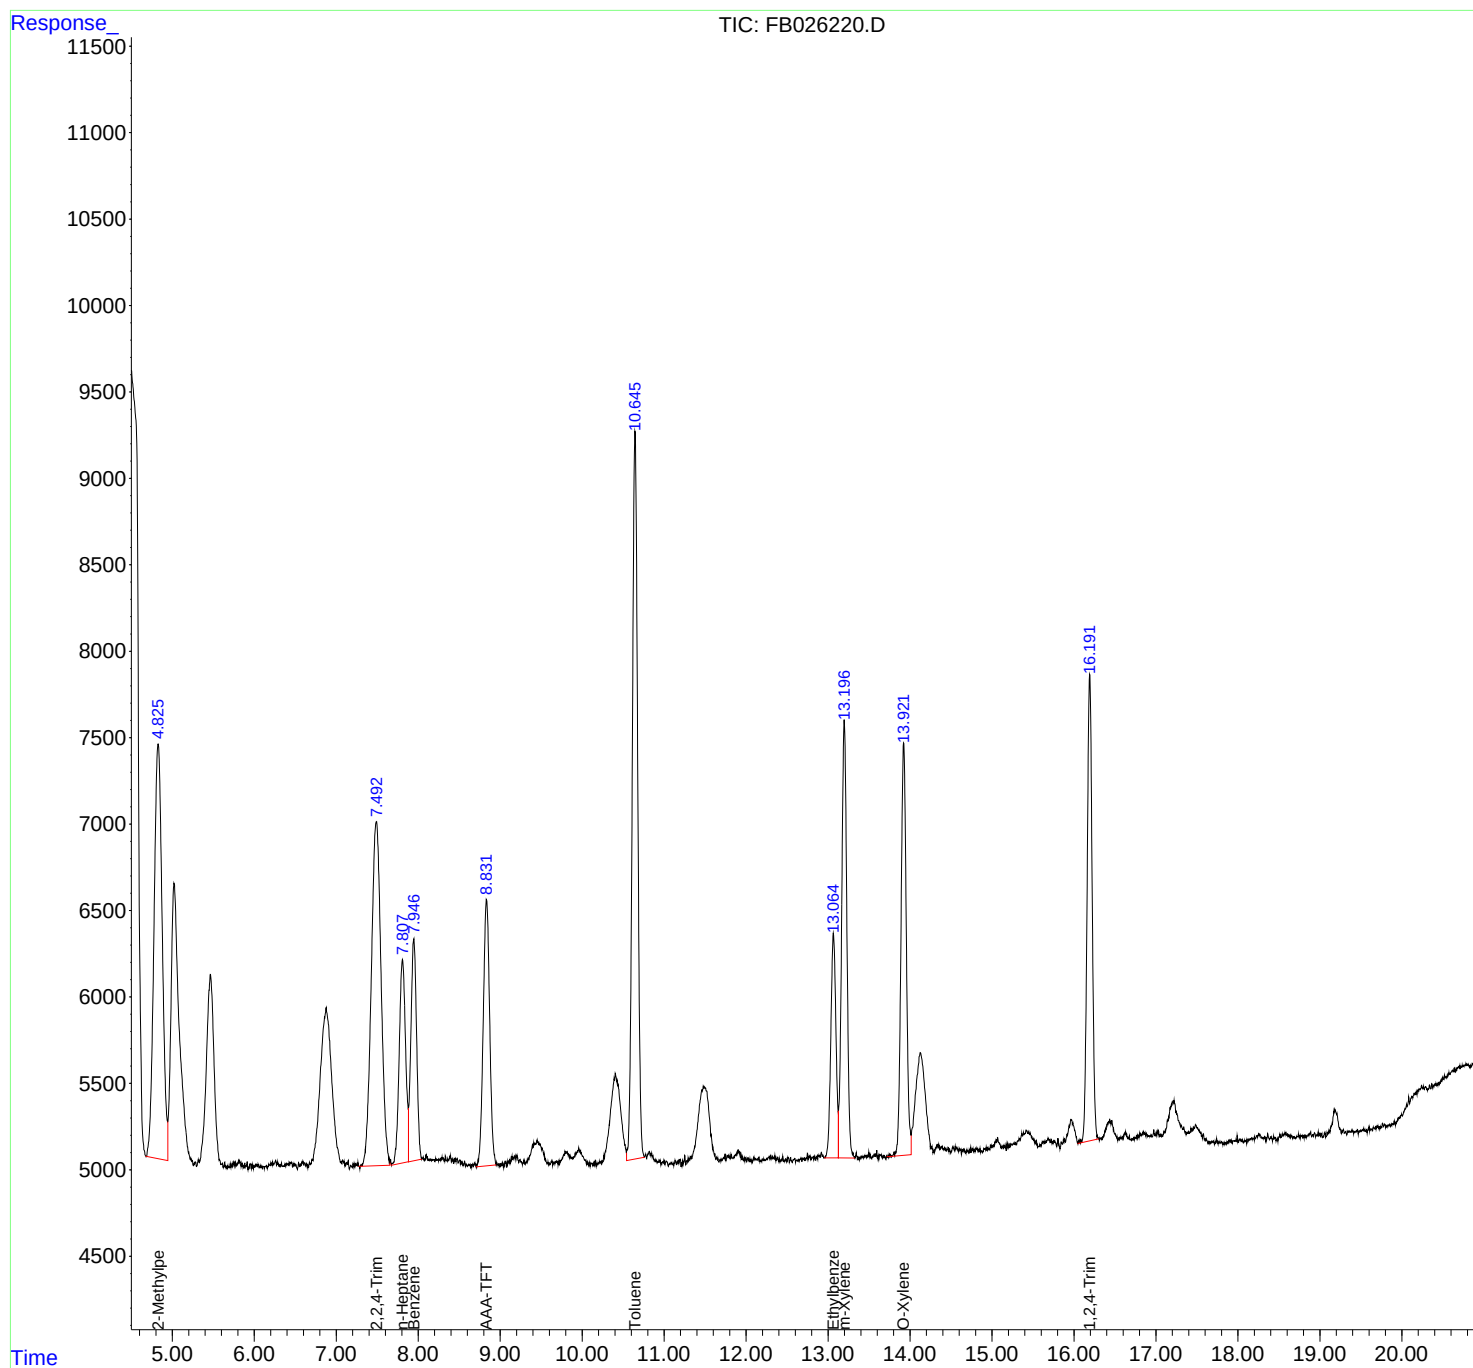


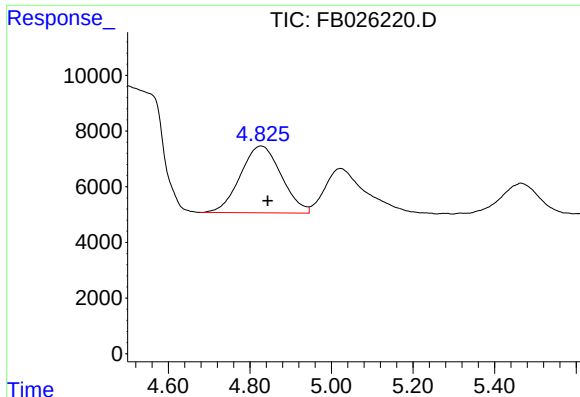

#1 2-Methylpentane


R.T.: 4.827 min
Delta R.T.: -0.017 min
Response: 167508
Conc: 7.46 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

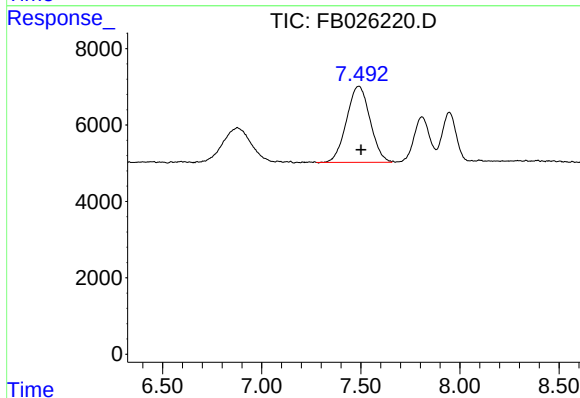


#2 2,2,4-Trimethylpentane

R.T.: 7.492 min
Delta R.T.: -0.009 min
Response: 163978
Conc: 7.36 ng/ml

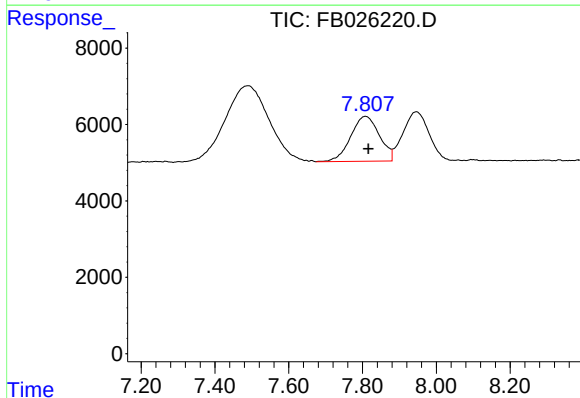


#3 n-Heptane

R.T.: 7.809 min
Delta R.T.: -0.007 min
Response: 63289
Conc: 2.48 ng/ml

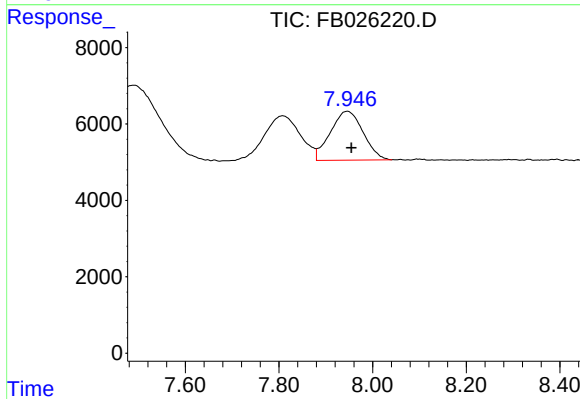

#4 Benzene


R.T.: 7.947 min
Delta R.T.: -0.007 min
Response: 62245
Conc: 2.28 ng/ml

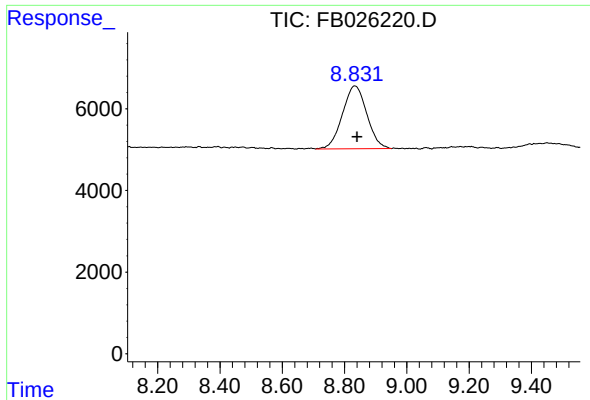

#5 AAA-TFT


R.T.: 8.833 min
Delta R.T.: -0.007 min
Response: 83722
Conc: 4.89 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

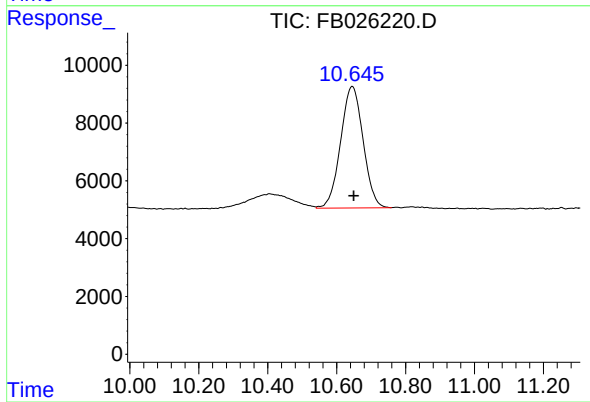


#6 Toluene

R.T.: 10.646 min
Delta R.T.: -0.004 min
Response: 190461
Conc: 7.26 ng/ml

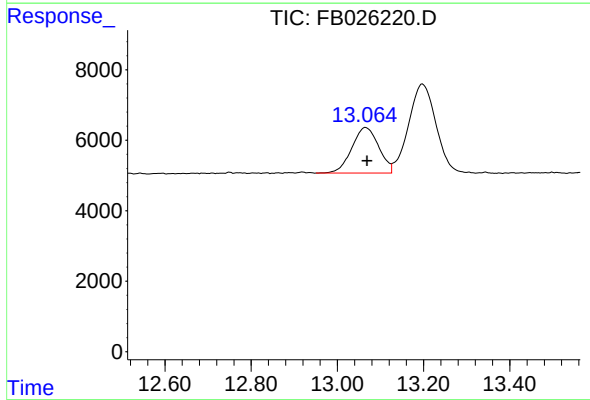


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.004 min
Response: 55961
Conc: 2.46 ng/ml

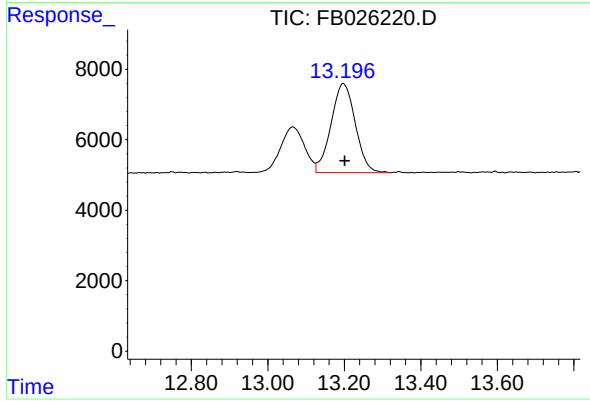

#8 m-Xylene


R.T.: 13.198 min
Delta R.T.: -0.003 min
Response: 111421
Conc: 4.97 ng/ml

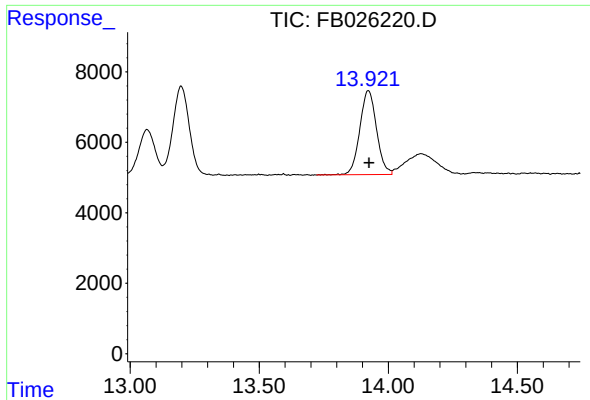

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: -0.002 min
Response: 107275
Conc: 5.02 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

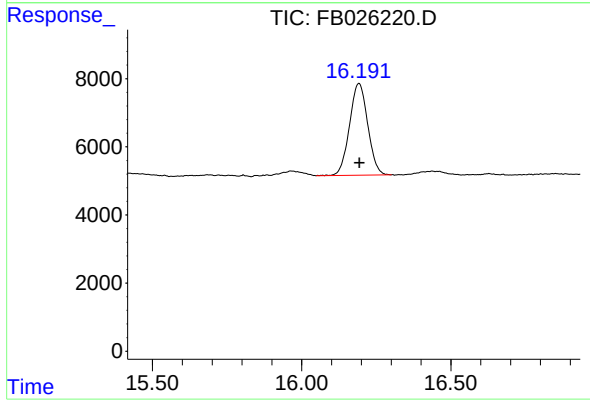

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 114325
Conc: 5.09 ng/ml