

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091621\
 Data File : FB026228.D
 Signal(s) : FID2B.CH
 Acq On : 16 Sep 2021 15:23
 Operator : AJ/MA
 Sample : BSF0916S1
 Misc : 5.00G/5.00ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0916S1

Integration File: Calibration.e
 Quant Time: Sep 16 16:25:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
 Quant Title :
 QLast Update : Thu Sep 16 16:24:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.837	335486	19.698 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.831	651941	29.343 ng/ml
2) t 2,2,4-Trimethylpentane	7.495	648173	29.162 ng/ml
3) t n-Heptane	7.812	253324	9.809 ng/ml
4) t Benzene	7.949	274893	10.093 ng/ml
6) t Toluene	10.649	778996	29.722 ng/ml
7) t Ethylbenzene	13.069	222836	9.772 ng/ml
8) t m-Xylene	13.201	437805	19.529 ng/ml
9) t O-Xylene	13.926	411927	19.399 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	425059	18.850 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091621\
Data File : FB026228.D
Signal(s) : FID2B.CH
Acq On : 16 Sep 2021 15:23
Operator : AJ/MA
Sample : BSF0916S1
Misc : 5.00G/5.00ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0916S1

Integration File: Calibration.e
Quant Time: Sep 16 16:25:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
Quant Title :
QLast Update : Thu Sep 16 16:24:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

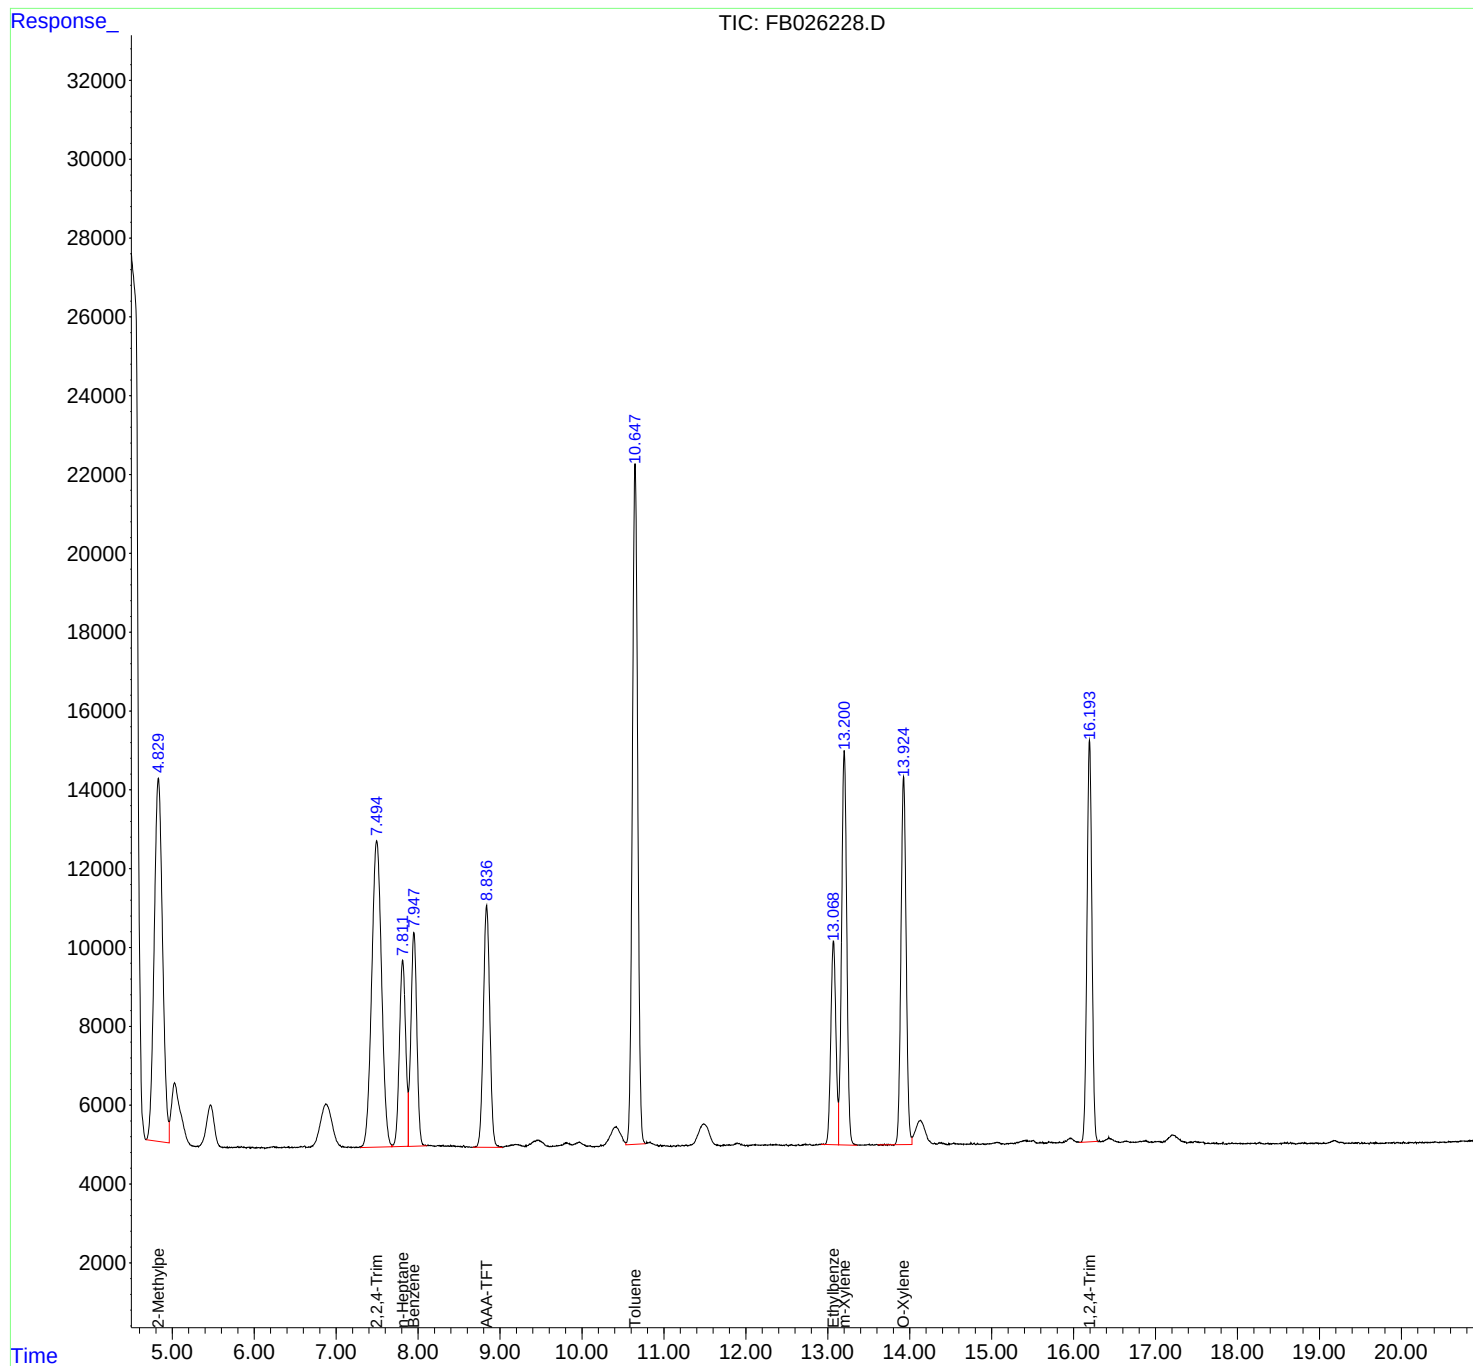


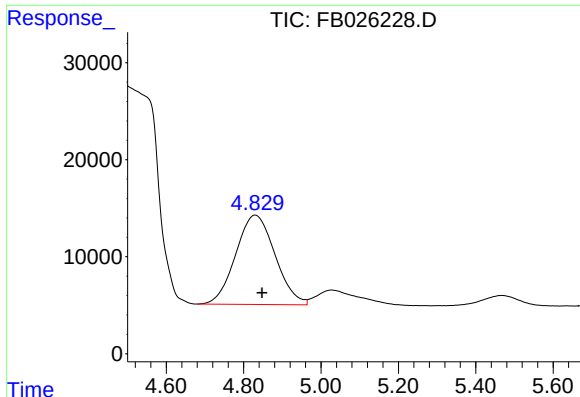

#1 2-Methylpentane


R.T.: 4.831 min
Delta R.T.: -0.017 min
Response: 651941
Conc: 29.34 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0916S1

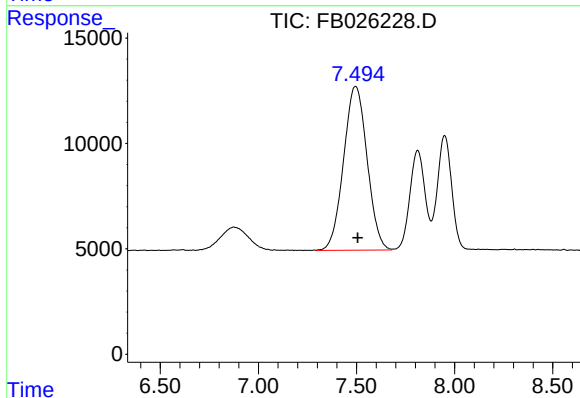


#2 2,2,4-Trimethylpentane

R.T.: 7.495 min
Delta R.T.: -0.011 min
Response: 648173
Conc: 29.16 ng/ml

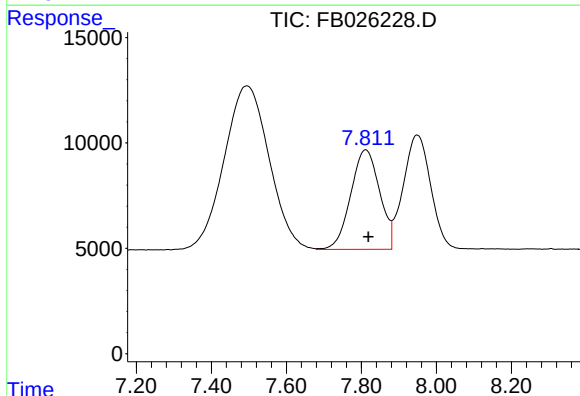


#3 n-Heptane

R.T.: 7.812 min
Delta R.T.: -0.007 min
Response: 253324
Conc: 9.81 ng/ml

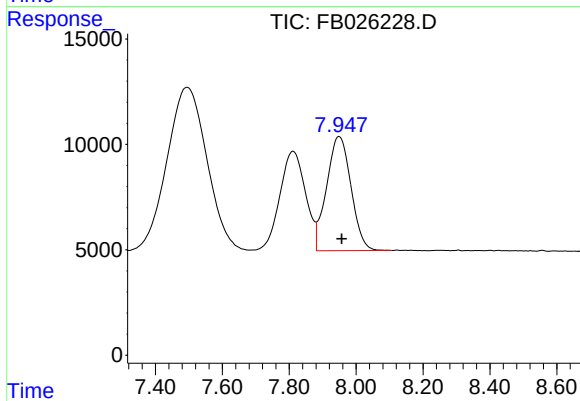

#4 Benzene


R.T.: 7.949 min
Delta R.T.: -0.008 min
Response: 274893
Conc: 10.09 ng/ml

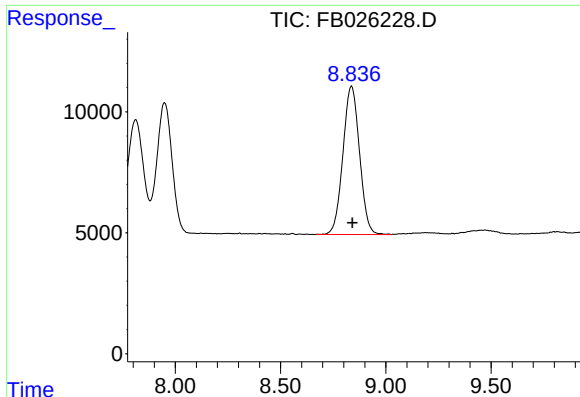

#5 AAA-TFT


R.T.: 8.837 min
Delta R.T.: -0.005 min
Response: 335486
Conc: 19.70 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0916S1

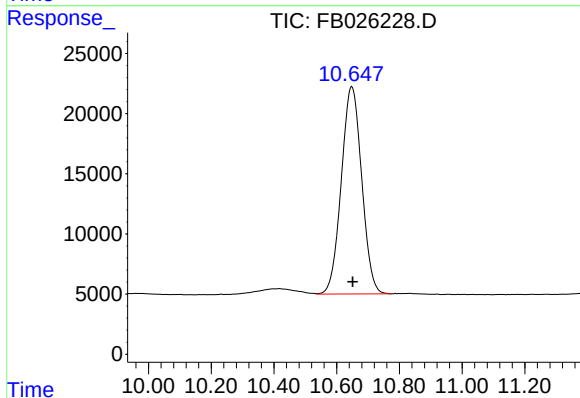


#6 Toluene

R.T.: 10.649 min
Delta R.T.: -0.003 min
Response: 778996
Conc: 29.72 ng/ml

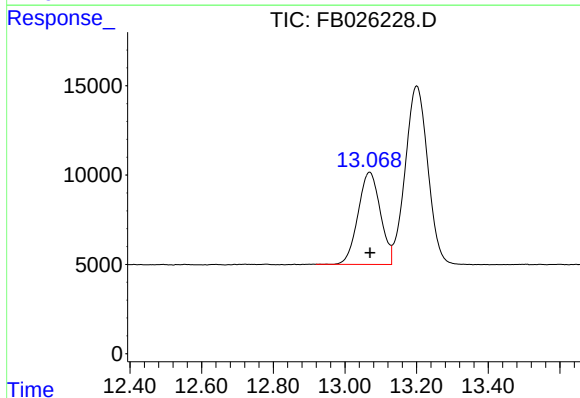


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 222836
Conc: 9.77 ng/ml

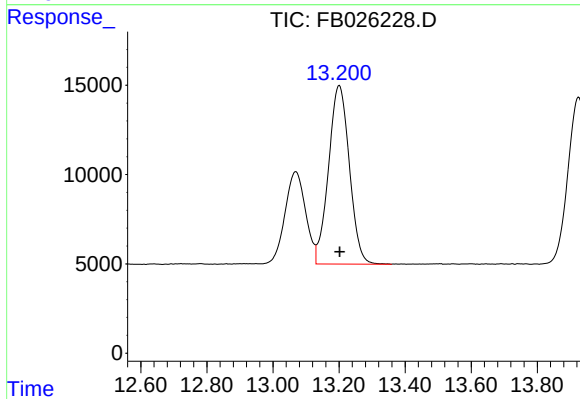

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.001 min
Response: 437805
Conc: 19.53 ng/ml

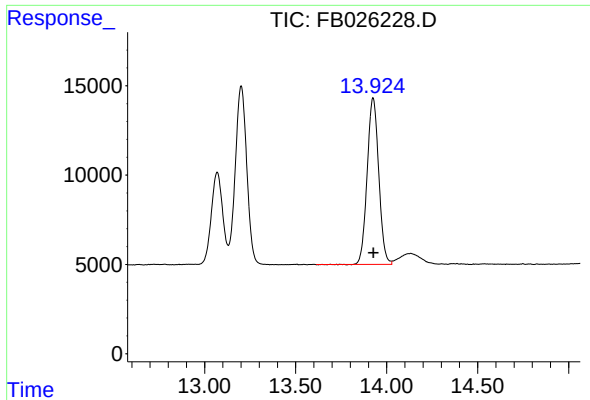

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.000 min
Response: 411927
Conc: 19.40 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0916S1

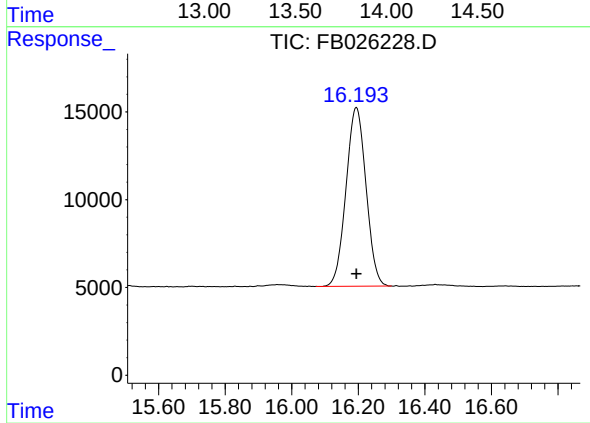

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 425059
Conc: 18.85 ng/ml