

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091621\
 Data File : FB026231.D
 Signal(s) : FID2B.CH
 Acq On : 16 Sep 2021 17:11
 Operator : AJ/MA
 Sample : M3757-01MS
 Misc : 5.01G/5.00ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-06-091521MS

Integration File: Calibration.e
 Quant Time: Sep 17 01:09:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
 Quant Title :
 QLast Update : Thu Sep 16 16:24:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.844	48784	2.864 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.846	104126	4.687 ng/ml
2) t 2,2,4-Trimethylpentane	7.497	93064	4.187 ng/ml
3) t n-Heptane	7.817	26835	1.039 ng/ml
4) t Benzene	7.958	25405	0.933 ng/ml
6) t Toluene	10.654	73808	2.816 ng/ml
7) t Ethylbenzene	13.074	24301	1.066 ng/ml
8) t m-Xylene	13.204	46208	2.061 ng/ml
9) t O-Xylene	13.929	37000	1.742 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	29764	1.320 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091621\
Data File : FB026231.D
Signal(s) : FID2B.CH
Acq On : 16 Sep 2021 17:11
Operator : AJ/MA
Sample : M3757-01MS
Misc : 5.01G/5.00ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-091521MS

Integration File: Calibration.e
Quant Time: Sep 17 01:09:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
Quant Title :
QLast Update : Thu Sep 16 16:24:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

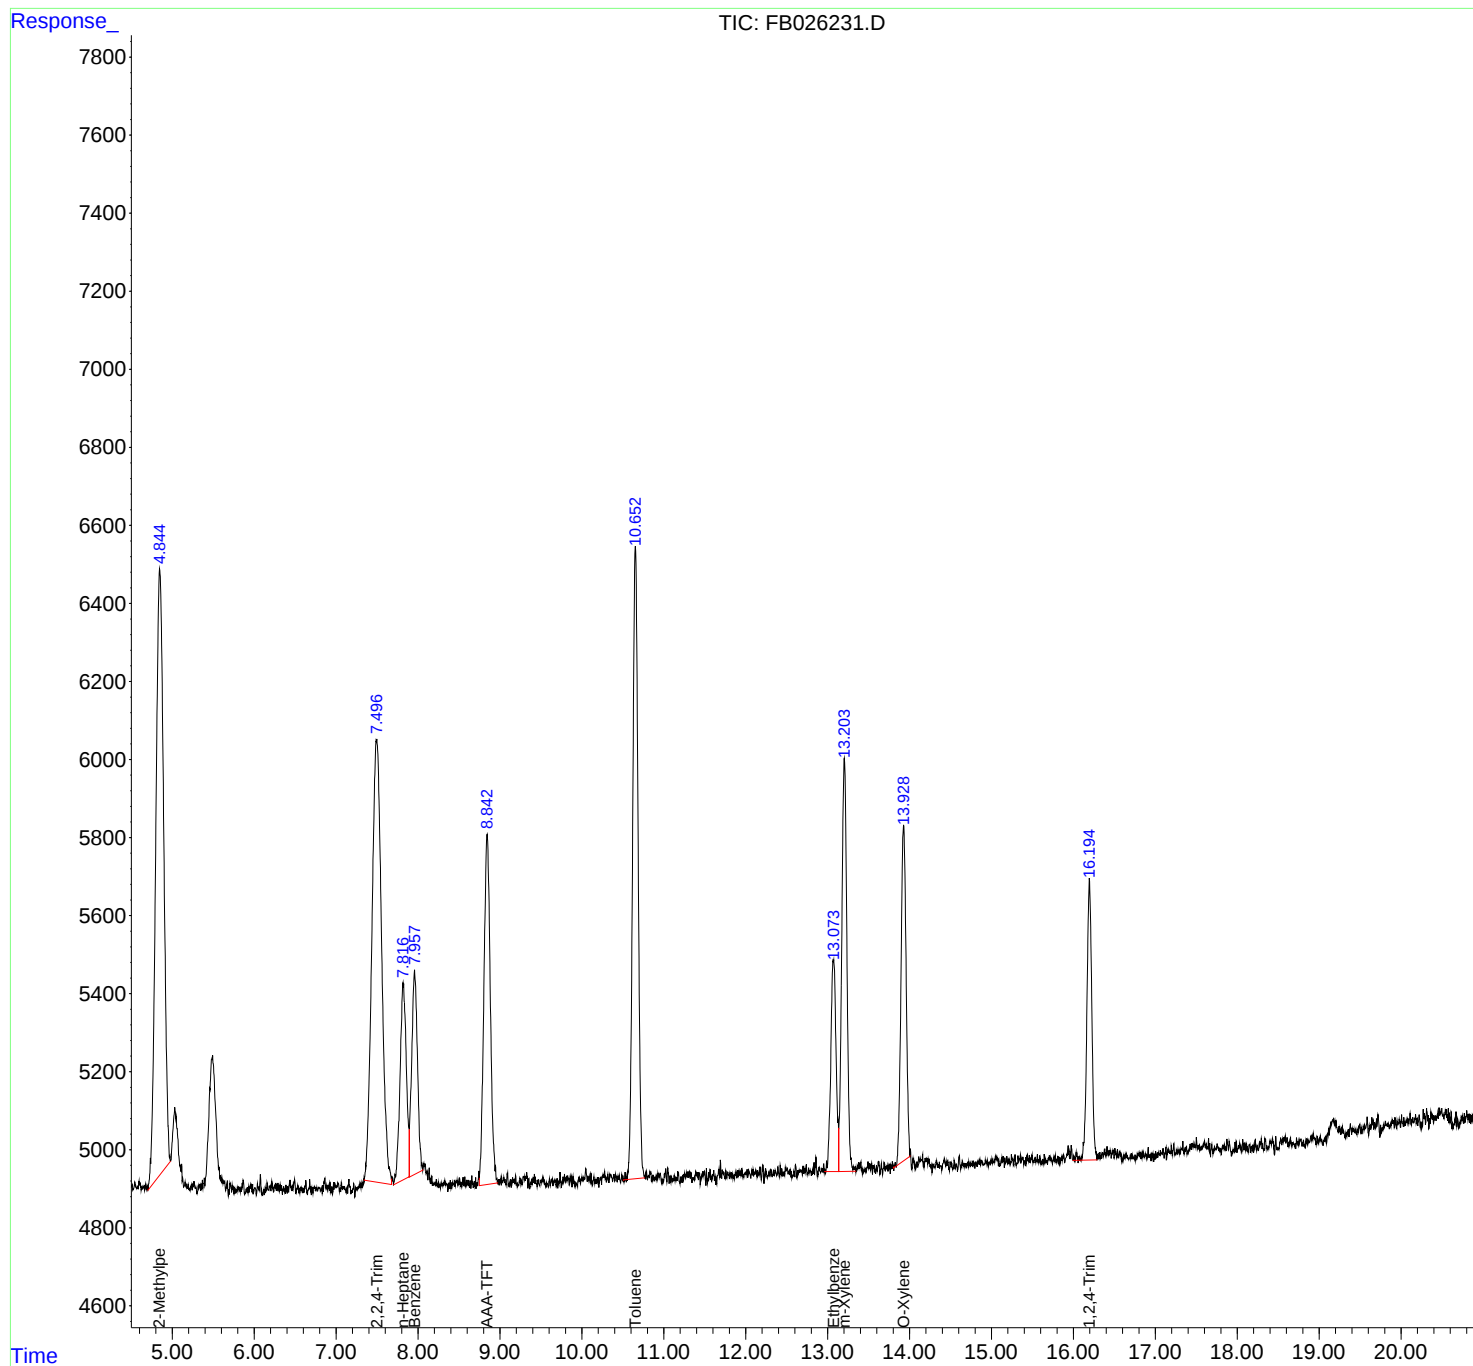


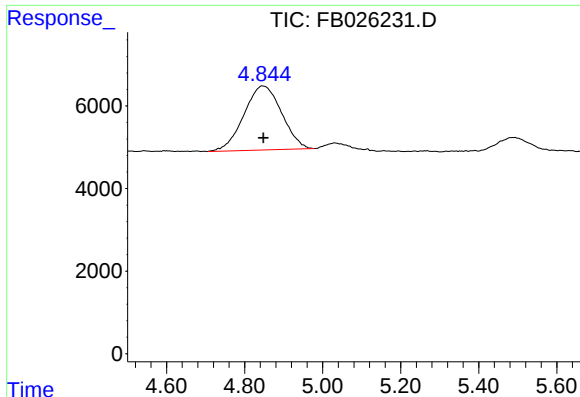

#1 2-Methylpentane


R.T.: 4.846 min
Delta R.T.: -0.002 min
Response: 104126
Conc: 4.69 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-091521MS

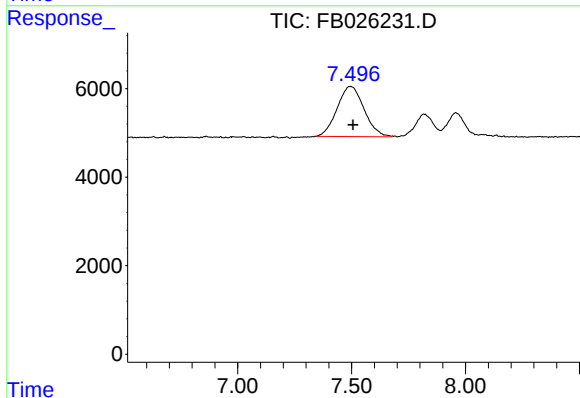


#2 2,2,4-Trimethylpentane

R.T.: 7.497 min
Delta R.T.: -0.009 min
Response: 93064
Conc: 4.19 ng/ml

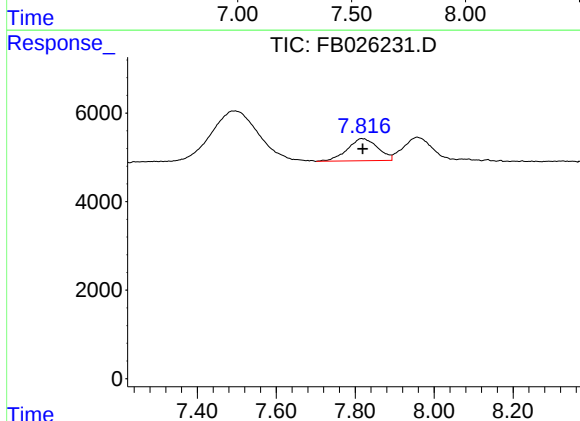


#3 n-Heptane

R.T.: 7.817 min
Delta R.T.: -0.002 min
Response: 26835
Conc: 1.04 ng/ml

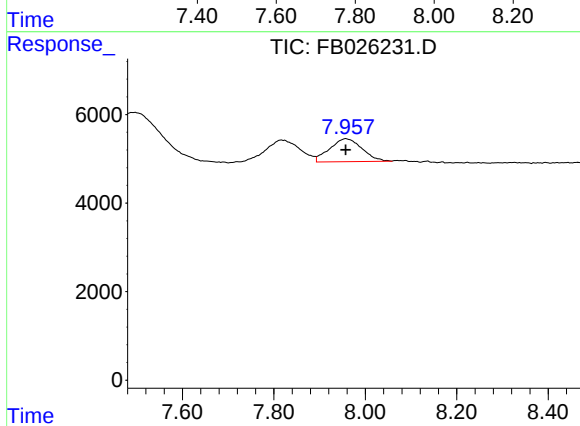

#4 Benzene


R.T.: 7.958 min
Delta R.T.: 0.000 min
Response: 25405
Conc: 0.93 ng/ml

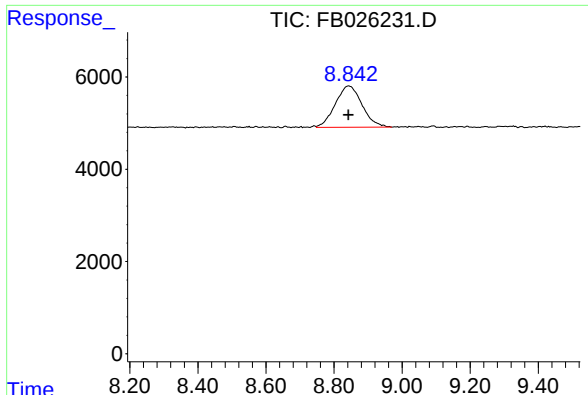

#5 AAA-TFT


R.T.: 8.844 min
Delta R.T.: 0.002 min
Response: 48784
Conc: 2.86 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-091521MS

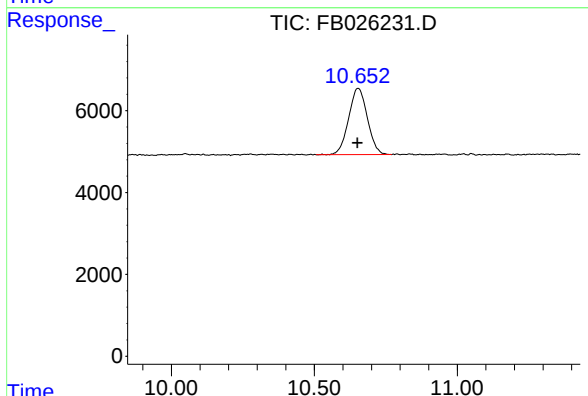


#6 Toluene

R.T.: 10.654 min
Delta R.T.: 0.002 min
Response: 73808
Conc: 2.82 ng/ml

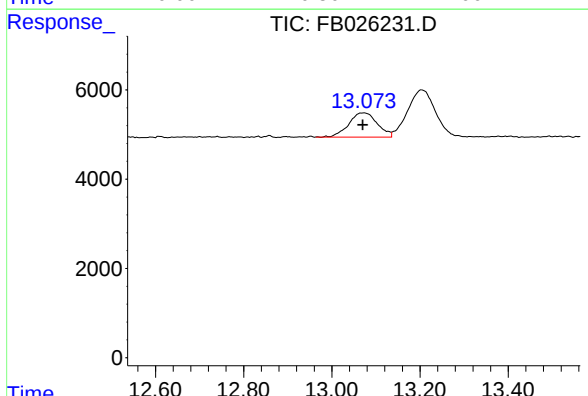


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: 0.004 min
Response: 24301
Conc: 1.07 ng/ml

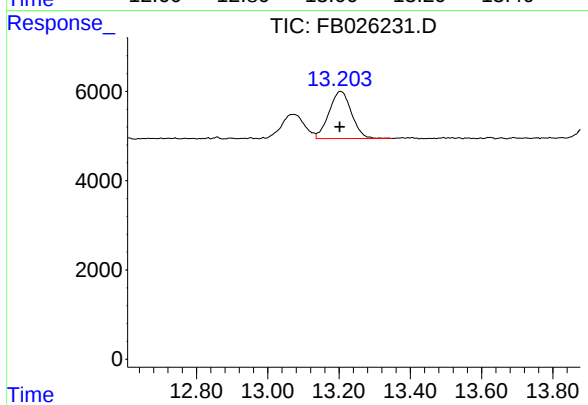

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.002 min
Response: 46208
Conc: 2.06 ng/ml

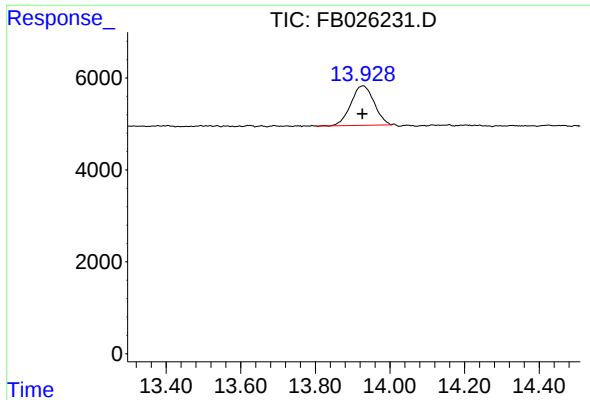

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.003 min
Response: 37000
Conc: 1.74 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-091521MS

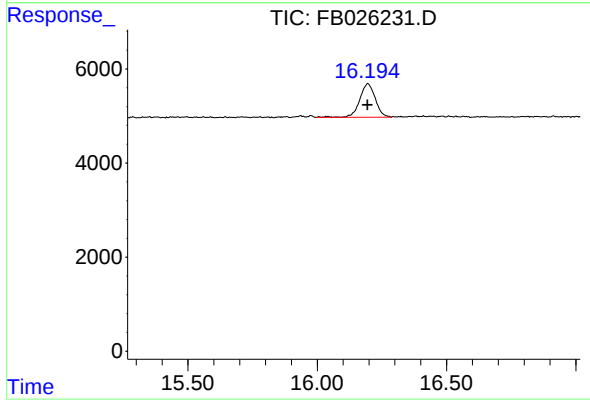

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.002 min
Response: 29764
Conc: 1.32 ng/ml