

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091819\
 Data File : FB022560.D
 Signal(s) : FID2B.CH
 Acq On : 18 Sep 2019 11:26
 Operator : DD/AJ
 Sample : BSF0918S1
 Misc : 5.00g/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 19 00:50:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.965	537878	18.492 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.831	1040595	21.179 ng/ml
2) t	2,2,4-Trimethylpentane	7.583	1180080	22.853 ng/ml
3) t	n-Heptane	7.922	386681	7.683 ng/ml
4) t	Benzene	8.058	468819	7.899 ng/ml
6) t	Toluene	10.806	1381828	29.046 ng/ml
7) t	Ethylbenzene	13.253	439824	14.671 ng/ml
8) t	m-Xylene	13.386	866768	32.627 ng/ml
9) t	O-Xylene	14.115	814102	33.557 ng/ml
10) t	1,2,4-Trimethylbenzene	16.395	570355	21.877 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091819\
Data File : FB022560.D
Signal(s) : FID2B.CH
Acq On : 18 Sep 2019 11:26
Operator : DD/AJ
Sample : BSF0918S1
Misc : 5.00g/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 19 00:50:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

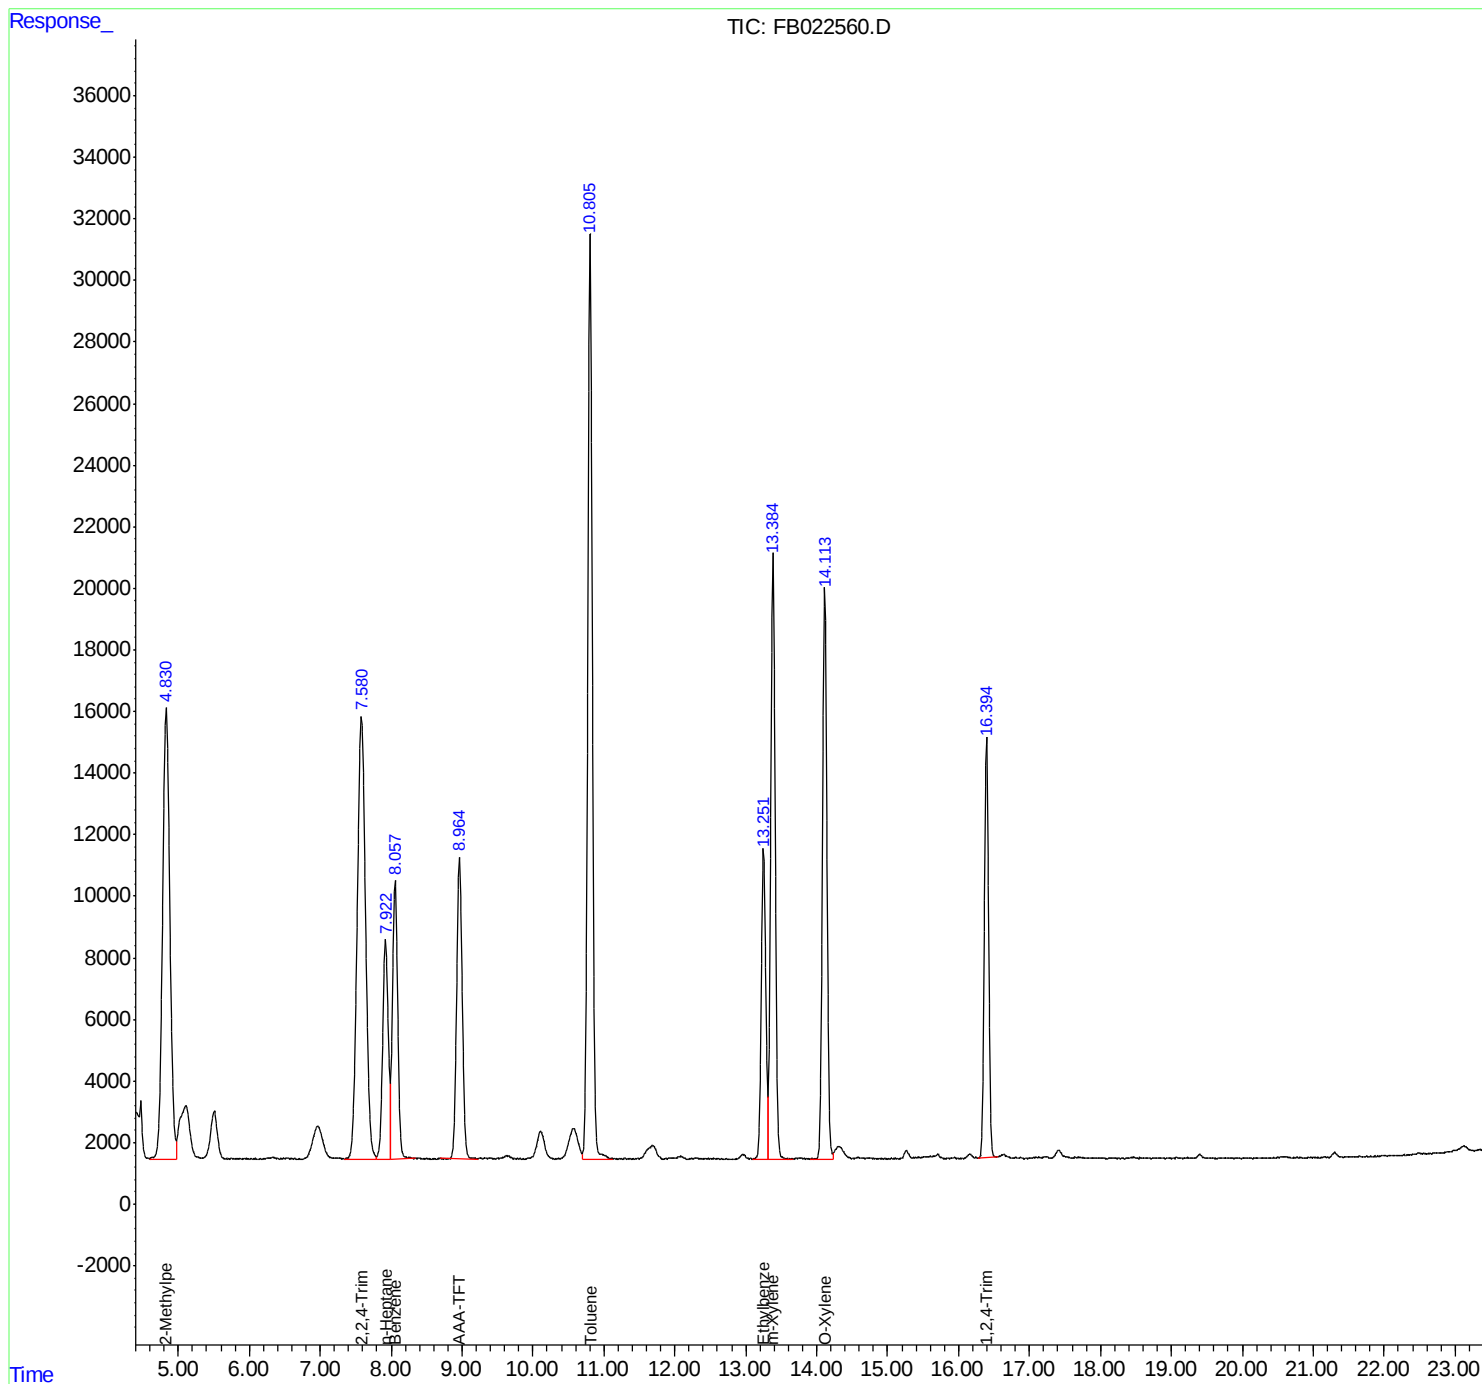

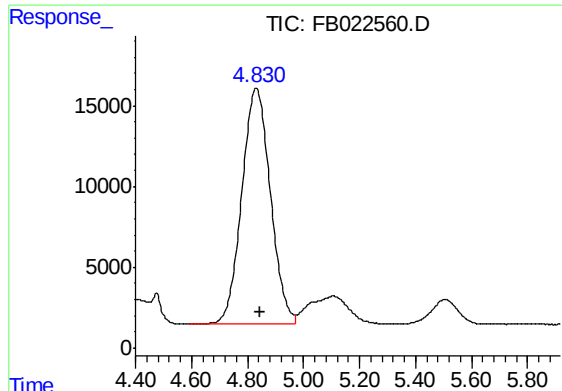


#1 2-Methylpentane

R.T.: 4.831 min
Delta R.T.: -0.016 min
Response: 1040595
Conc: 21.18 ng/ml

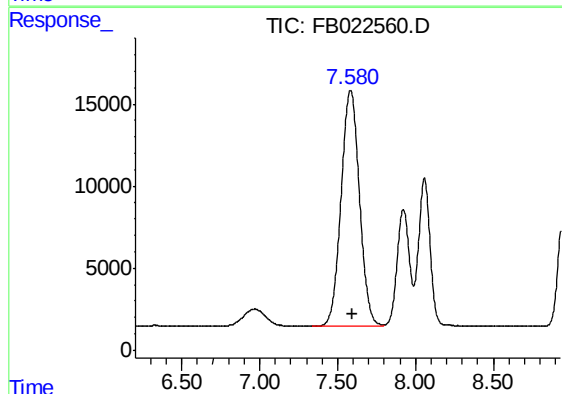


#2 2,2,4-Trimethylpentane

R.T.: 7.583 min
Delta R.T.: -0.015 min
Response: 1180080
Conc: 22.85 ng/ml

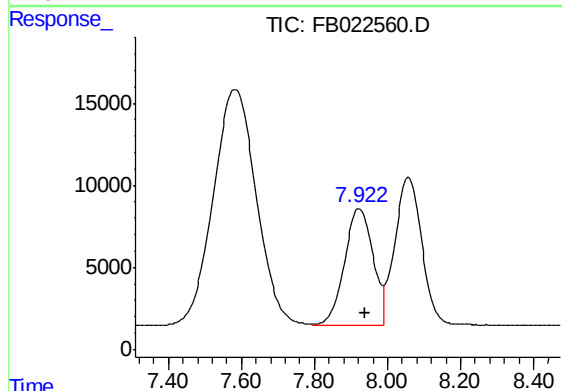


#3 n-Heptane

R.T.: 7.922 min
Delta R.T.: -0.015 min
Response: 386681
Conc: 7.68 ng/ml

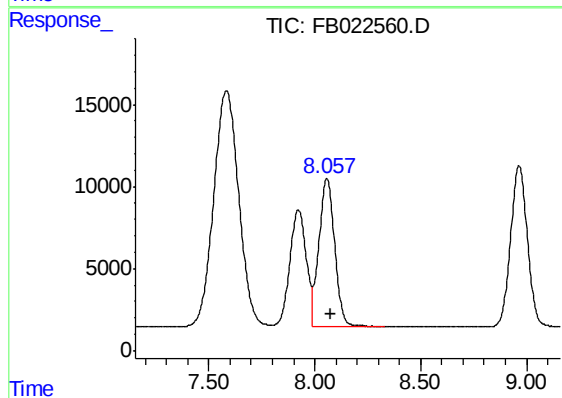


#4 Benzene

R.T.: 8.058 min
Delta R.T.: -0.015 min
Response: 468819
Conc: 7.90 ng/ml

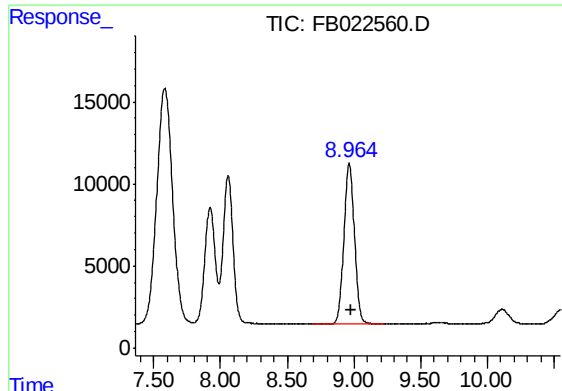


#5 AAA-TFT

R.T.: 8.965 min
Delta R.T.: -0.014 min
Response: 537878
Conc: 18.49 ng/ml

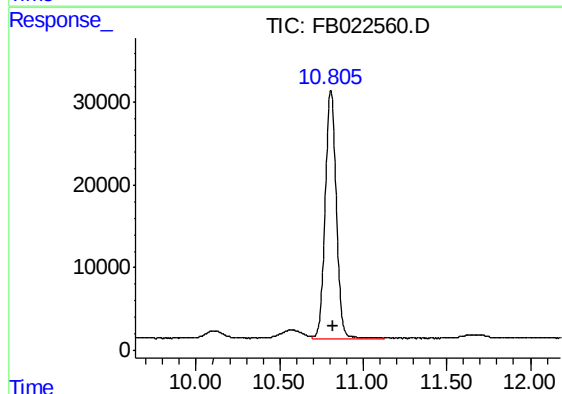


#6 Toluene

R.T.: 10.806 min
Delta R.T.: -0.013 min
Response: 1381828
Conc: 29.05 ng/ml

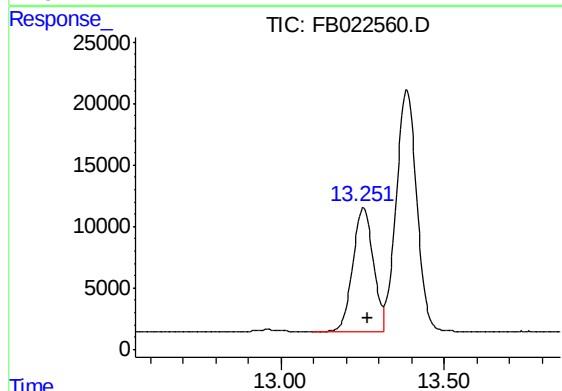


#7 Ethylbenzene

R.T.: 13.253 min
Delta R.T.: -0.012 min
Response: 439824
Conc: 14.67 ng/ml

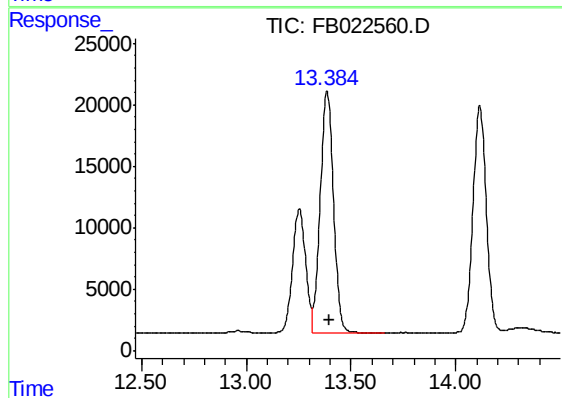


#8 m-Xylene

R.T.: 13.386 min
Delta R.T.: -0.012 min
Response: 866768
Conc: 32.63 ng/ml

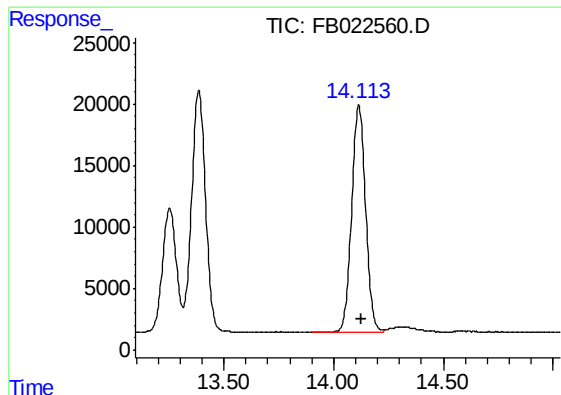

#9 O-Xylene

R.T.: 14.115 min
Delta R.T.: -0.013 min
Response: 814102
Conc: 33.56 ng/ml

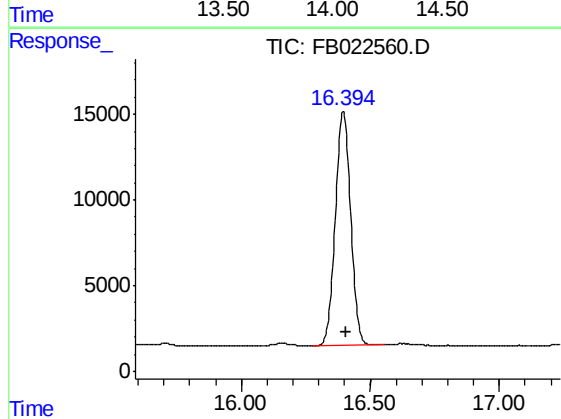

#10 1,2,4-Trimethylbenzene

R.T.: 16.395 min
Delta R.T.: -0.012 min
Response: 570355
Conc: 21.88 ng/ml