

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091919\
 Data File : FB022577.D
 Signal(s) : FID2B.CH
 Acq On : 19 Sep 2019 14:01
 Operator : DD/AJ
 Sample : BSF0919S1
 Misc : 5.00g/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 20 00:58:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.963	526611	18.104 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.832	964713	19.635 ng/ml
2) t 2,2,4-Trimethylpentane	7.582	1106078	21.420 ng/ml
3) t n-Heptane	7.921	364469	7.242 ng/ml
4) t Benzene	8.056	451521	7.608 ng/ml
6) t Toluene	10.804	1357009	28.525 ng/ml
7) t Ethylbenzene	13.251	438613	14.631 ng/ml
8) t m-Xylene	13.383	868130	32.678 ng/ml
9) t O-Xylene	14.113	816455	33.654 ng/ml
10) t 1,2,4-Trimethylbenzene	16.393	559962	21.478 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091919\
Data File : FB022577.D
Signal(s) : FID2B.CH
Acq On : 19 Sep 2019 14:01
Operator : DD/AJ
Sample : BSF0919S1
Misc : 5.00g/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 20 00:58:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

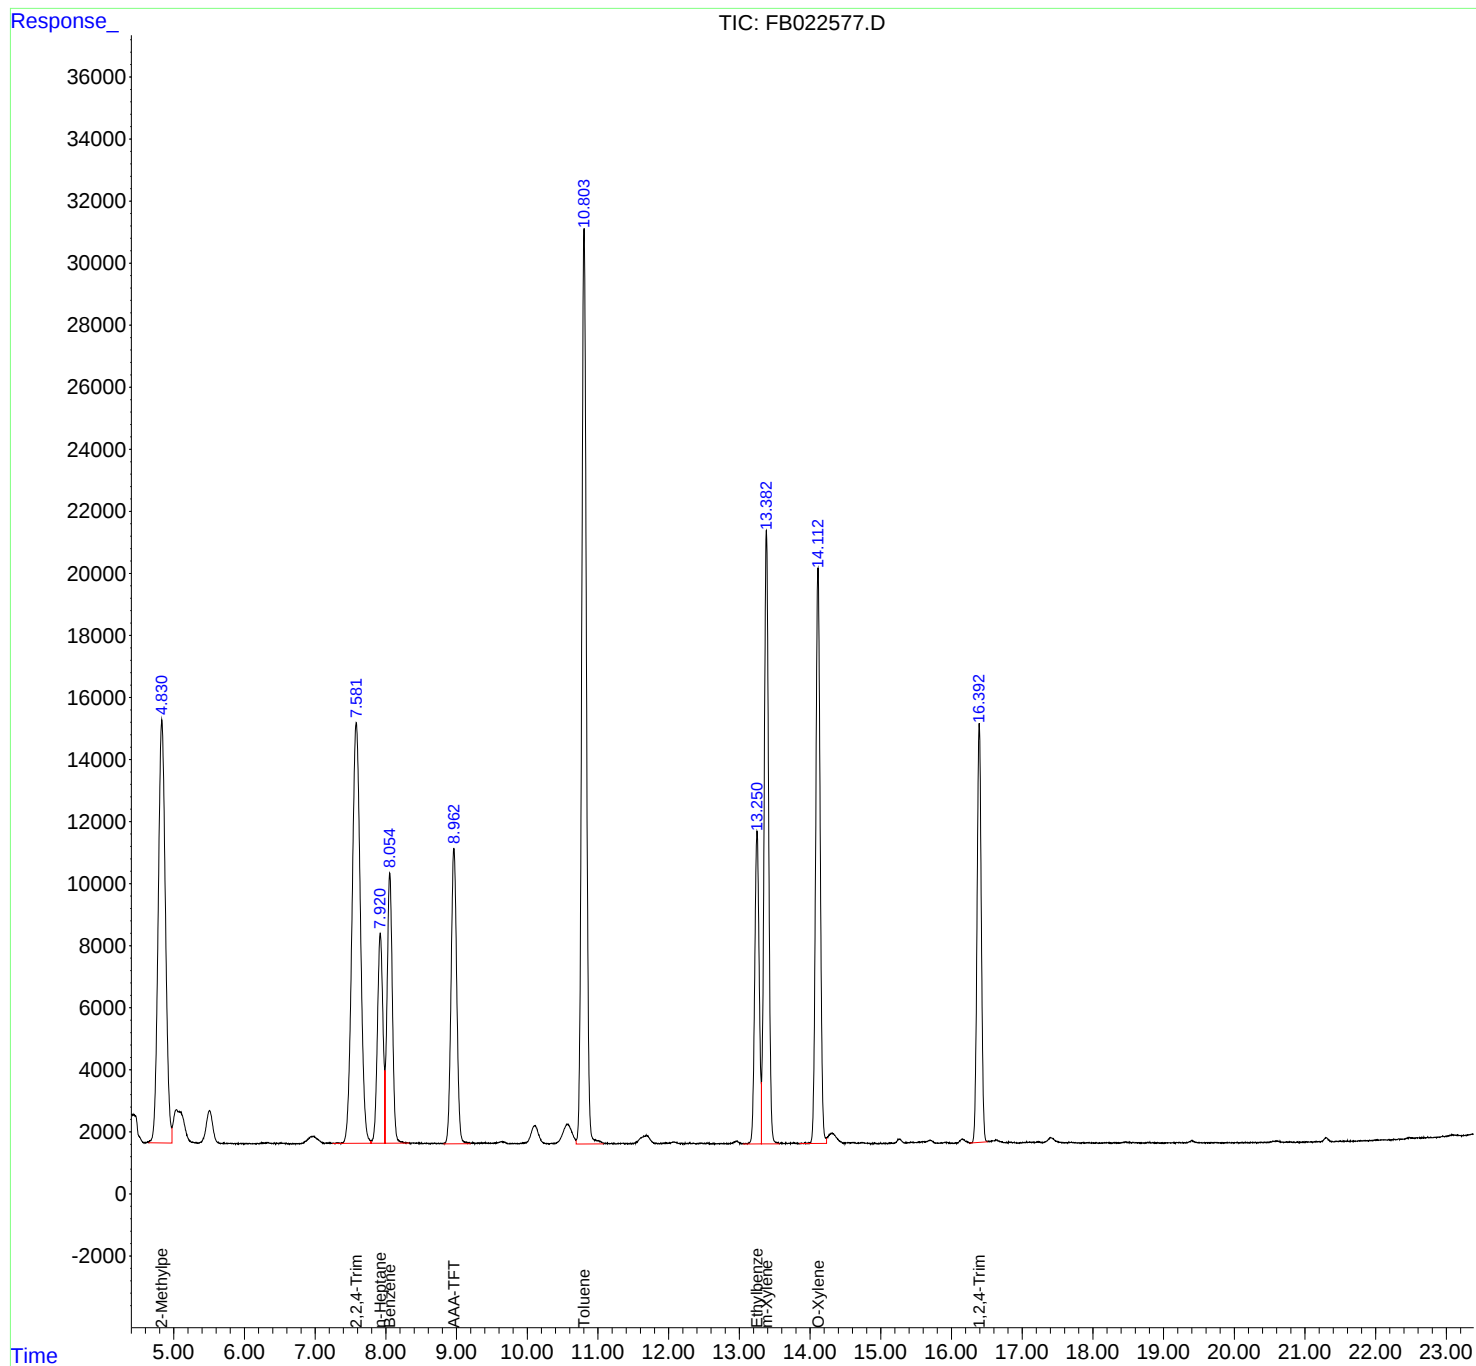

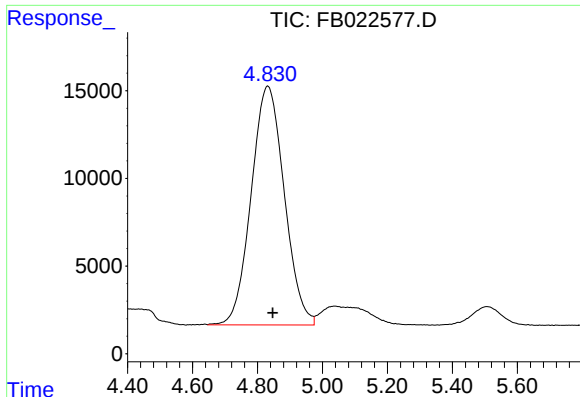


#1 2-Methylpentane

R.T.: 4.832 min
Delta R.T.: -0.015 min
Response: 964713
Conc: 19.63 ng/ml

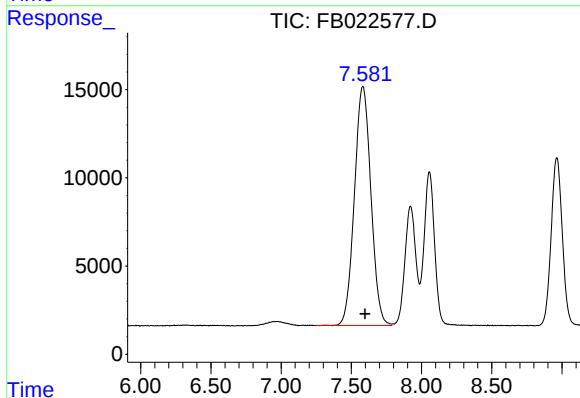


#2 2,2,4-Trimethylpentane

R.T.: 7.582 min
Delta R.T.: -0.016 min
Response: 1106078
Conc: 21.42 ng/ml

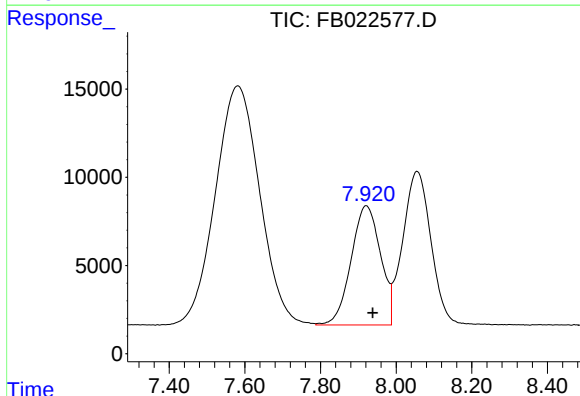


#3 n-Heptane

R.T.: 7.921 min
Delta R.T.: -0.016 min
Response: 364469
Conc: 7.24 ng/ml

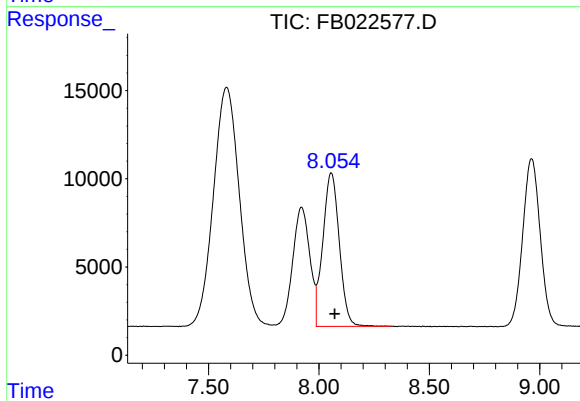


#4 Benzene

R.T.: 8.056 min
Delta R.T.: -0.016 min
Response: 451521
Conc: 7.61 ng/ml

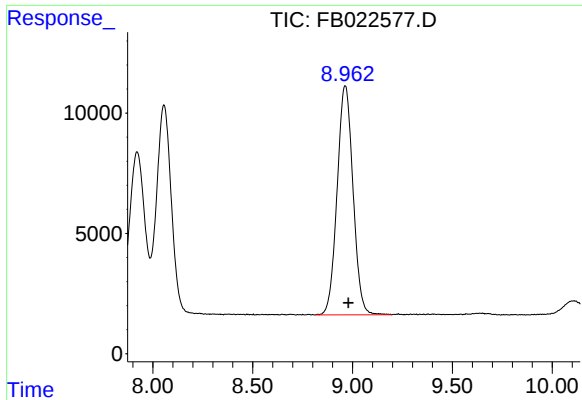


#5 AAA-TFT

R.T.: 8.963 min
Delta R.T.: -0.016 min
Response: 526611
Conc: 18.10 ng/ml

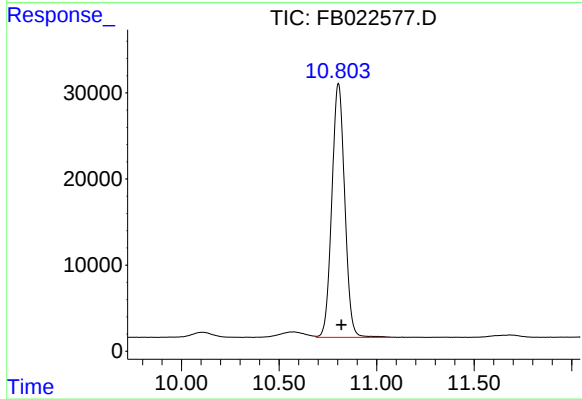


#6 Toluene

R.T.: 10.804 min
Delta R.T.: -0.015 min
Response: 1357009
Conc: 28.52 ng/ml

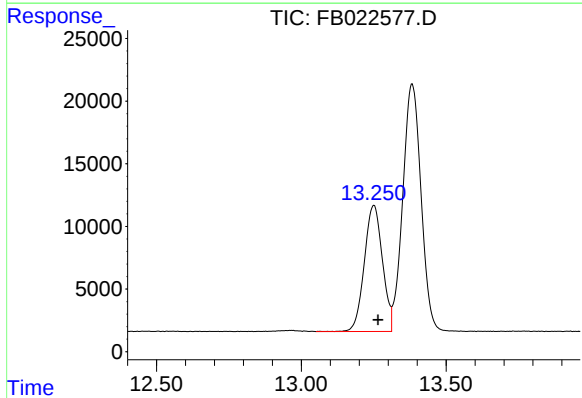


#7 Ethylbenzene

R.T.: 13.251 min
Delta R.T.: -0.014 min
Response: 438613
Conc: 14.63 ng/ml

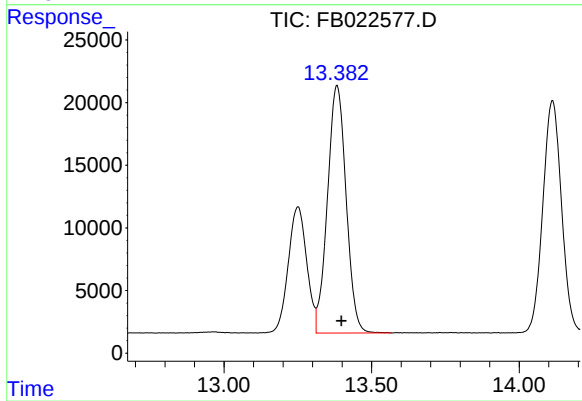


#8 m-Xylene

R.T.: 13.383 min
Delta R.T.: -0.015 min
Response: 868130
Conc: 32.68 ng/ml

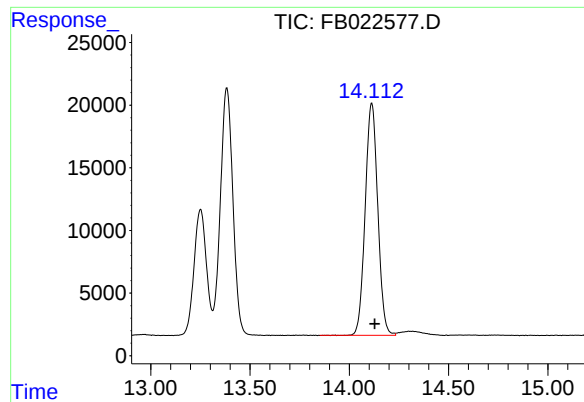

#9 O-Xylene

R.T.: 14.113 min
Delta R.T.: -0.015 min
Response: 816455
Conc: 33.65 ng/ml

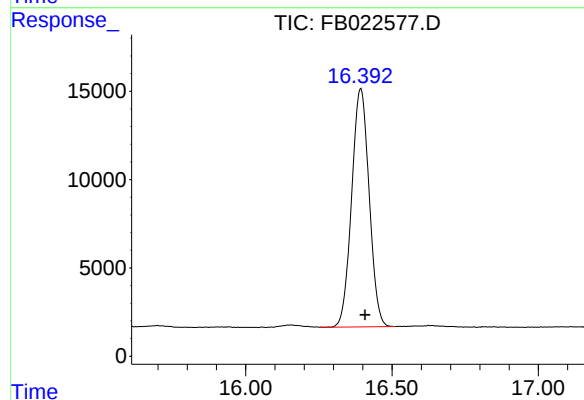

#10 1,2,4-Trimethylbenzene

R.T.: 16.393 min
Delta R.T.: -0.014 min
Response: 559962
Conc: 21.48 ng/ml