

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091919\
 Data File : FB022580.D
 Signal(s) : FID2B.CH
 Acq On : 19 Sep 2019 15:41
 Operator : DD/AJ
 Sample : K4662-10MS
 Misc : 5.01g/5.00ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 20 00:59:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.963	634622	21.818 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.830	864035	17.586 ng/ml
2) t 2,2,4-Trimethylpentane	7.582	907026	17.565 ng/ml
3) t n-Heptane	7.921	297313	5.907 ng/ml
4) t Benzene	8.056	455303	7.672 ng/ml
6) t Toluene	10.805	1346041	28.294 ng/ml
7) t Ethylbenzene	13.250	445207	14.851 ng/ml
8) t m-Xylene	13.384	892500	33.595 ng/ml
9) t O-Xylene	14.113	817753	33.708 ng/ml
10) t 1,2,4-Trimethylbenzene	16.394	557720	21.392 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091919\
Data File : FB022580.D
Signal(s) : FID2B.CH
Acq On : 19 Sep 2019 15:41
Operator : DD/AJ
Sample : K4662-10MS
Misc : 5.01g/5.00ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 20 00:59:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

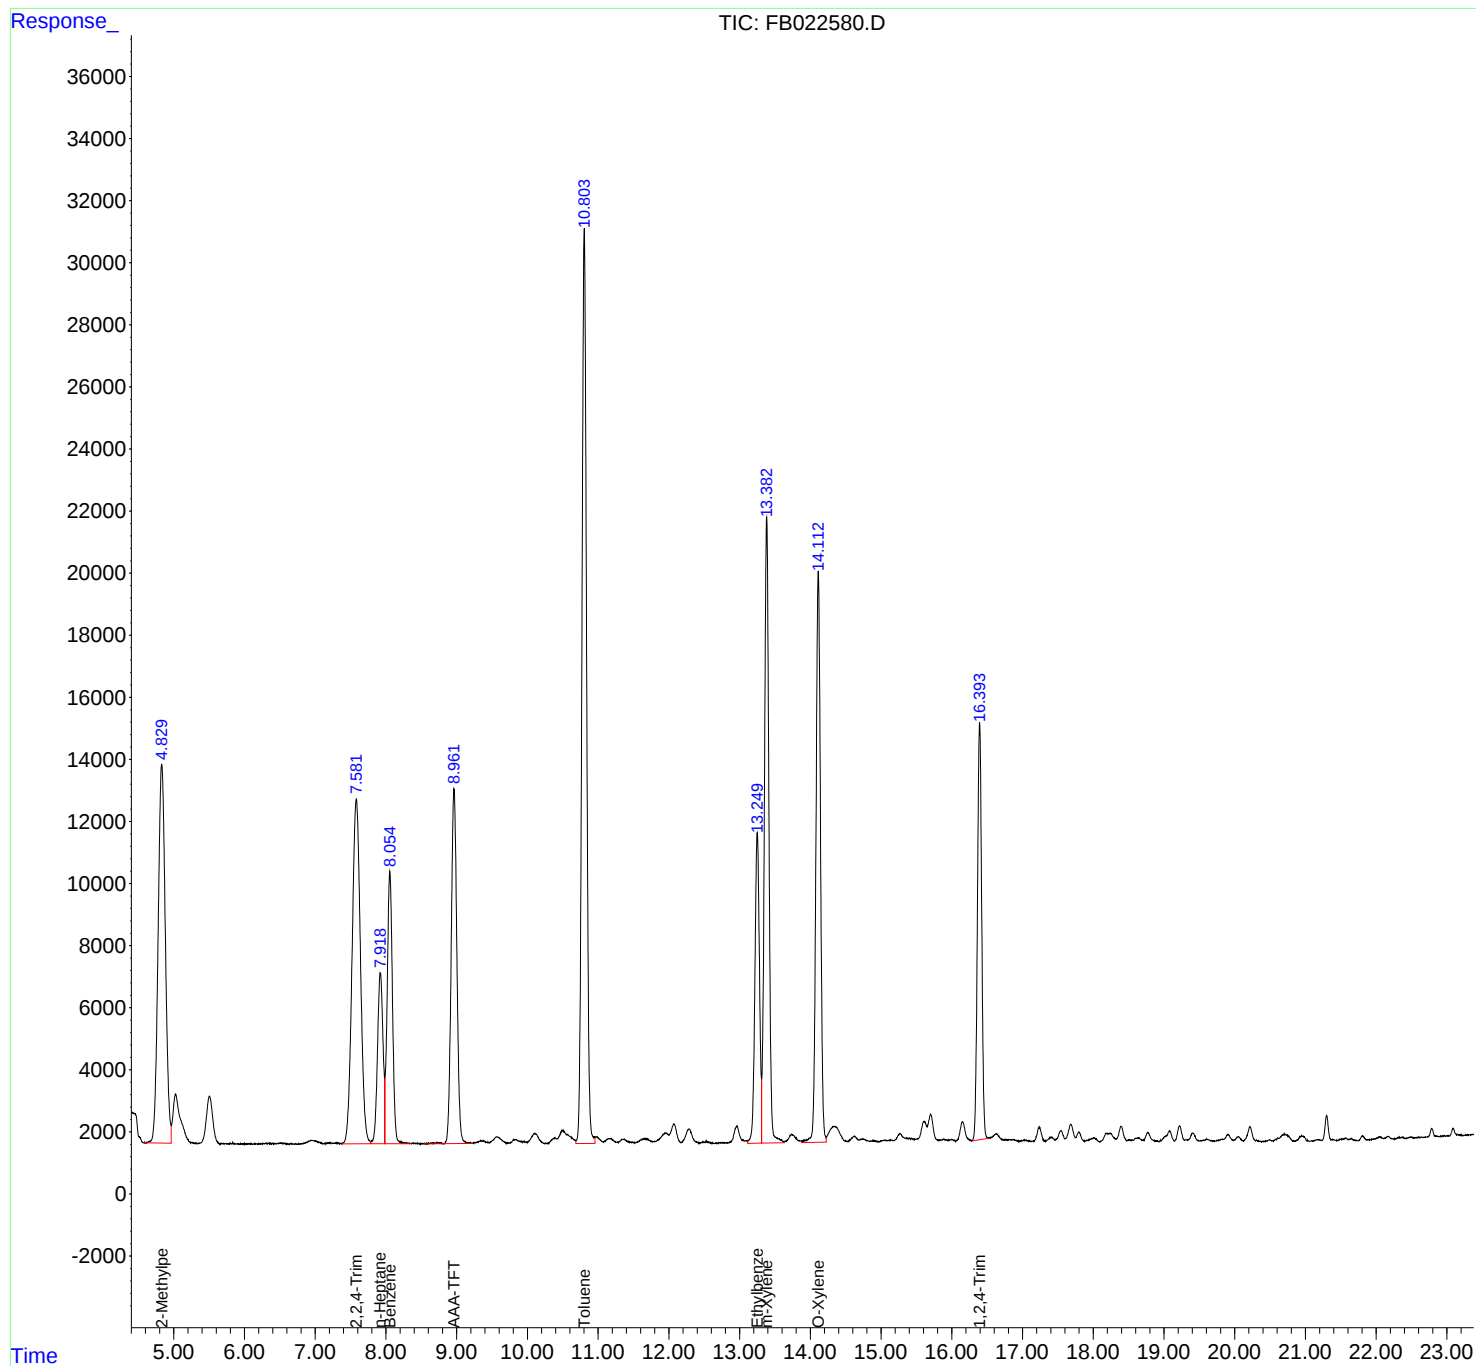

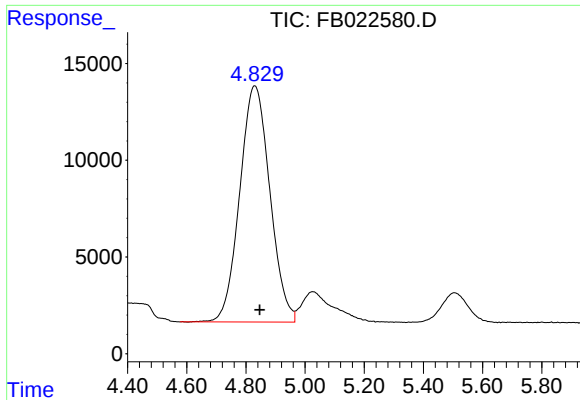


#1 2-Methylpentane

R.T.: 4.830 min
 Delta R.T.: -0.017 min
 Response: 864035
 Conc: 17.59 ng/ml

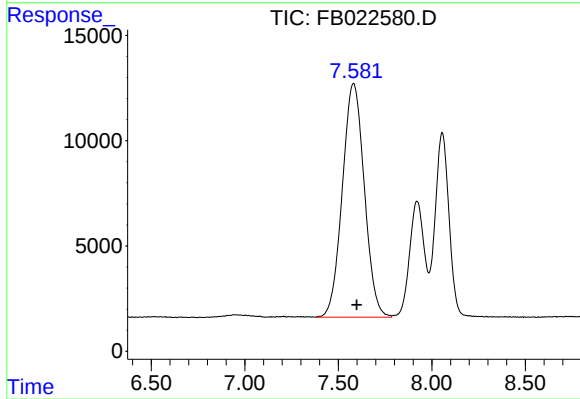


#2 2,2,4-Trimethylpentane

R.T.: 7.582 min
 Delta R.T.: -0.016 min
 Response: 907026
 Conc: 17.57 ng/ml

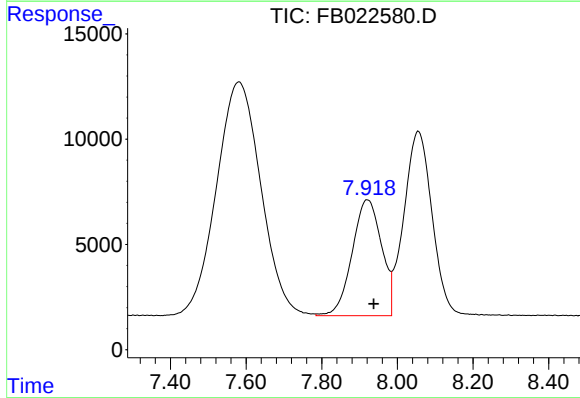


#3 n-Heptane

R.T.: 7.921 min
 Delta R.T.: -0.017 min
 Response: 297313
 Conc: 5.91 ng/ml

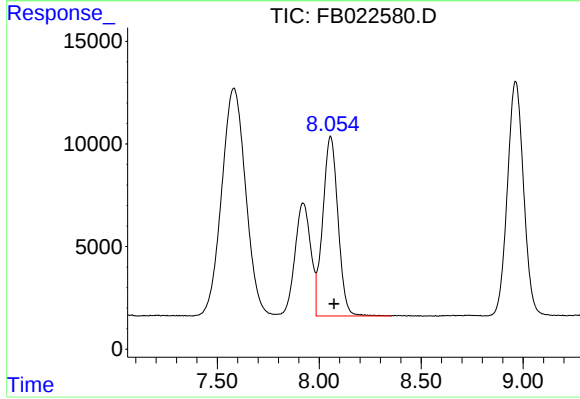


#4 Benzene

R.T.: 8.056 min
 Delta R.T.: -0.017 min
 Response: 455303
 Conc: 7.67 ng/ml

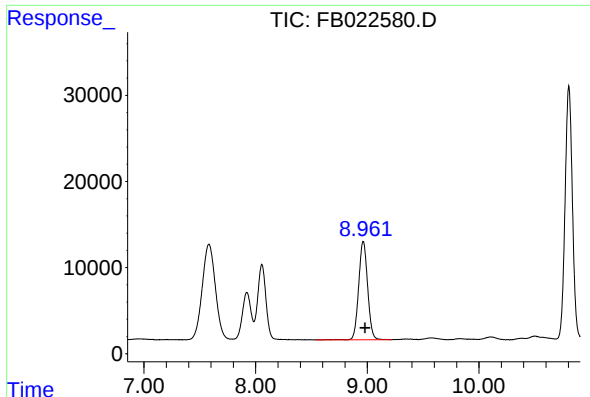


#5 AAA-TFT

R.T.: 8.963 min
Delta R.T.: -0.016 min
Response: 634622
Conc: 21.82 ng/ml

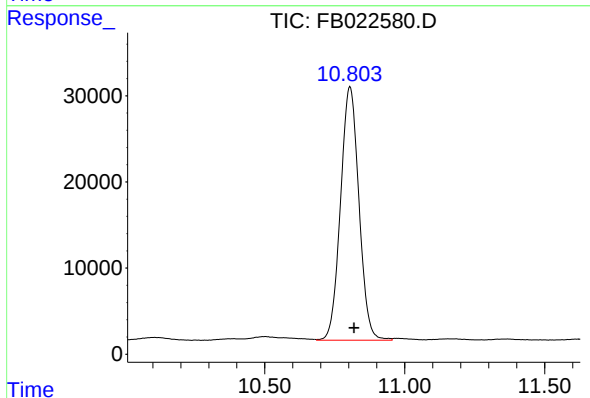


#6 Toluene

R.T.: 10.805 min
Delta R.T.: -0.015 min
Response: 1346041
Conc: 28.29 ng/ml

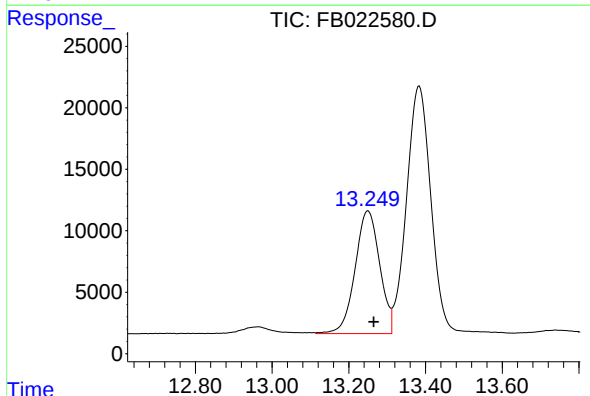


#7 Ethylbenzene

R.T.: 13.250 min
Delta R.T.: -0.015 min
Response: 445207
Conc: 14.85 ng/ml

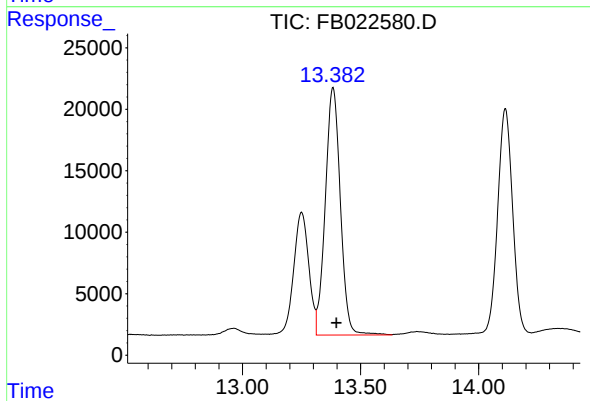


#8 m-Xylene

R.T.: 13.384 min
Delta R.T.: -0.014 min
Response: 892500
Conc: 33.60 ng/ml

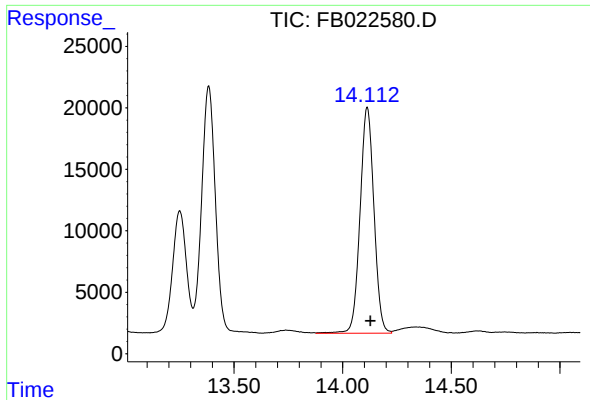

#9 O-Xylene

R.T.: 14.113 min
Delta R.T.: -0.015 min
Response: 817753
Conc: 33.71 ng/ml

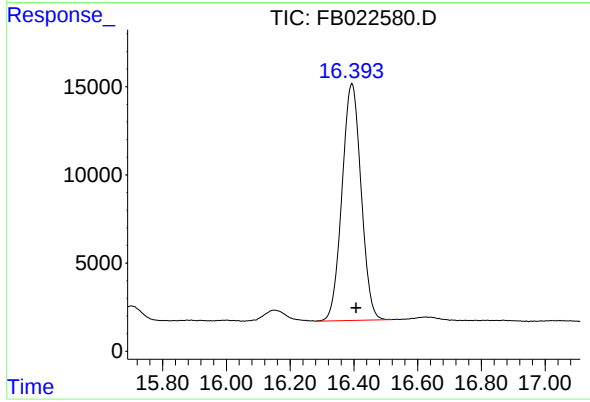

#10 1,2,4-Trimethylbenzene

R.T.: 16.394 min
Delta R.T.: -0.013 min
Response: 557720
Conc: 21.39 ng/ml