

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091924\
 Data File : FB030928.D
 Signal(s) : FID2B.CH
 Acq On : 19 Sep 2024 11:05
 Operator : YP/AJ
 Sample : BSF0919S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0919S1

Integration File: Calibration.e
 Quant Time: Sep 20 01:54:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
 Quant Title :
 QLast Update : Tue Aug 27 11:54:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	243379	20.116 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	536990	30.051 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	521543	28.445 ng/ml
3) t n-Heptane	7.747	188912	10.215 ng/ml
4) t Benzene	7.884	222059	9.829 ng/ml
6) t Toluene	10.616	643471	29.462 ng/ml
7) t Ethylbenzene	13.052	201041	9.604 ng/ml
8) t m-Xylene	13.184	398363	19.199 ng/ml
9) t O-Xylene	13.911	381614	18.935 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	369933	18.540 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091924\
Data File : FB030928.D
Signal(s) : FID2B.CH
Acq On : 19 Sep 2024 11:05
Operator : YP/AJ
Sample : BSF0919S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0919S1

Integration File: Calibration.e
Quant Time: Sep 20 01:54:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
Quant Title :
QLast Update : Tue Aug 27 11:54:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

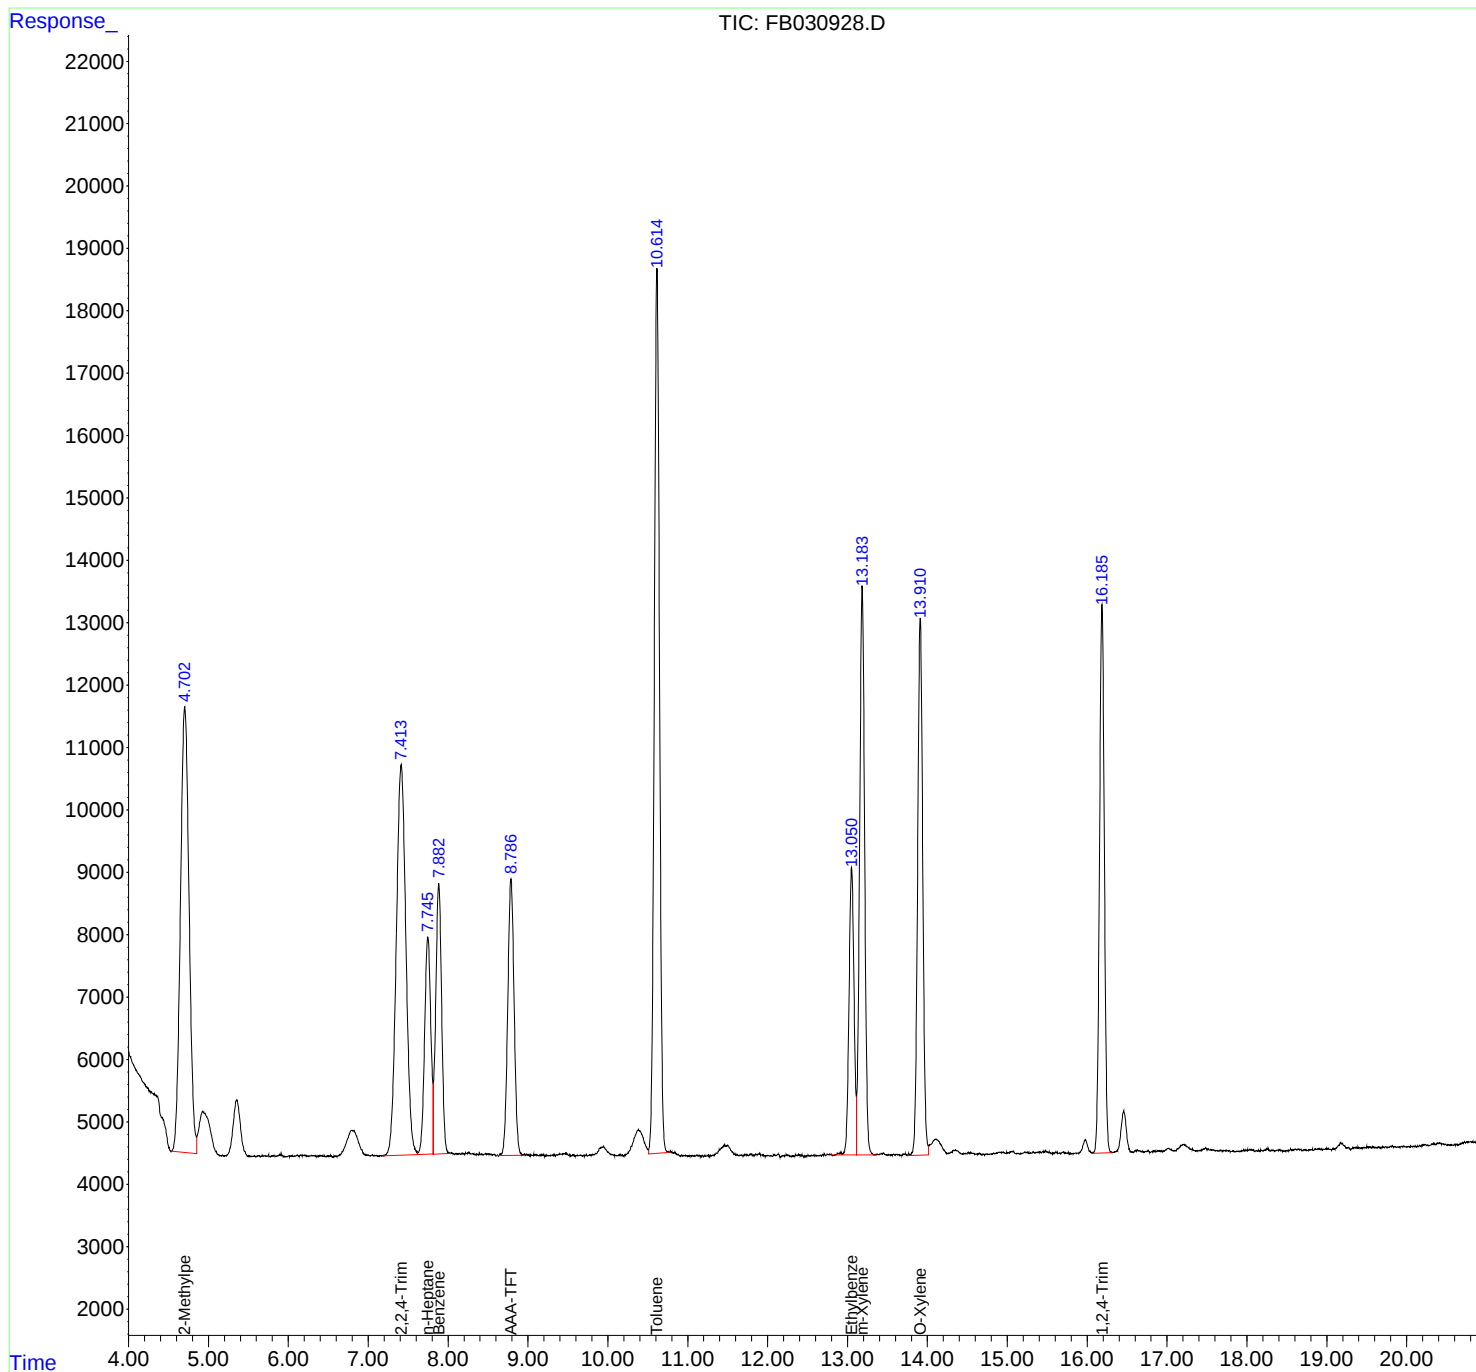


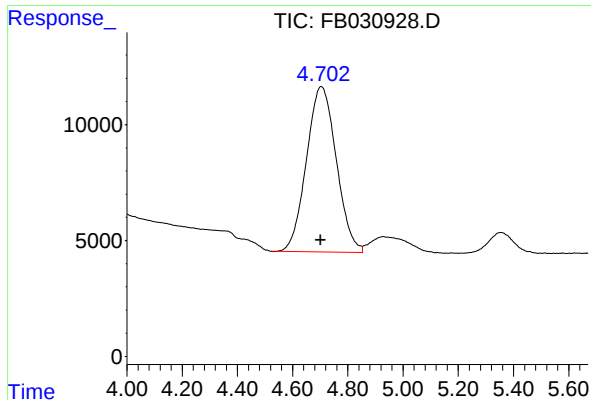

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: 0.002 min
Response: 536990
Conc: 30.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0919S1

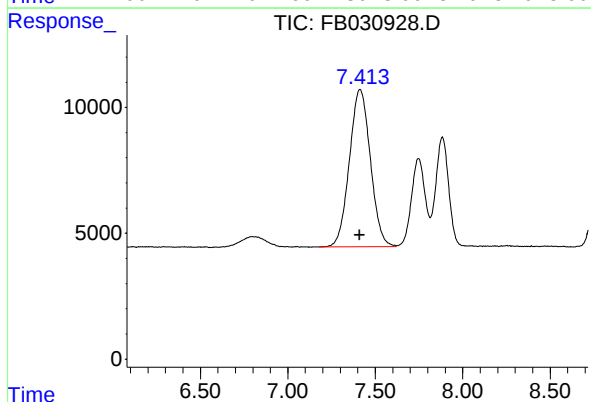


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: 0.003 min
Response: 521543
Conc: 28.45 ng/ml

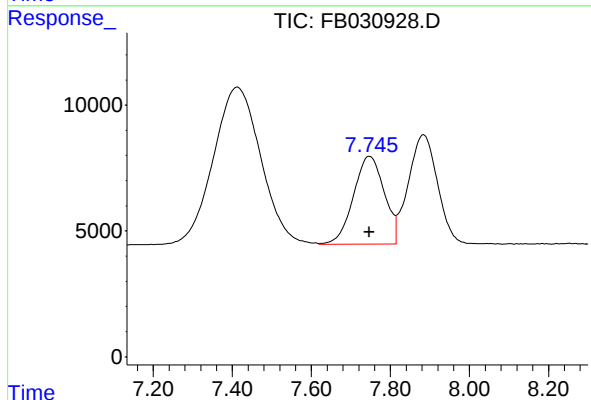


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 188912
Conc: 10.21 ng/ml

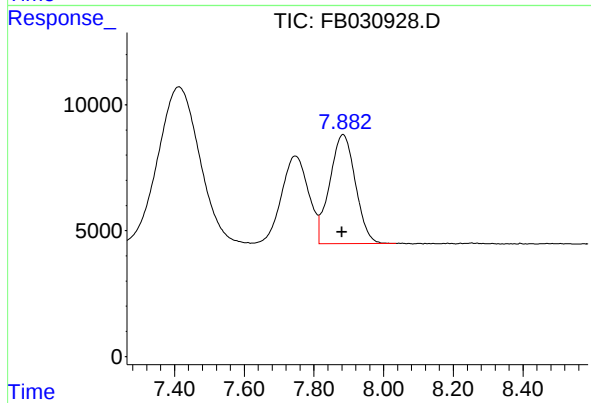

#4 Benzene


R.T.: 7.884 min
Delta R.T.: 0.003 min
Response: 222059
Conc: 9.83 ng/ml

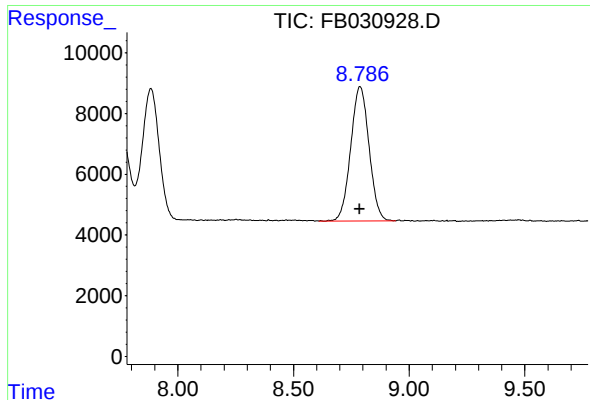

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.002 min
Response: 243379
Conc: 20.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0919S1

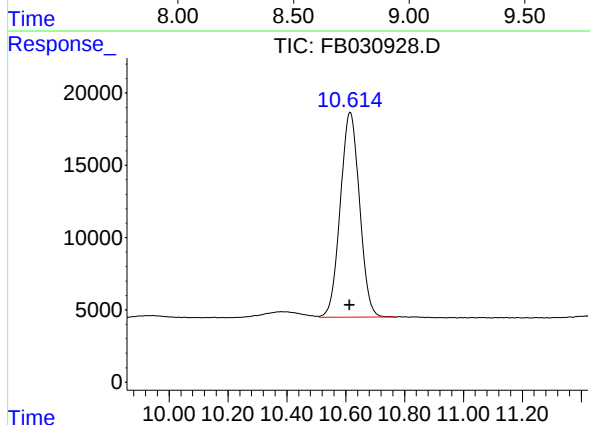


#6 Toluene

R.T.: 10.616 min
Delta R.T.: 0.001 min
Response: 643471
Conc: 29.46 ng/ml

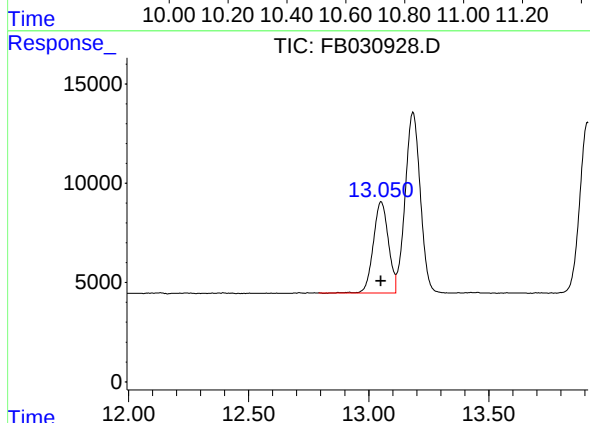


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: 0.002 min
Response: 201041
Conc: 9.60 ng/ml

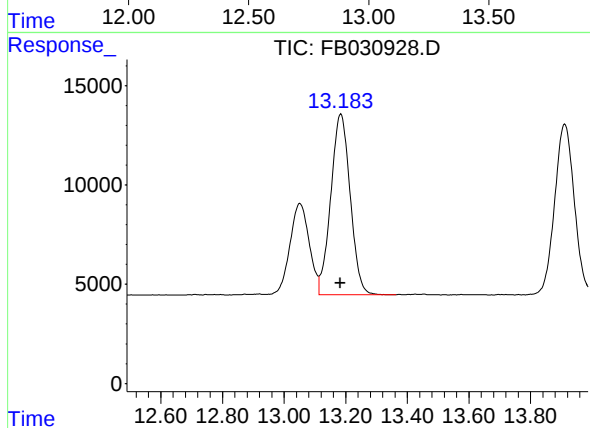

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: 0.002 min
Response: 398363
Conc: 19.20 ng/ml

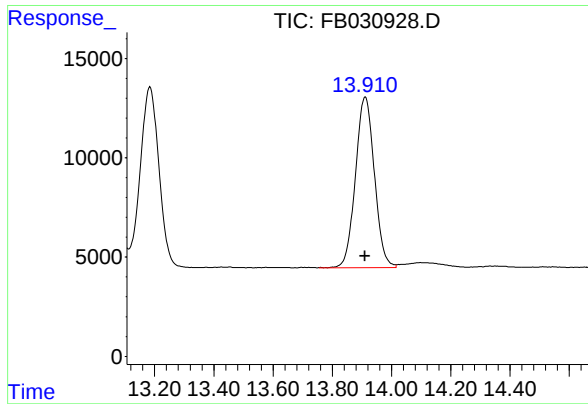

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: 0.002 min
Response: 381614
Conc: 18.93 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0919S1

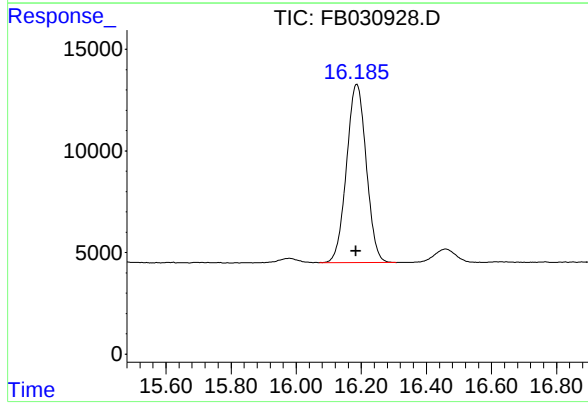

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: 0.002 min
Response: 369933
Conc: 18.54 ng/ml