

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091924\
 Data File : FB030938.D
 Signal(s) : FID2B.CH
 Acq On : 19 Sep 2024 19:28
 Operator : YP/AJ
 Sample : P4103-04
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC-14-5-7.5A

Integration File: Calibration.e
 Quant Time: Sep 20 01:55:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
 Quant Title :
 QLast Update : Tue Aug 27 11:54:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.779	1522	0.126 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.452	11880	0.648 ng/ml
3) t n-Heptane	7.783	23497	1.270 ng/ml
4) t Benzene	7.842	3261	0.144 ng/ml
7) t Ethylbenzene	13.057	113673	5.430 ng/ml
8) t m-Xylene	13.166	81895	3.947 ng/ml
9) t O-Xylene	13.874	103271	5.124 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	24474	1.227 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091924\
Data File : FB030938.D
Signal(s) : FID2B.CH
Acq On : 19 Sep 2024 19:28
Operator : YP/AJ
Sample : P4103-04
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WC-14-5-7.5A

Integration File: Calibration.e
Quant Time: Sep 20 01:55:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
Quant Title :
QLast Update : Tue Aug 27 11:54:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

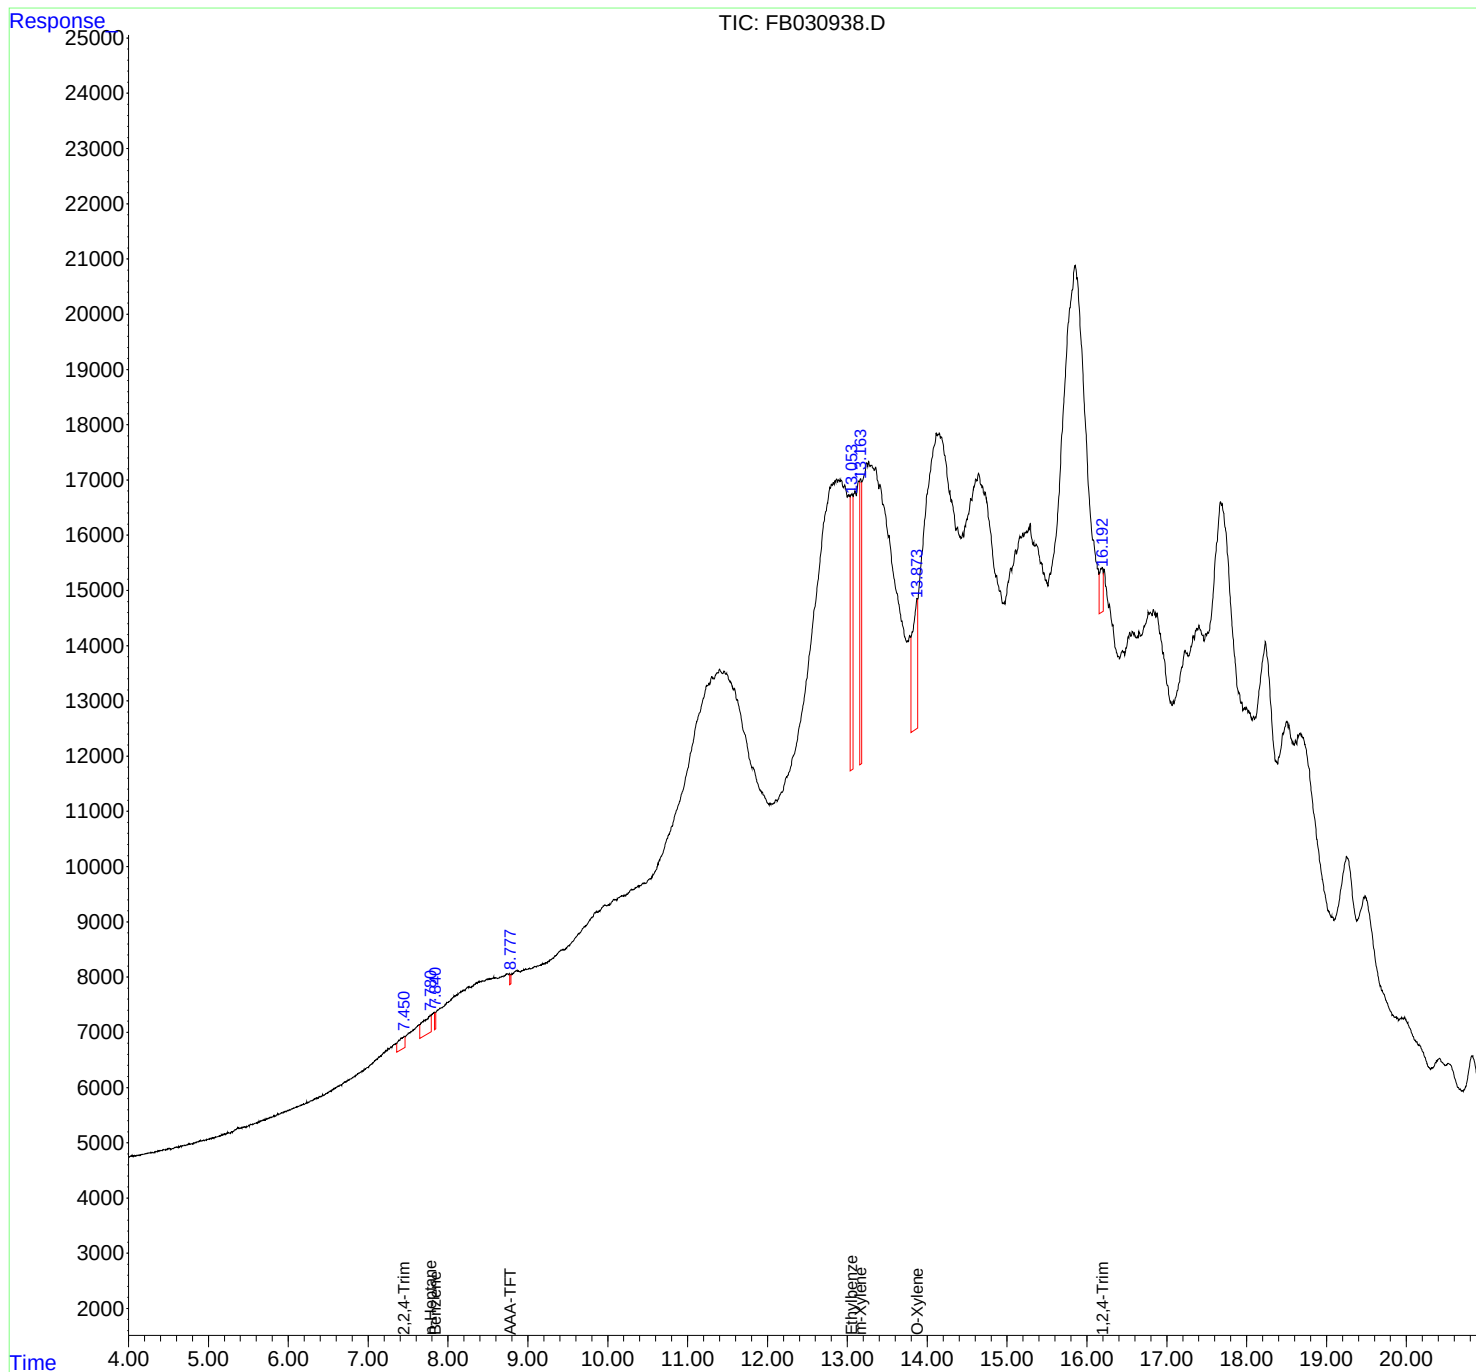


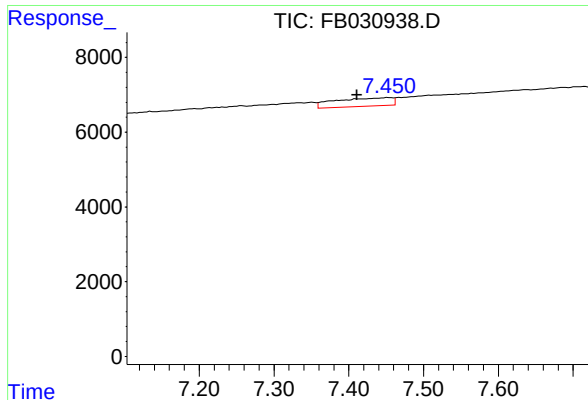

#2 2,2,4-Trimethylpentane


R.T.: 7.452 min
Delta R.T.: 0.041 min
Response: 11880
Conc: 0.65 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-14-5-7.5A

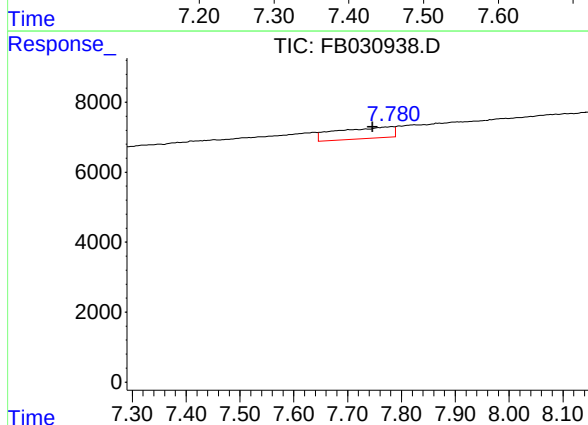


#3 n-Heptane

R.T.: 7.783 min
Delta R.T.: 0.037 min
Response: 23497
Conc: 1.27 ng/ml

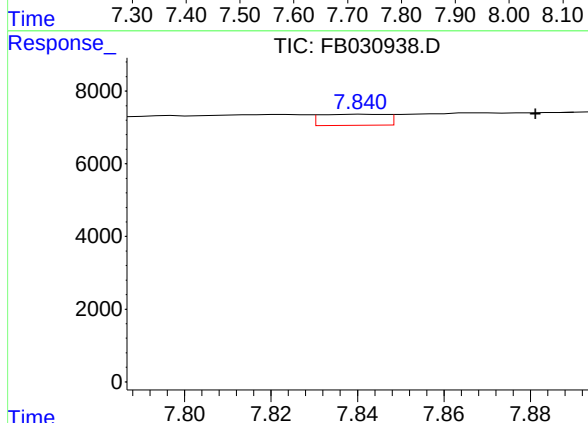


#4 Benzene

R.T.: 7.842 min
Delta R.T.: -0.039 min
Response: 3261
Conc: 0.14 ng/ml

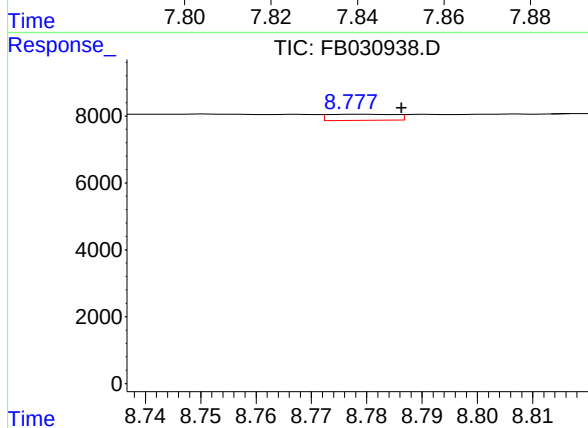

#5 AAA-TFT


R.T.: 8.779 min
Delta R.T.: -0.007 min
Response: 1522
Conc: 0.13 ng/ml

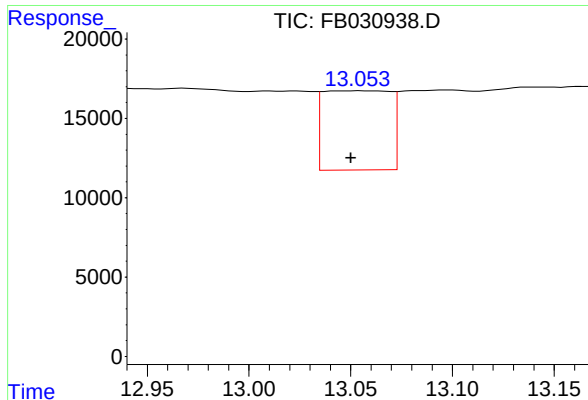

#7 Ethylbenzene


R.T.: 13.057 min
Delta R.T.: 0.006 min
Response: 113673
Conc: 5.43 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-14-5-7.5A

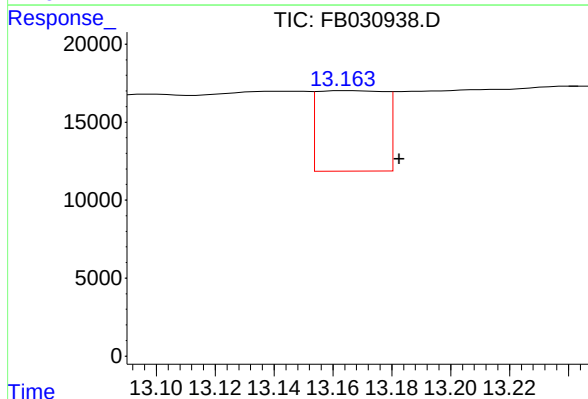


#8 m-Xylene

R.T.: 13.166 min
Delta R.T.: -0.017 min
Response: 81895
Conc: 3.95 ng/ml

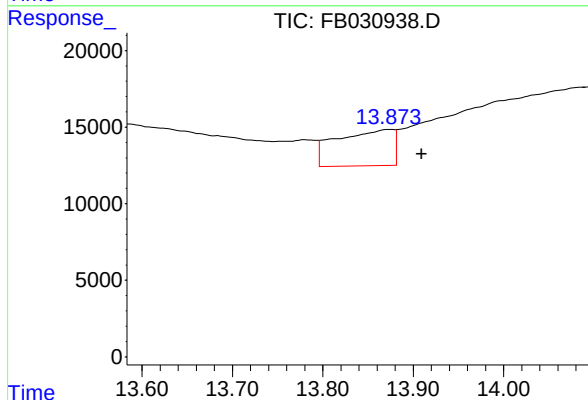

#9 o-Xylene

R.T.: 13.874 min
Delta R.T.: -0.035 min
Response: 103271
Conc: 5.12 ng/ml

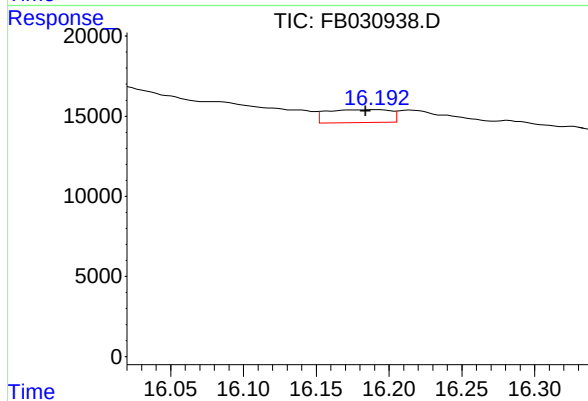

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.009 min
Response: 24474
Conc: 1.23 ng/ml